


Data Path : Z:\HPCHEM1\BNA_M\Data\BM081417\
 Data File : BM011225.D
 Acq On : 14 Aug 2017 12:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

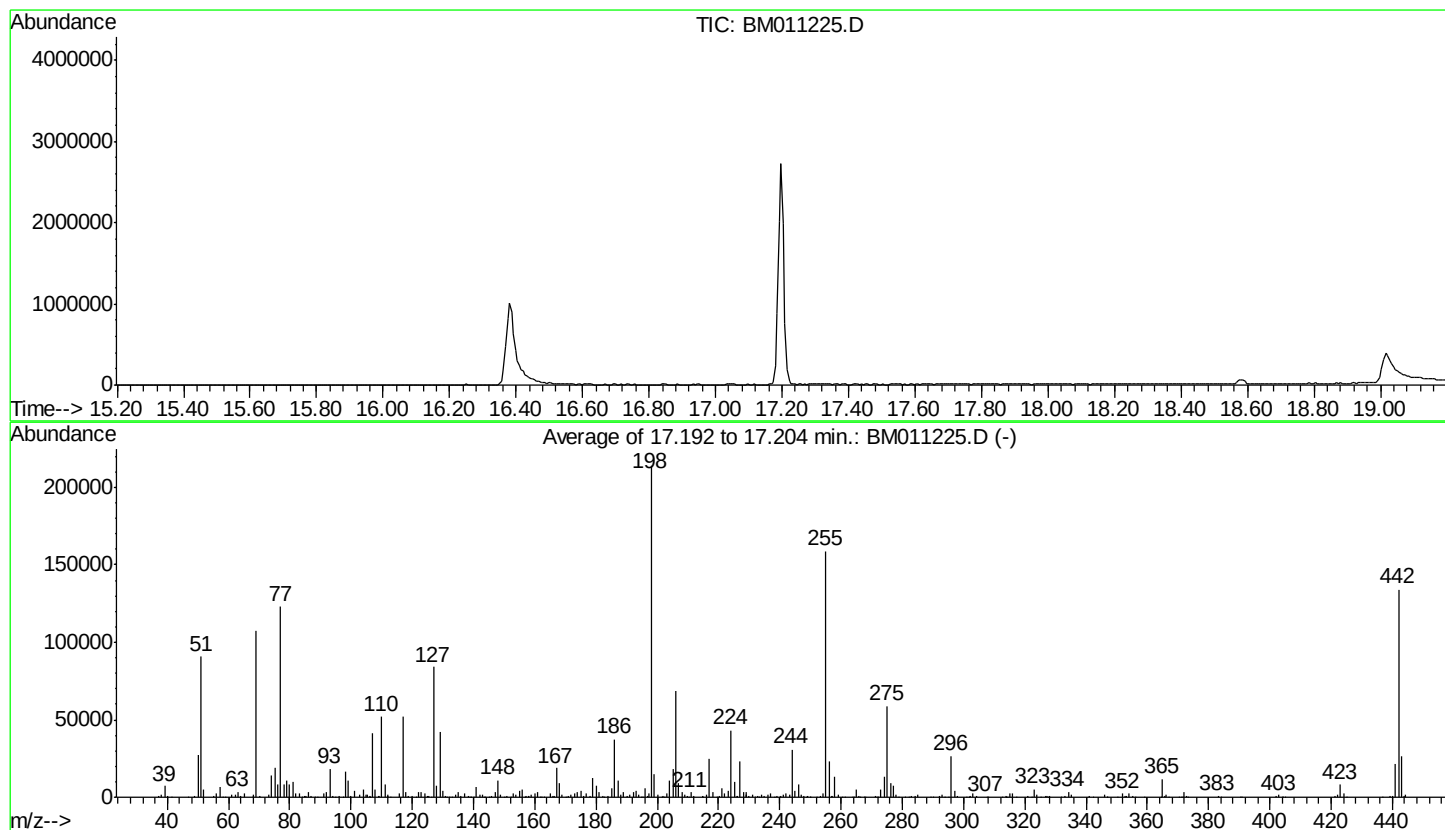

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	90704	PASS
68	69	0.00	2	1.4	1504	PASS
69	198	0.00	100	50.2	107501	PASS
70	69	0.00	2	0.6	606	PASS
127	198	10	80	39.3	84064	PASS
197	198	0.00	2	1.0	2189	PASS
198	198	100	100	100.0	214016	PASS
199	198	5	9	6.8	14523	PASS
275	198	10	60	27.4	58666	PASS
365	198	1	100	5.4	11569	PASS
441	443	0.01	100	82.2	21882	PASS
442	198	50	100	62.7	134114	PASS
443	442	15	24	19.9	26634	PASS