

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036269.D
 Acq On : 14 Aug 2022 14:18
 Operator : CG/JU
 Sample : PB146982BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	27	rVB	60745	71536	1.74%	0.148%
2	3.640	92	94	114	rBV	325984	529961	12.86%	1.096%
3	3.957	145	148	153	rBV	19640	27293	0.66%	0.056%
4	5.140	345	349	354	rVB8	2473	4484	0.11%	0.009%
5	6.992	658	664	680	rBV	781193	1263868	30.66%	2.614%
6	7.145	684	690	703	rVB	702468	1083272	26.28%	2.241%
7	7.339	716	723	734	rBV	818118	1301369	31.57%	2.692%
8	7.804	795	802	815	rBV	868105	1406914	34.13%	2.910%
9	7.916	818	821	826	rVB7	2858	4332	0.11%	0.009%
10	8.533	918	926	943	rBV	914191	1558451	37.81%	3.223%
11	8.975	994	1001	1015	rBV	735873	1249892	30.32%	2.585%
12	9.698	1117	1124	1135	rBV	581773	989483	24.00%	2.047%
13	10.239	1208	1216	1237	rBV	795409	1521575	36.91%	3.147%
14	10.610	1272	1279	1292	rBV	1266215	2097797	50.89%	4.339%
15	10.763	1297	1305	1324	rBV	445554	918155	22.27%	1.899%
16	12.227	1547	1554	1560	rBV3	11521	26987	0.65%	0.056%
17	13.092	1696	1701	1706	rVB5	3717	5915	0.14%	0.012%
18	13.868	1827	1833	1845	rBV	1564664	2223475	53.94%	4.599%
19	14.145	1873	1880	1898	rBV	1942972	2774356	67.30%	5.738%
20	14.451	1925	1932	1941	rBV	1871291	2667370	64.71%	5.517%
21	14.686	1966	1972	1996	rBV	414899	932130	22.61%	1.928%
22	14.862	2000	2002	2005	rVB4	5895	6760	0.16%	0.014%
23	15.280	2069	2073	2079	rVB4	5261	7669	0.19%	0.016%
24	15.445	2090	2101	2115	rBV	2355377	3462398	83.99%	7.162%
25	15.574	2117	2123	2138	rBV	540627	891721	21.63%	1.844%
26	15.680	2138	2141	2145	rVB4	11852	16226	0.39%	0.034%
27	16.227	2229	2234	2239	rVB8	3433	5934	0.14%	0.012%
28	16.498	2275	2280	2285	rBV8	4738	8036	0.19%	0.017%
29	16.656	2304	2307	2309	rBV4	4059	4235	0.10%	0.009%
30	16.951	2354	2357	2359	rBV4	3822	4481	0.11%	0.009%
31	16.980	2361	2362	2365	rVB3	5090	4181	0.10%	0.009%
32	17.192	2392	2398	2408	rBV	2118324	2942802	71.39%	6.087%
33	17.292	2408	2415	2429	rVV	2667054	3705782	89.90%	7.665%
34	17.703	2479	2485	2486	rBV6	3810	4603	0.11%	0.010%
35	17.727	2486	2489	2492	rVV5	4015	5306	0.13%	0.011%
36	18.174	2560	2565	2570	rVB	5516	9215	0.22%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036269.D
 Acq On : 14 Aug 2022 14:18
 Operator : CG/JU
 Sample : PB146982BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	18.580	2630	2634	2635	rBV4	3142	4283	0.10%	0.009%
38	19.150	2727	2731	2736	rBV4	27811	40627	0.99%	0.084%
39	19.227	2740	2744	2747	rBV2	23667	34779	0.84%	0.072%
40	19.586	2799	2805	2814	rBV	3116313	4114066	99.80%	8.509%
41	20.586	2972	2975	2980	rBV	63302	72311	1.75%	0.150%
42	21.374	3104	3109	3118	rBV	2449133	3130916	75.95%	6.476%
43	23.556	3474	3480	3495	rVB2	2081524	4122251	100.00%	8.526%
44	23.709	3500	3506	3519	rVB2	1551974	3089830	74.95%	6.391%


Sum of corrected areas: 48347027

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036269.D
Acq On : 14 Aug 2022 14:18
Operator : CG/JU
Sample : PB146982BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

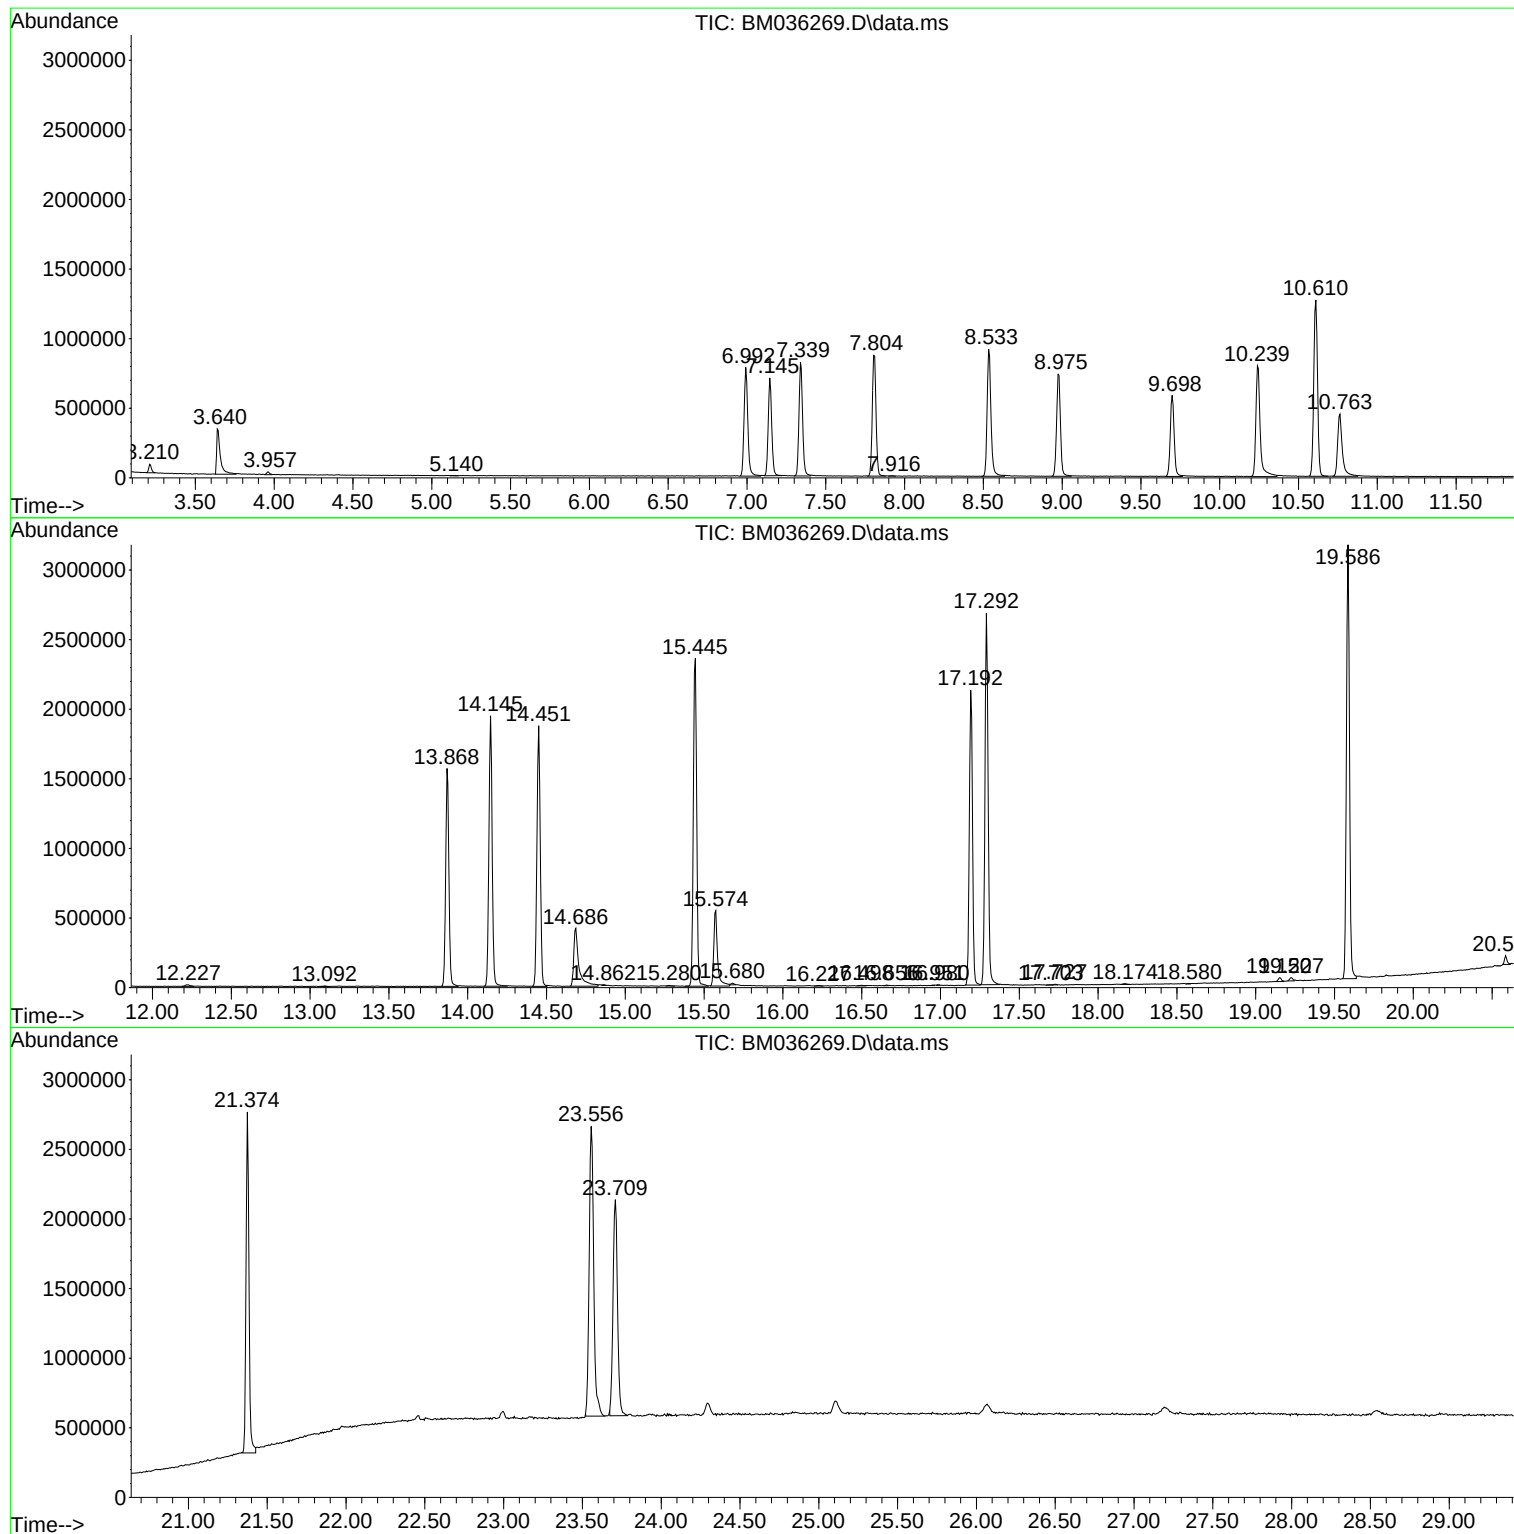

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036269.D
Acq On : 14 Aug 2022 14:18
Operator : CG/JU
Sample : PB146982BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036269.D
Acq On : 14 Aug 2022 14:18
Operator : CG/JU
Sample : PB146982BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------