

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036271.D
 Acq On : 14 Aug 2022 15:31
 Operator : CG/JU
 Sample : N4166-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	29	rVB	51827	66596	1.38%	0.136%
2	3.652	93	96	110	rBV	122652	204425	4.24%	0.418%
3	3.869	127	133	139	rVB	22734	33945	0.70%	0.069%
4	3.963	145	149	154	rVB	20379	25930	0.54%	0.053%
5	4.410	220	225	230	rVB	43187	55962	1.16%	0.115%
6	5.022	324	329	332	rVB6	5313	7855	0.16%	0.016%
7	5.081	336	339	345	rVB8	5165	7384	0.15%	0.015%
8	5.781	454	458	468	rVB	32510	52773	1.09%	0.108%
9	6.928	645	653	657	rBV	23618	34254	0.71%	0.070%
10	6.998	659	665	679	rVB	104652	197879	4.10%	0.405%
11	7.145	683	690	701	rBV	695248	1076668	22.32%	2.203%
12	7.340	717	723	734	rBV	536918	894715	18.55%	1.831%
13	7.416	734	736	747	rVB9	8678	16036	0.33%	0.033%
14	7.810	795	803	811	rBV	908439	1451037	30.08%	2.969%
15	8.034	835	841	846	rBV8	2661	6464	0.13%	0.013%
16	8.539	920	927	940	rBV	372165	662011	13.73%	1.355%
17	8.975	994	1001	1016	rBV	765075	1294624	26.84%	2.649%
18	9.369	1062	1068	1074	rVB	21507	35037	0.73%	0.072%
19	9.698	1116	1124	1137	rBV	575705	963392	19.97%	1.972%
20	10.239	1209	1216	1239	rBV	735916	1367310	28.35%	2.798%
21	10.610	1270	1279	1290	rBV	1284323	2145488	44.48%	4.391%
22	10.757	1296	1304	1324	rBV	784635	1553439	32.21%	3.179%
23	11.869	1485	1493	1499	rVB	16624	27393	0.57%	0.056%
24	12.222	1546	1553	1563	rBV2	12744	26541	0.55%	0.054%
25	13.869	1827	1833	1852	rBV	1746922	2529564	52.45%	5.177%
26	14.145	1873	1880	1893	rBV	2208047	3118049	64.65%	6.381%
27	14.451	1925	1932	1947	rBV	1934731	2707623	56.14%	5.541%
28	14.710	1970	1976	1986	rBV3	28330	88771	1.84%	0.182%
29	15.286	2072	2074	2079	rVB5	4519	4834	0.10%	0.010%
30	15.445	2091	2101	2117	rBV	2808170	3986818	82.66%	8.159%
31	15.574	2117	2123	2138	rVV	572173	910633	18.88%	1.864%
32	15.686	2138	2142	2150	rVB3	17252	33241	0.69%	0.068%
33	16.186	2223	2227	2230	rVB6	4759	6757	0.14%	0.014%
34	16.339	2251	2253	2259	rVB6	3869	5206	0.11%	0.011%
35	16.662	2303	2308	2313	rBV3	12820	16859	0.35%	0.035%
36	16.957	2355	2358	2359	rBV3	4390	4913	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036271.D
 Acq On : 14 Aug 2022 15:31
 Operator : CG/JU
 Sample : N4166-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGBZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	17.110	2378	2384	2385	rBV6	3630	5255	0.11%	0.011%
38	17.192	2392	2398	2409	rBV	2126771	2968726	61.55%	6.075%
39	17.292	2409	2415	2430	rVV	3153351	4301240	89.18%	8.802%
40	17.733	2487	2490	2492	rVB2	11751	12115	0.25%	0.025%
41	18.098	2549	2552	2559	rBV9	9272	17679	0.37%	0.036%
42	18.168	2561	2564	2568	rVV3	6107	7990	0.17%	0.016%
43	18.674	2648	2650	2655	rVB3	11943	11344	0.24%	0.023%
44	19.151	2727	2731	2735	rBV2	34158	44669	0.93%	0.091%
45	19.227	2740	2744	2749	rVB	31381	47179	0.98%	0.097%
46	19.521	2791	2794	2798	rVB5	11183	14532	0.30%	0.030%
47	19.586	2799	2805	2823	rVV	3619993	4823246	100.00%	9.871%
48	20.586	2972	2975	2980	rBV2	59569	68996	1.43%	0.141%
49	21.374	3104	3109	3120	rBV	2412093	3123625	64.76%	6.392%
50	23.556	3474	3480	3494	rVB2	2467433	4782673	99.16%	9.788%
51	23.709	3500	3506	3517	rVB2	1584366	3015116	62.51%	6.170%




Sum of corrected areas: 48864811

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036271.D
Acq On : 14 Aug 2022 15:31
Operator : CG/JU
Sample : N4166-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

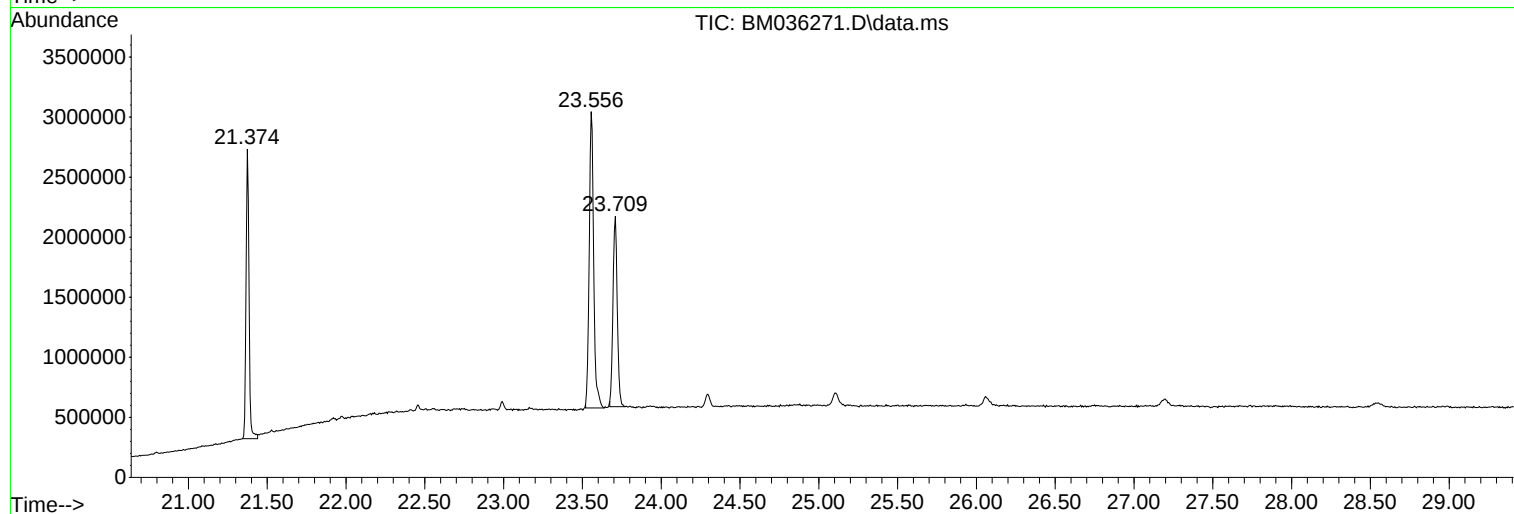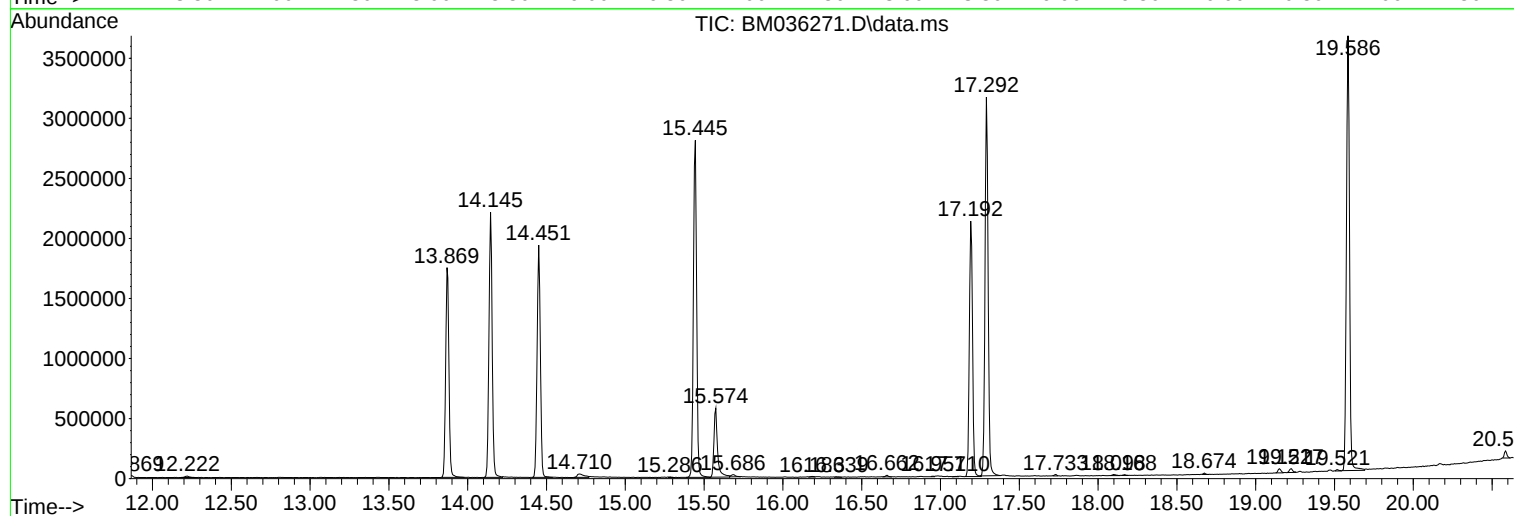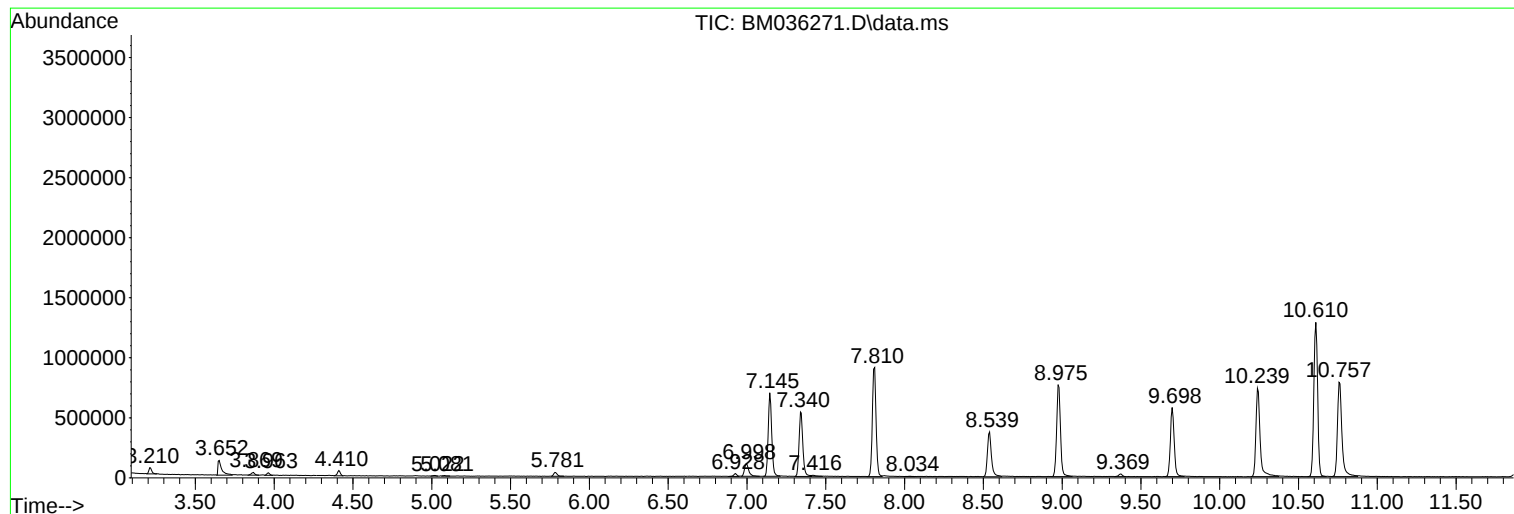

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036271.D
Acq On : 14 Aug 2022 15:31
Operator : CG/JU
Sample : N4166-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036271.D
Acq On : 14 Aug 2022 15:31
Operator : CG/JU
Sample : N4166-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGBZ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------