

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036274.D
 Acq On : 14 Aug 2022 17:19
 Operator : CG/JU
 Sample : N4166-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGC15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	27	rVB	54506	65871	1.45%	0.147%
2	3.652	93	96	109	rBV	102183	167945	3.70%	0.374%
3	3.869	128	133	139	rVB	24126	34666	0.76%	0.077%
4	3.963	145	149	152	rBV	16801	19331	0.43%	0.043%
5	4.410	220	225	233	rVB	43489	59554	1.31%	0.133%
6	4.916	303	311	319	rBV	43506	75227	1.66%	0.168%
7	5.016	325	328	331	rVB6	7453	7486	0.16%	0.017%
8	6.928	648	653	659	rBV	20905	26703	0.59%	0.059%
9	6.992	659	664	677	rBV	133702	237920	5.24%	0.530%
10	7.145	684	690	705	rBV	739765	1128776	24.85%	2.514%
11	7.339	716	723	734	rBV	621691	1020769	22.47%	2.273%
12	7.416	734	736	744	rVB7	8820	14511	0.32%	0.032%
13	7.810	795	803	813	rBV	796367	1292507	28.45%	2.878%
14	8.539	919	927	941	rBV	426173	754477	16.61%	1.680%
15	8.975	994	1001	1016	rBV	794997	1312077	28.89%	2.922%
16	9.369	1063	1068	1076	rVB	20472	31297	0.69%	0.070%
17	9.698	1115	1124	1133	rBV	591897	970018	21.36%	2.160%
18	10.239	1209	1216	1238	rBV	745828	1402140	30.87%	3.123%
19	10.610	1272	1279	1288	rBV	1149706	1878071	41.35%	4.183%
20	10.763	1297	1305	1322	rBV	590651	1163004	25.60%	2.590%
21	11.863	1487	1492	1496	rBV	13357	19398	0.43%	0.043%
22	12.216	1548	1552	1561	rBV2	11734	26028	0.57%	0.058%
23	13.351	1743	1745	1749	rVB5	3677	4561	0.10%	0.010%
24	13.868	1827	1833	1847	rBV	1617717	2288258	50.38%	5.096%
25	14.145	1872	1880	1893	rBV	1967973	2848717	62.72%	6.344%
26	14.451	1925	1932	1944	rBV	1584434	2301467	50.67%	5.125%
27	14.704	1969	1975	1990	rBV3	39549	130032	2.86%	0.290%
28	15.445	2092	2101	2113	rBV	2535479	3636660	80.06%	8.099%
29	15.574	2117	2123	2137	rVV	573261	918684	20.23%	2.046%
30	15.680	2137	2141	2149	rVB4	15322	33847	0.75%	0.075%
31	16.657	2302	2307	2312	rBV3	10162	15259	0.34%	0.034%
32	16.968	2354	2360	2361	rBV6	4121	6714	0.15%	0.015%
33	16.980	2361	2362	2370	rVB5	5719	6497	0.14%	0.014%
34	17.192	2392	2398	2408	rBV	1847813	2479550	54.59%	5.522%
35	17.292	2408	2415	2429	rVV	3044157	4125040	90.81%	9.187%
36	17.486	2447	2448	2460	rVB9	5165	6724	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036274.D
 Acq On : 14 Aug 2022 17:19
 Operator : CG/JU
 Sample : N4166-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGC15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	17.727	2485	2489	2494	rBV3	8696	14825	0.33%	0.033%
38	18.098	2548	2552	2559	rBV9	7342	13701	0.30%	0.031%
39	18.168	2561	2564	2567	rVB4	4270	6030	0.13%	0.013%
40	18.674	2647	2650	2653	rVB4	6218	7276	0.16%	0.016%
41	19.150	2727	2731	2735	rBV3	31718	43589	0.96%	0.097%
42	19.227	2739	2744	2748	rBV	32095	46643	1.03%	0.104%
43	19.586	2799	2805	2816	rBV	3504171	4521076	99.53%	10.069%
44	20.586	2972	2975	2980	rBV2	53165	57944	1.28%	0.129%
45	21.374	3104	3109	3117	rBV	1968042	2543430	55.99%	5.664%
46	23.556	3474	3480	3496	rVB2	2394766	4542300	100.00%	10.116%
47	23.709	3500	3506	3516	rVB2	1337766	2595761	57.15%	5.781%




Sum of corrected areas: 44902361

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036274.D
Acq On : 14 Aug 2022 17:19
Operator : CG/JU
Sample : N4166-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

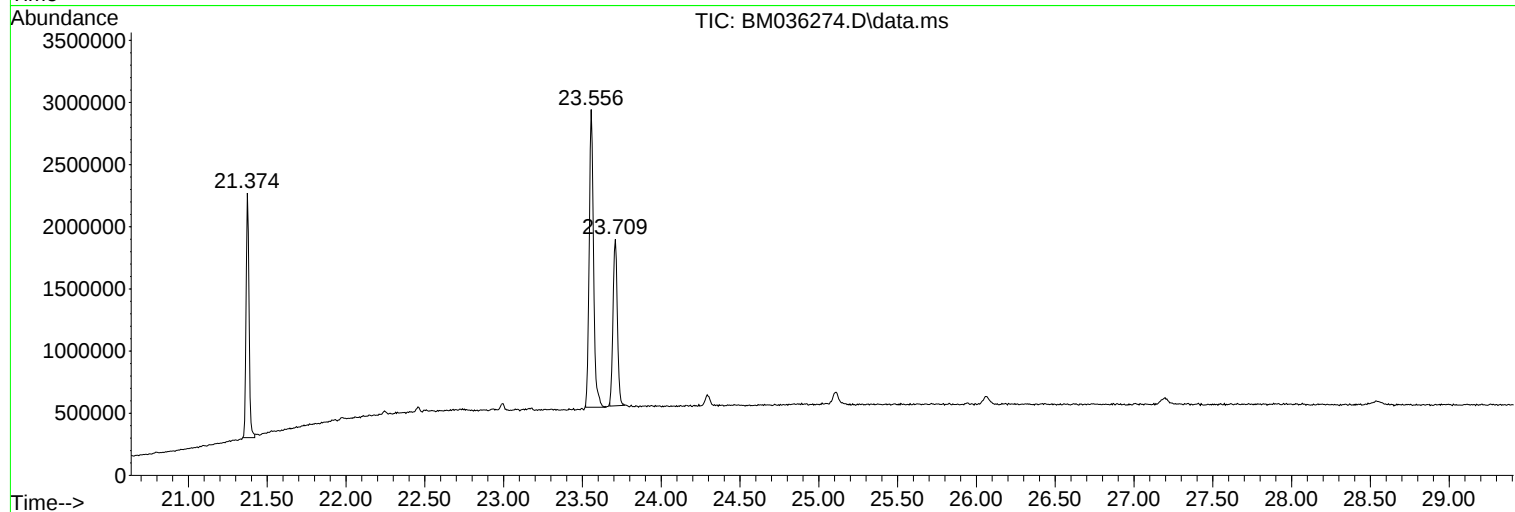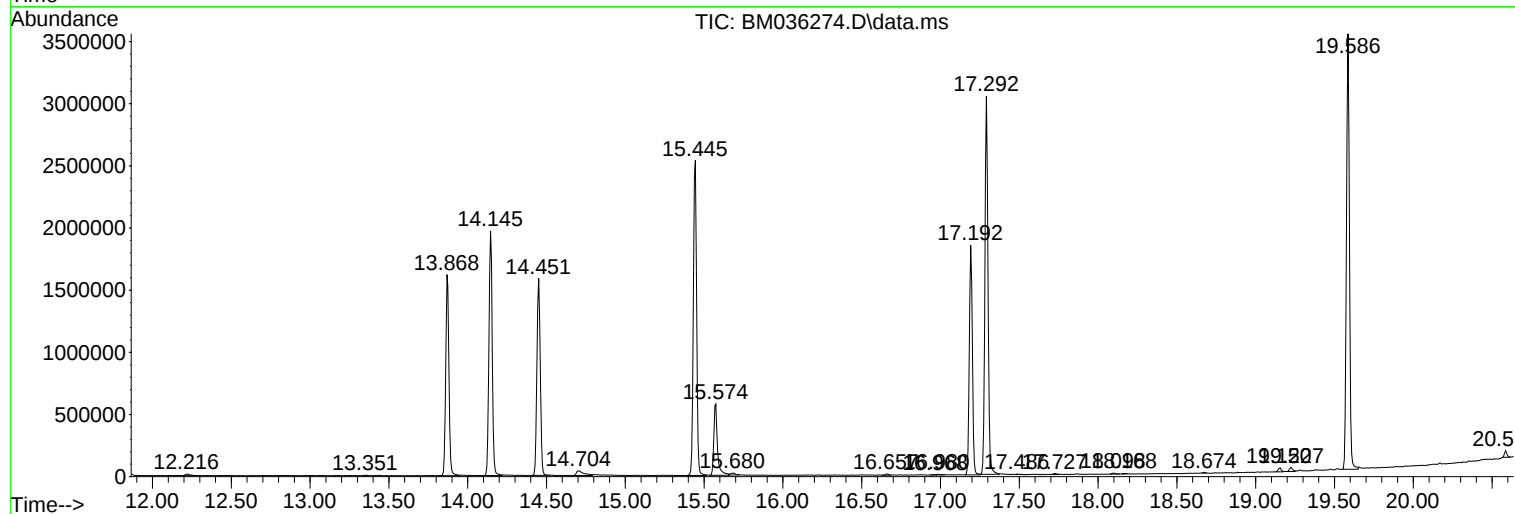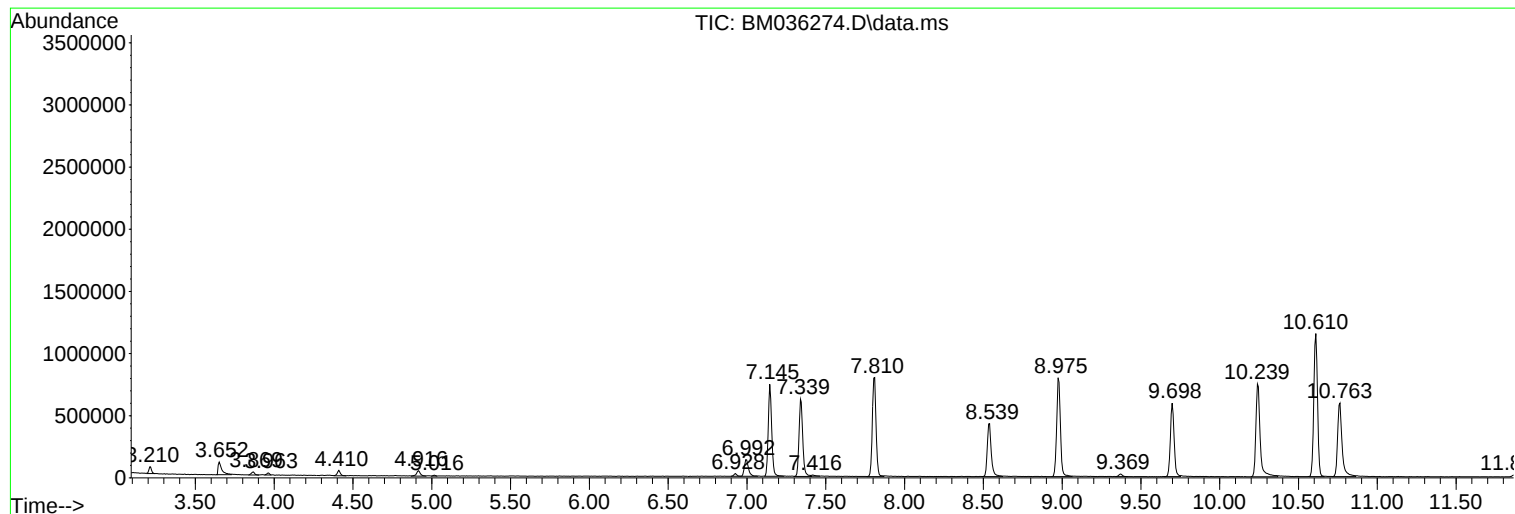

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036274.D
Acq On : 14 Aug 2022 17:19
Operator : CG/JU
Sample : N4166-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036274.D
Acq On : 14 Aug 2022 17:19
Operator : CG/JU
Sample : N4166-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------