

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
 Data File : BM036275.D
 Acq On : 14 Aug 2022 17:56
 Operator : CG/JU
 Sample : N4166-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGC02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	32	rVB	59759	83503	1.53%	0.181%
2	3.651	94	96	110	rBV	108468	184822	3.39%	0.401%
3	3.869	128	133	137	rVB	23635	34486	0.63%	0.075%
4	3.963	145	149	155	rVB	19432	30384	0.56%	0.066%
5	4.410	221	225	232	rVB	45544	59222	1.09%	0.128%
6	4.916	307	311	318	rVB	34791	49179	0.90%	0.107%
7	5.016	325	328	332	rVB6	6141	7056	0.13%	0.015%
8	6.440	566	570	576	rBV7	2592	5790	0.11%	0.013%
9	6.928	648	653	658	rVB	22658	30866	0.57%	0.067%
10	6.998	658	665	675	rBV	122998	225075	4.13%	0.488%
11	7.145	684	690	703	rBV	727112	1126011	20.65%	2.441%
12	7.339	716	723	734	rBV	595044	984894	18.06%	2.135%
13	7.422	734	737	741	rVB5	7039	10479	0.19%	0.023%
14	7.804	796	802	812	rBV	773608	1242095	22.78%	2.692%
15	8.081	845	849	855	rVB10	2461	6383	0.12%	0.014%
16	8.539	920	927	942	rBV	383409	696885	12.78%	1.511%
17	8.975	994	1001	1016	rBV	770868	1298205	23.81%	2.814%
18	9.369	1062	1068	1075	rVB	20810	34513	0.63%	0.075%
19	9.698	1117	1124	1135	rBV	552530	947356	17.37%	2.054%
20	10.239	1209	1216	1234	rBV	730952	1359504	24.93%	2.947%
21	10.610	1272	1279	1293	rBV	1074323	1766531	32.40%	3.829%
22	10.763	1297	1305	1320	rBV	652413	1280438	23.48%	2.776%
23	11.869	1487	1493	1497	rVB	11944	19426	0.36%	0.042%
24	12.221	1544	1553	1560	rBV3	10567	26531	0.49%	0.058%
25	13.868	1827	1833	1847	rBV	1581553	2187547	40.12%	4.742%
26	14.145	1873	1880	1894	rBV	1973047	2799731	51.35%	6.069%
27	14.451	1925	1932	1948	rBV	1522587	2164455	39.70%	4.692%
28	14.704	1969	1975	1989	rBV3	32870	115752	2.12%	0.251%
29	15.445	2089	2101	2117	rBV	2464240	3558002	65.25%	7.713%
30	15.574	2117	2123	2139	rVV	551630	911150	16.71%	1.975%
31	15.686	2139	2142	2147	rVB3	13885	23869	0.44%	0.052%
32	16.509	2275	2282	2284	rBV8	3138	5501	0.10%	0.012%
33	16.662	2304	2308	2312	rVB2	9371	10483	0.19%	0.023%
34	17.192	2392	2398	2408	rBV	1816597	2419264	44.37%	5.244%
35	17.292	2408	2415	2432	rVV	3006666	4125073	75.65%	8.942%
36	17.727	2486	2489	2496	rVB2	7740	11224	0.21%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036275.D
Acq On : 14 Aug 2022 17:56
Operator : CG/JU
Sample : N4166-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC02

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	18.098	2547	2552	2560	rBV2	10985	25148	0.46%	0.055%
38	18.674	2647	2650	2653	rVB3	8230	9457	0.17%	0.020%
39	19.150	2727	2731	2736	rBV	32751	47447	0.87%	0.103%
40	19.227	2740	2744	2751	rVV	28752	42887	0.79%	0.093%
41	19.586	2799	2805	2814	rBV	3695183	4724163	86.64%	10.240%
42	20.586	2972	2975	2979	rVB	48406	54356	1.00%	0.118%
43	21.374	3104	3109	3120	rBV	2240806	2854332	52.35%	6.187%
44	23.556	3473	3480	3495	rBV2	2768725	5452532	100.00%	11.819%
45	23.709	3499	3506	3518	rVB2	1523521	3080645	56.50%	6.678%




Sum of corrected areas: 46132652

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036275.D
Acq On : 14 Aug 2022 17:56
Operator : CG/JU
Sample : N4166-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

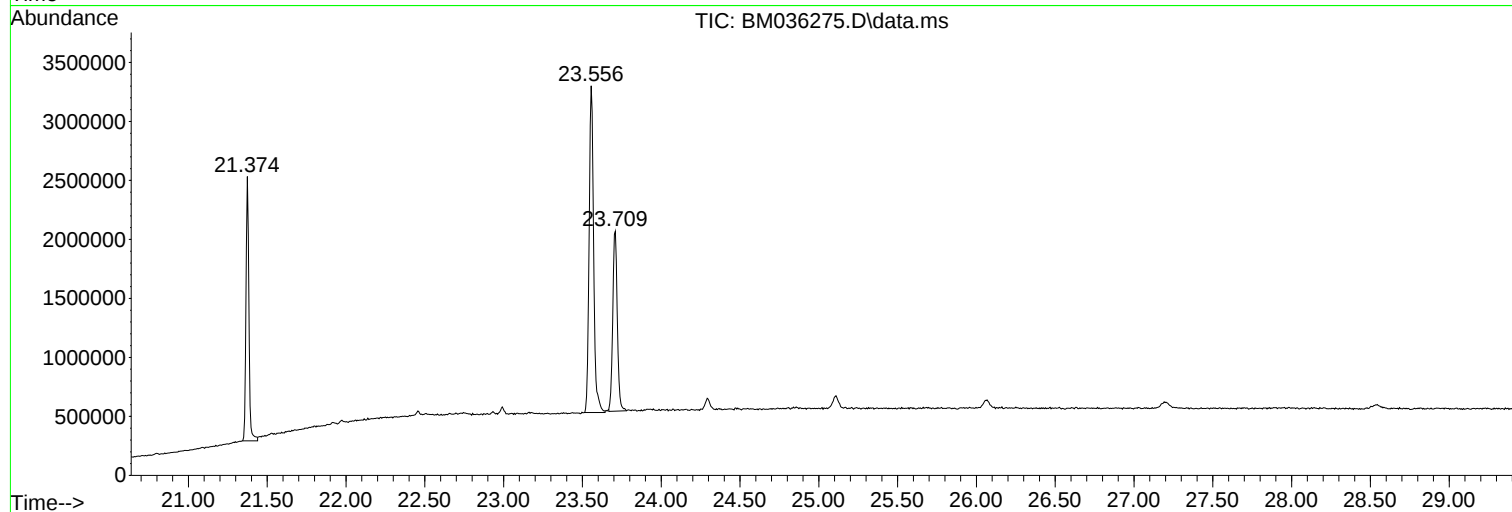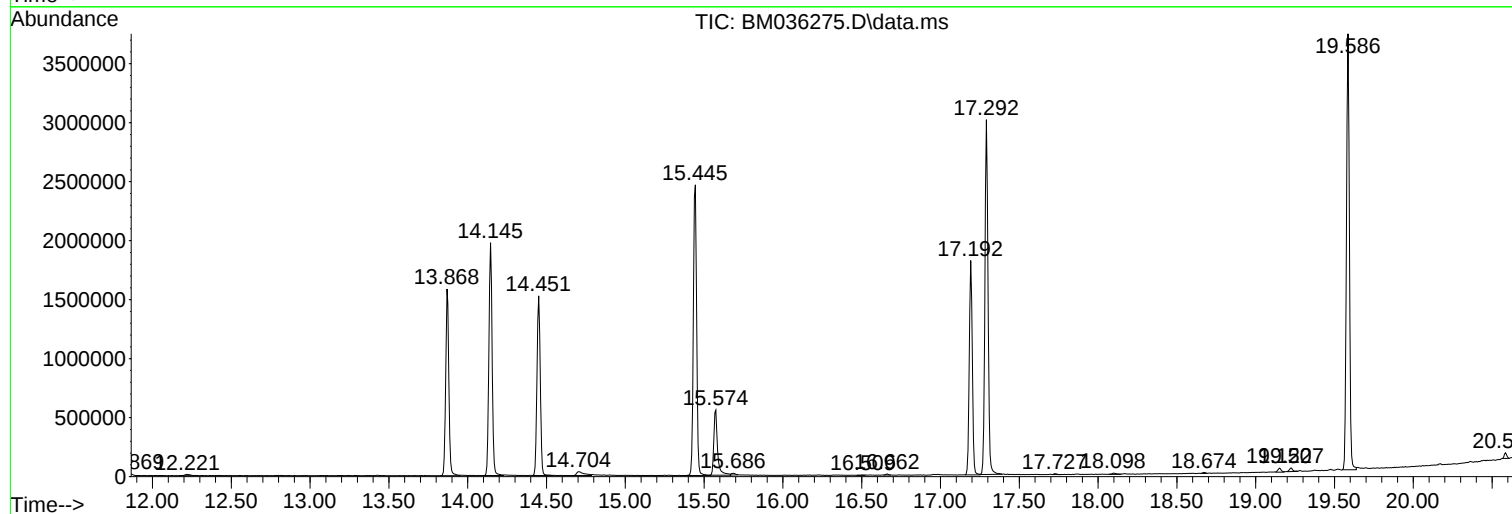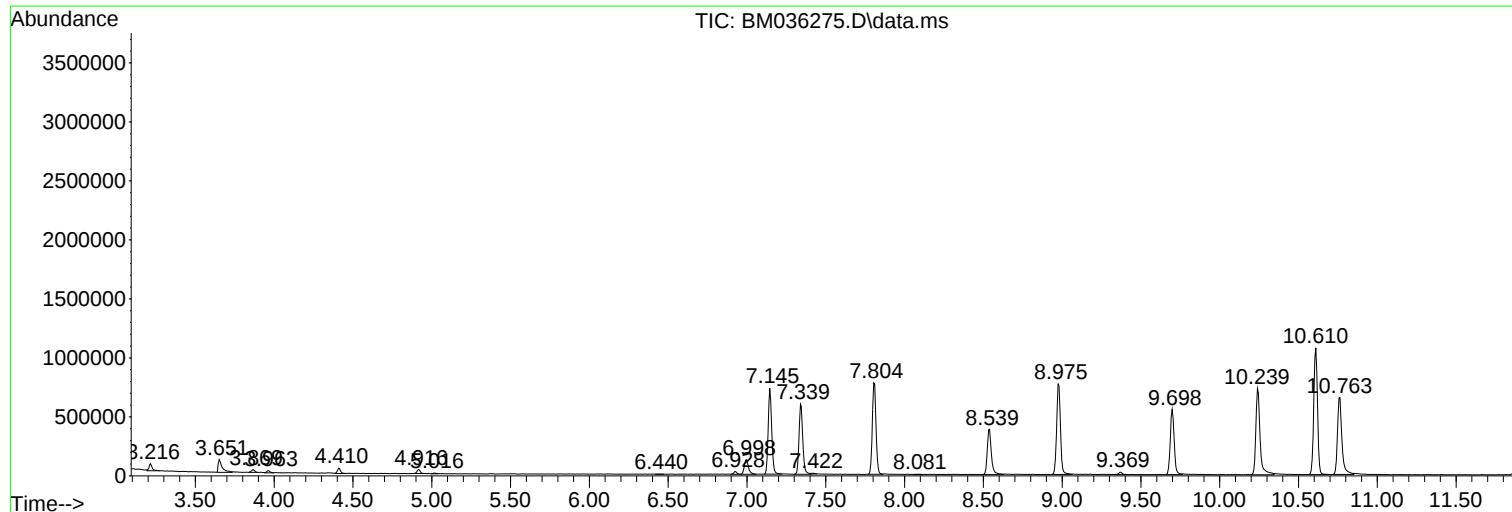

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036275.D
Acq On : 14 Aug 2022 17:56
Operator : CG/JU
Sample : N4166-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081422\
Data File : BM036275.D
Acq On : 14 Aug 2022 17:56
Operator : CG/JU
Sample : N4166-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGC02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------