




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
Data File : BM047186.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : PB162262BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Quant Time: Aug 14 12:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 16:46:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024

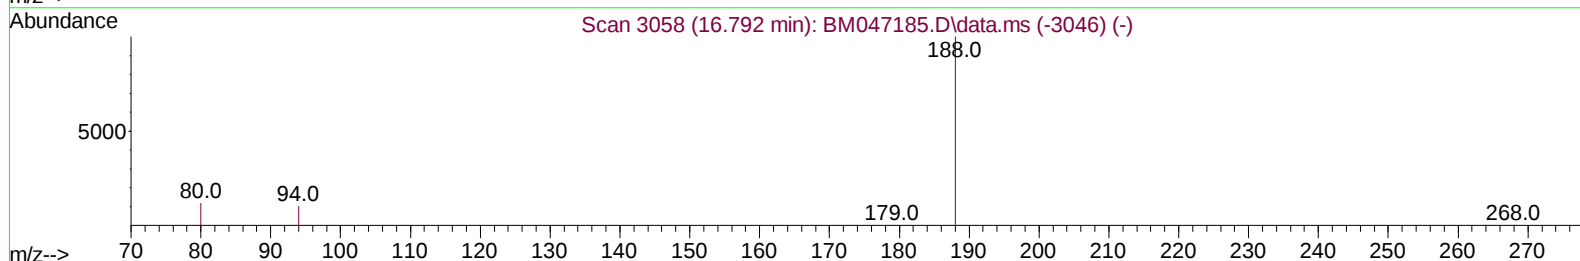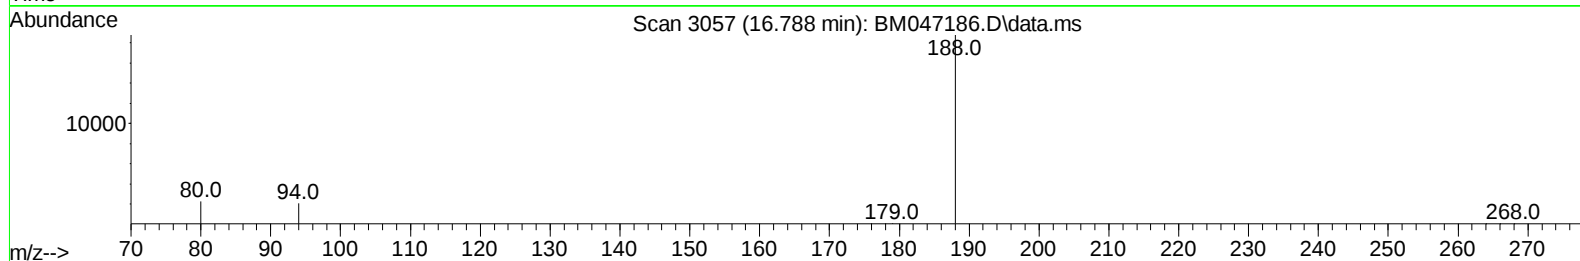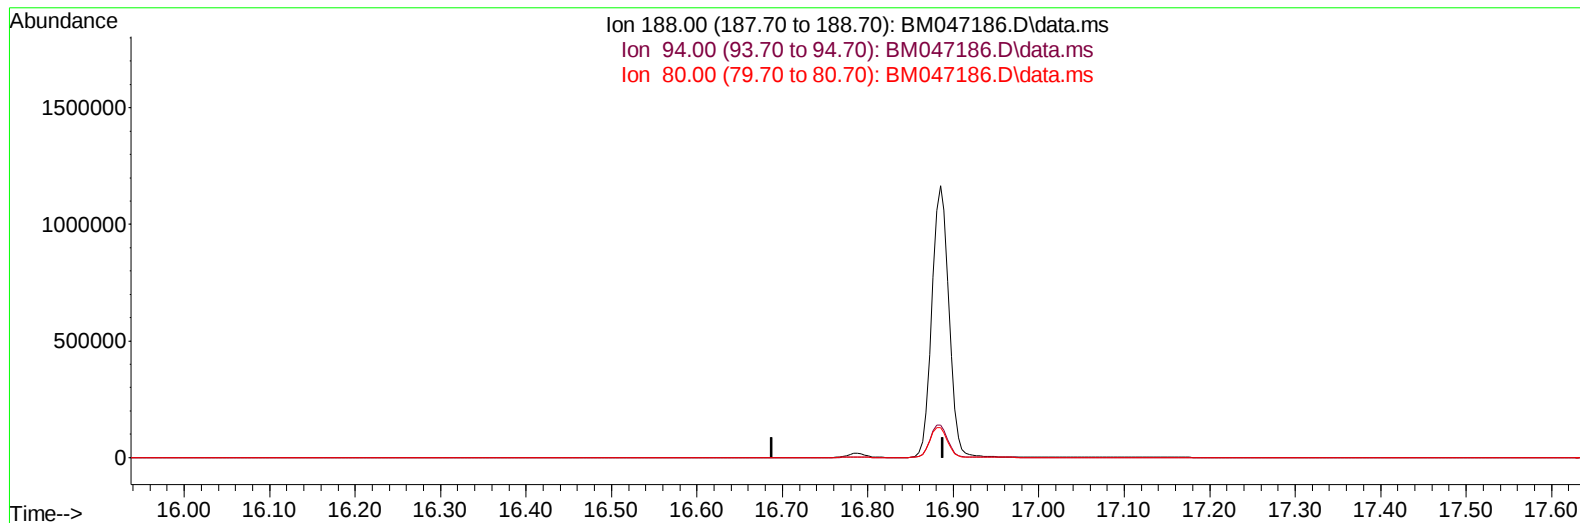

TIC: BM047186.D\data.ms

(13) Phenanthrene-d10 (I)

16.788min (-16.788) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	9.50	0.00#
80.00	10.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
Data File : BM047186.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : PB162262BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Quant Time: Aug 14 12:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 16:46:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024

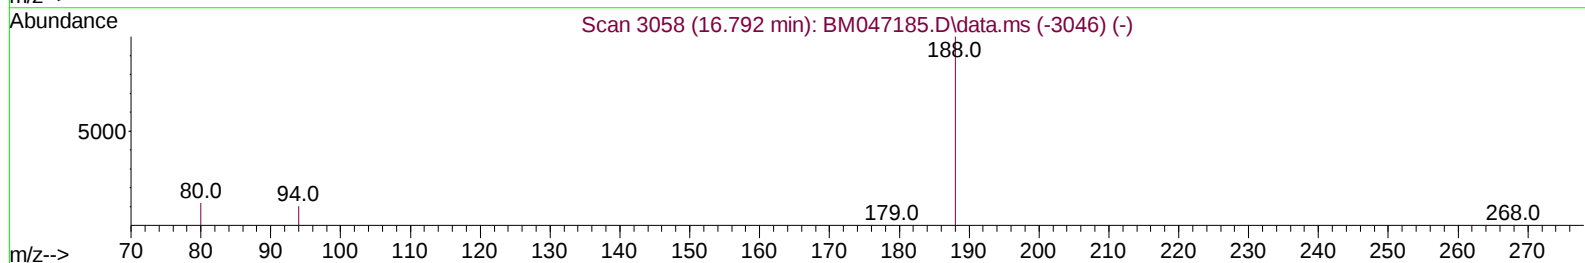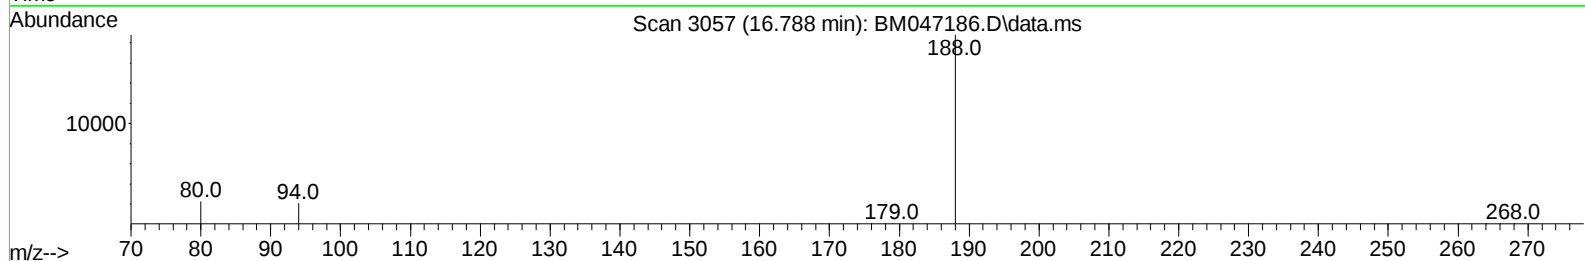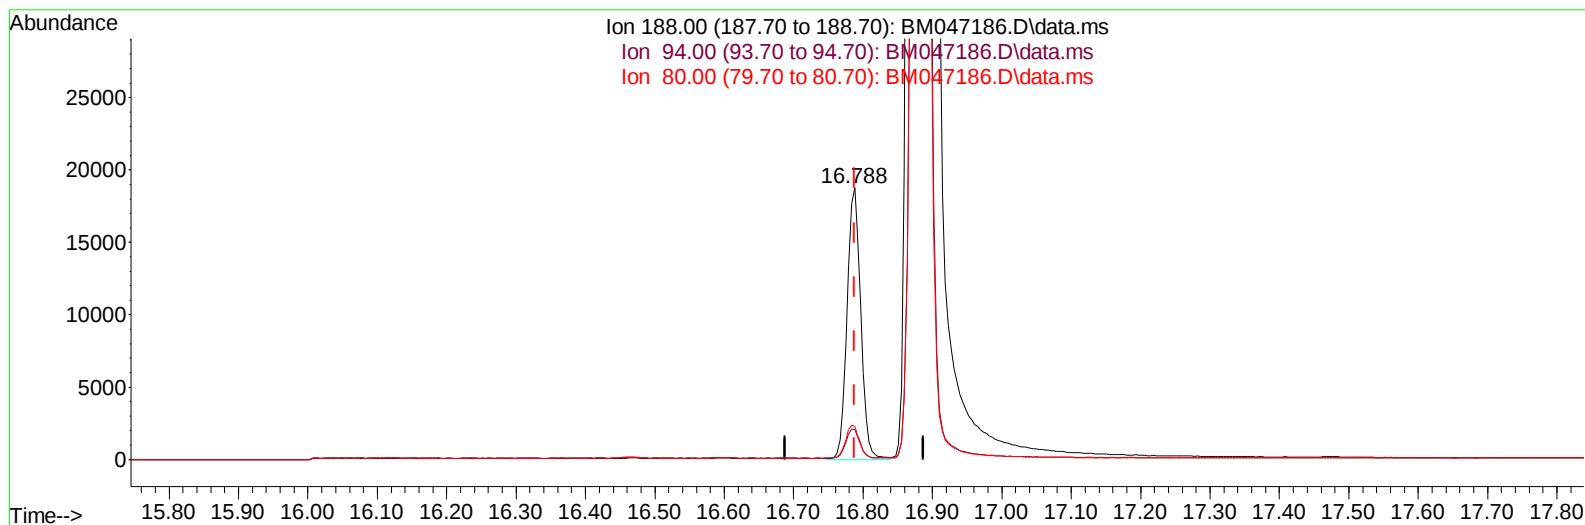

TIC: BM047186.D\data.ms

(13) Phenanthrene-d10 (I)

16.788min (+ 0.000) 0.40 ng/u1 m

response 25637

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.50	10.93
80.00	10.50	12.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
Data File : BM047186.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : PB162262BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024

Quant Time: Aug 14 12:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 16:46:53 2024
Response via : Initial Calibration

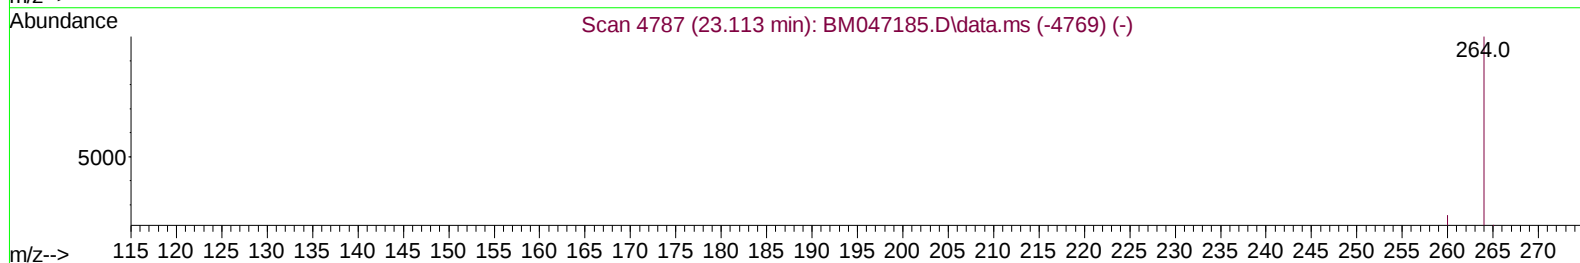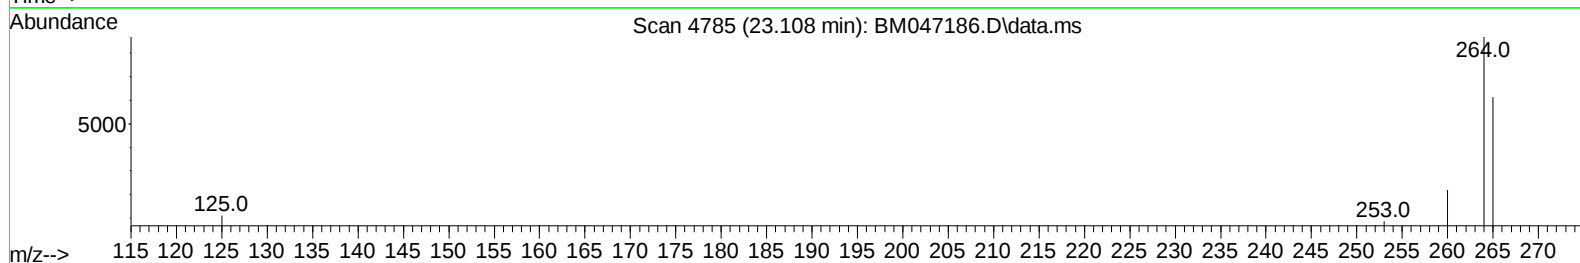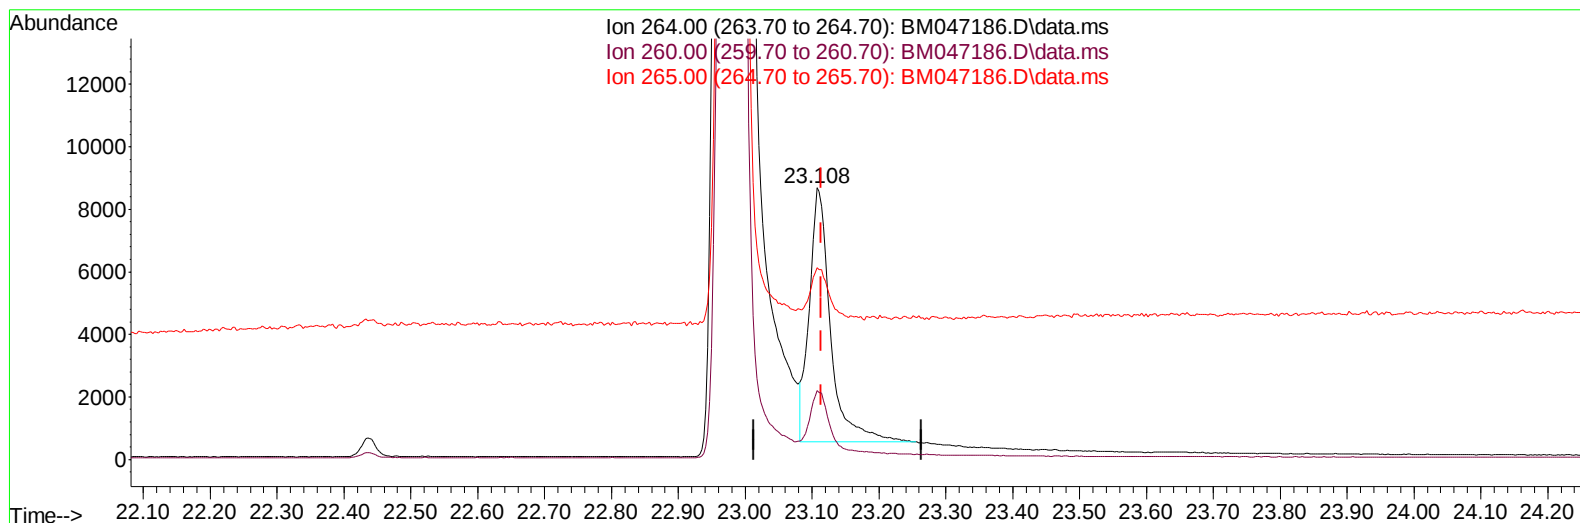

TIC: BM047186.D\data.ms

(23) Perylene-d12 (I)

23.108min (-0.006) 0.40 ng/u1

response 17789

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.34
265.00	73.20	70.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
Data File : BM047186.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : PB162262BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Quant Time: Aug 14 12:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 16:46:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024

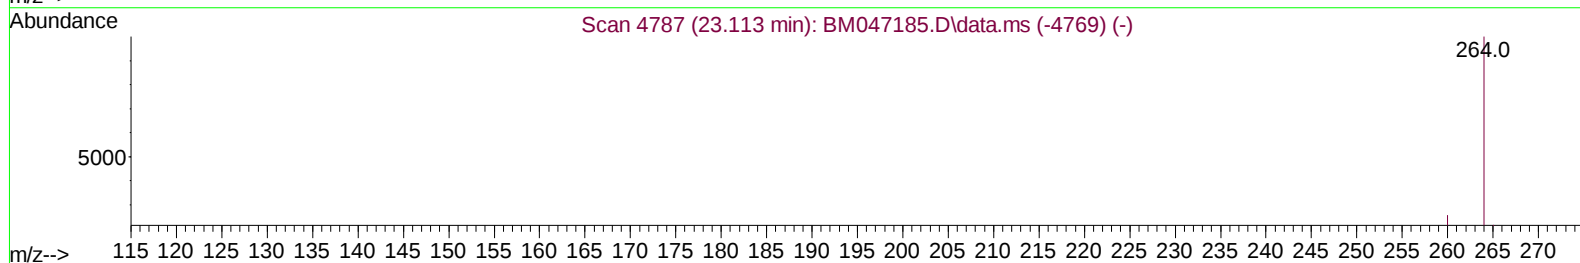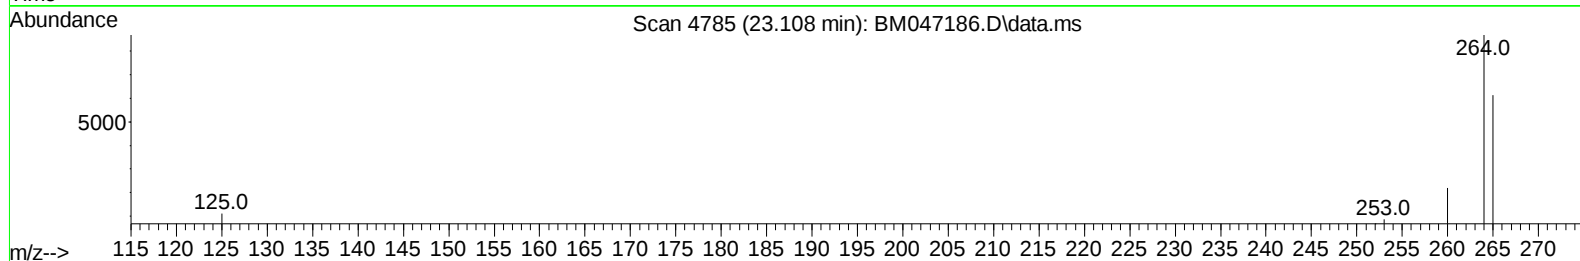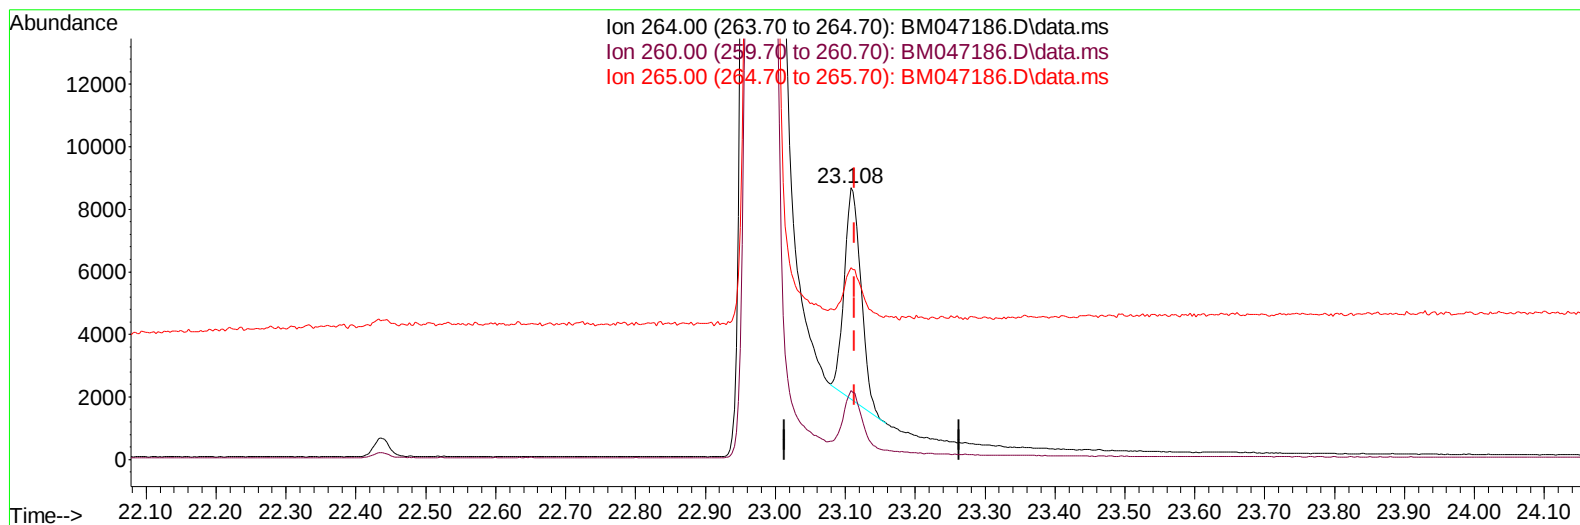

TIC: BM047186.D\data.ms

(23) Perylene-d12 (I)

23.108min (-0.006) 0.40 ng/ul m

response 11197

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.34
265.00	73.20	70.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
 Data File : BM047186.D
 Acq On : 14 Aug 2024 11:33
 Operator : RC/JU
 Sample : PB162262BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK262

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/14/2024
 Supervised By :mohammad ahmed 08/15/2024

Quant Time: Aug 14 12:37:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 13 16:46:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.372	152	6848	0.400	ng/ul	0.00
4) Naphthalene-d8	10.118	136	22760	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.027	164	12156	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.788	188	25637m	0.400	ng/ul	0.00
17) Chrysene-d12	21.015	240	13613	0.400	ng/ul #	0.00
23) Perylene-d12	23.108	264	11197m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.005	96	50385	7.298	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.730	152	9825	0.289	ng/ul	0.00
18) Fluoranthene-d10	18.831	212	15776	0.401	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
Data File : BM047186.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : PB162262BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK262

Manual IntegrationsAPPROVED

Quant Time: Aug 14 12:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 16:46:53 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024

