

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
 Data File : BM047188.D
 Acq On : 14 Aug 2024 12:46
 Operator : RC/JU
 Sample : P3540-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B42

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/14/2024
 Supervised By :mohammad ahmed 08/15/2024

Quant Time: Aug 14 13:45:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 13 16:46:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.372	152	5893	0.400	ng/ul	0.00
4) Naphthalene-d8	10.124	136	17957	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.027	164	8992	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.783	188	19018m	0.400	ng/ul	0.00
17) Chrysene-d12	21.015	240	12436	0.400	ng/ul	0.00
23) Perylene-d12	23.108	264	11348m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.009	96	29963	5.043	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.729	152	9014	0.336	ng/ul	0.00
18) Fluoranthene-d10	18.831	212	16802	0.468	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.039	88	13834	2.084	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081424\
Data File : BM047188.D
Acq On : 14 Aug 2024 12:46
Operator : RC/JU
Sample : P3540-04
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0B42

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024


Quant Time: Aug 14 13:45:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM080724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 16:46:53 2024
Response via : Initial Calibration

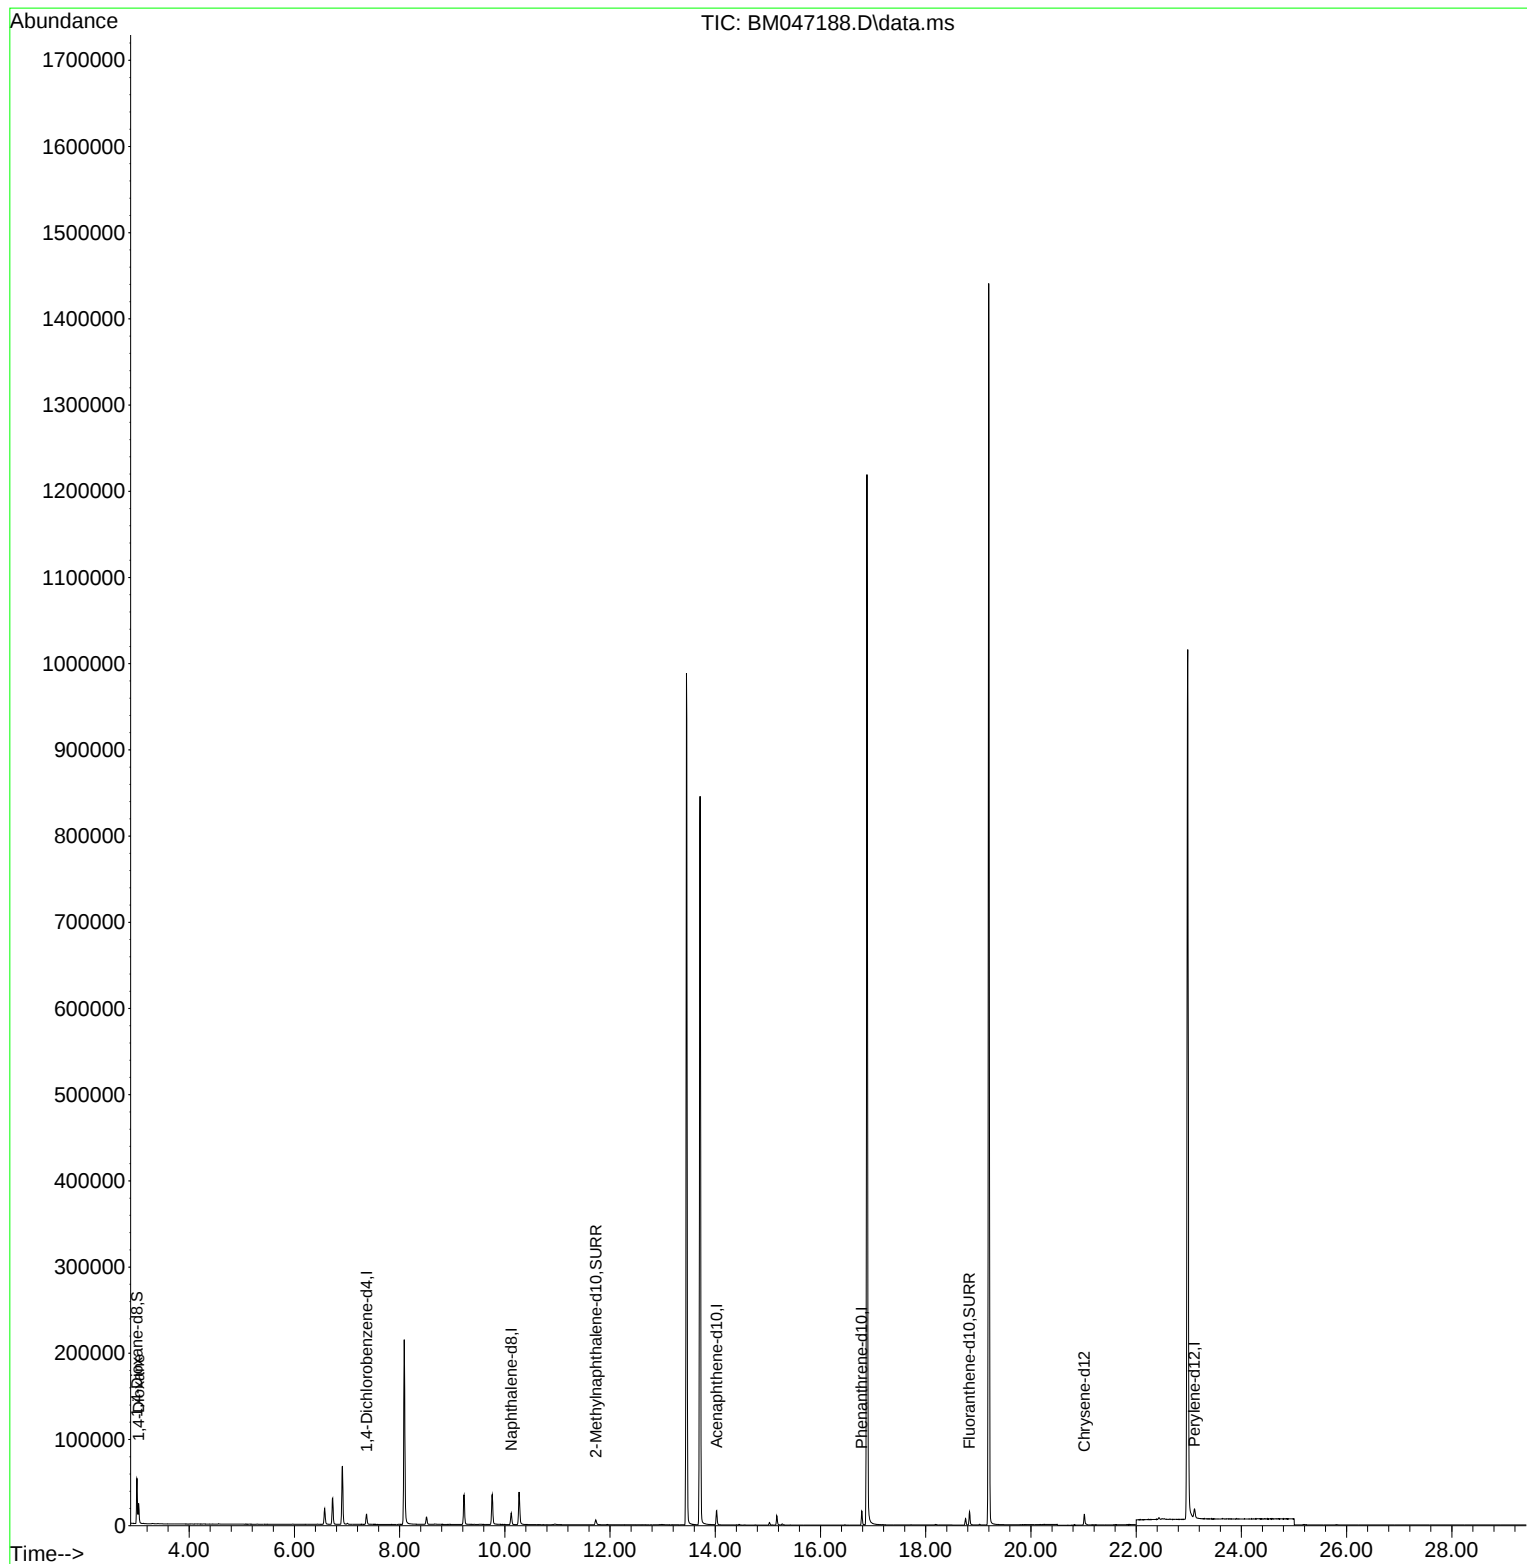

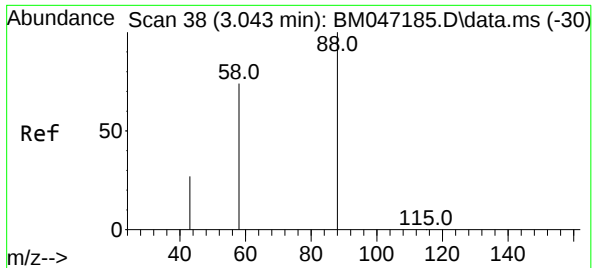

#2
1,4-Dioxane
Concen: 2.084 ng/ul
RT: 3.039 min Scan# 31
Delta R.T. 0.000 min
Lab File: BM047188.D
Acq: 14 Aug 2024 12:46

Instrument :
BNA_M
ClientSampleId :
C0B42

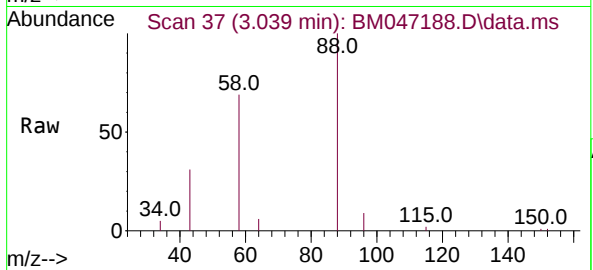

Tgt Ion: 88 Resp: 13834
Ion Ratio Lower Upper
88 100
43 30.9 32.0 48.0
58 69.1 48.1 72.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/14/2024
Supervised By :mohammad ahmed 08/15/2024

