

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM081516\
 Data File : BM007129.D
 Acq On : 15 Aug 2016 22:45
 Operator : UM/SJ
 Sample : H4338-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4V22

Manual Integrations
 APPROVED

umangi
 8/16/2016 7:30:54 PM

Quant Time: Aug 16 12:12:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM081516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 16 01:54:24 2016
 Response via : Initial Calibration

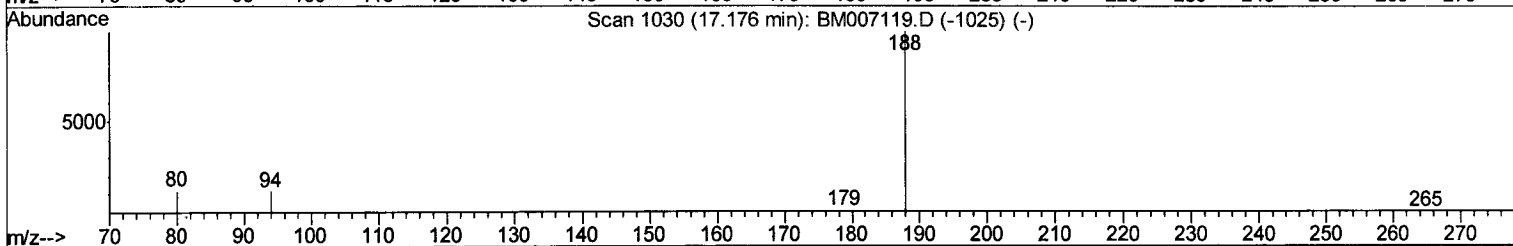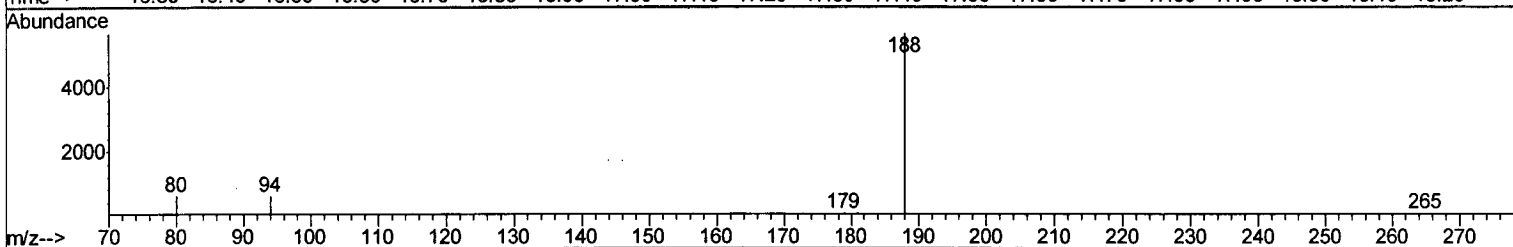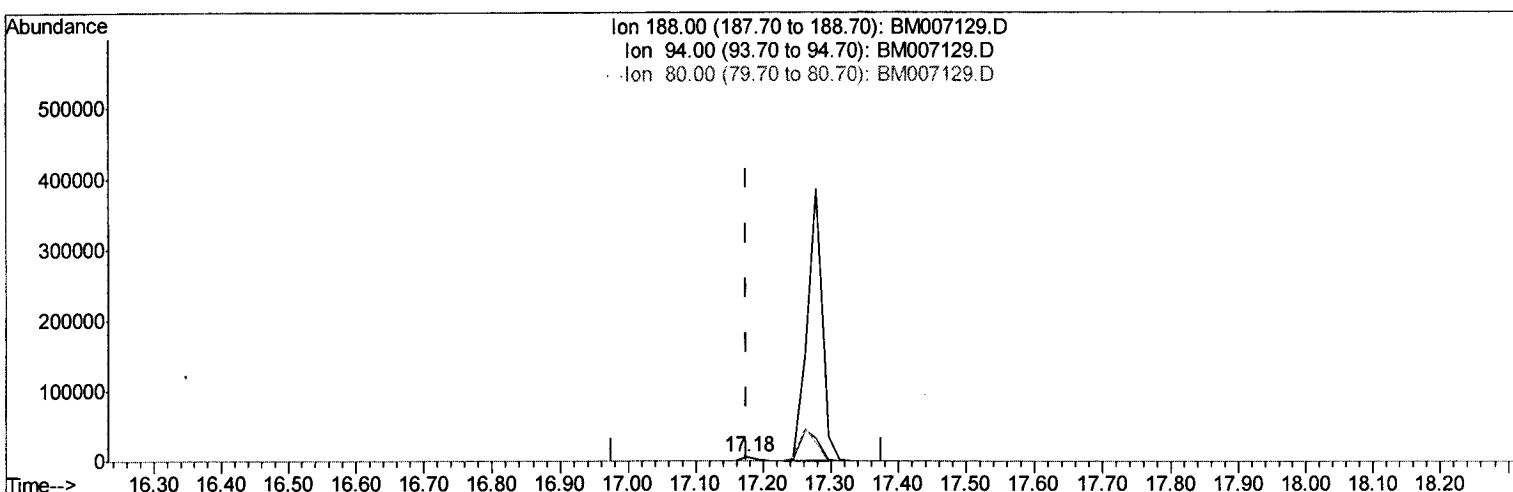

TIC: BM007129.D

(10) Phenanthrene-d10 (I)

17.176min (+0.000) 0.40ng/ul m

response 8233

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	11.01
80.00	11.90	10.93
0.00	0.00	0.00

U.M
08/17/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM081516\
 Data File : BM007129.D
 Acq On : 15 Aug 2016 22:45
 Operator : UM/SJ
 Sample : H4338-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 16 12:12:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM081516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 16 01:54:24 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 A4V22

Manual Integrations
APPROVED

umangi
 8/16/2016 7:30:54 PM

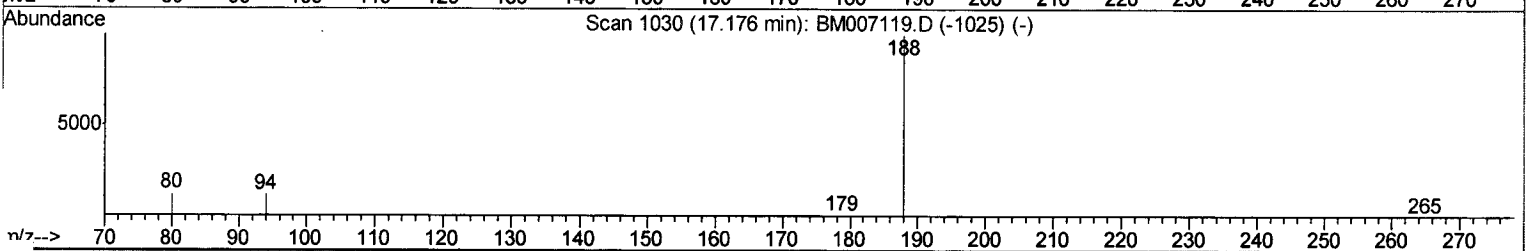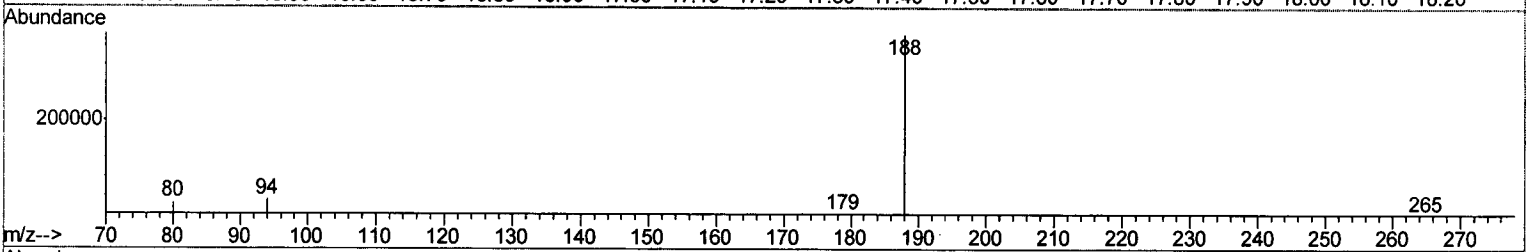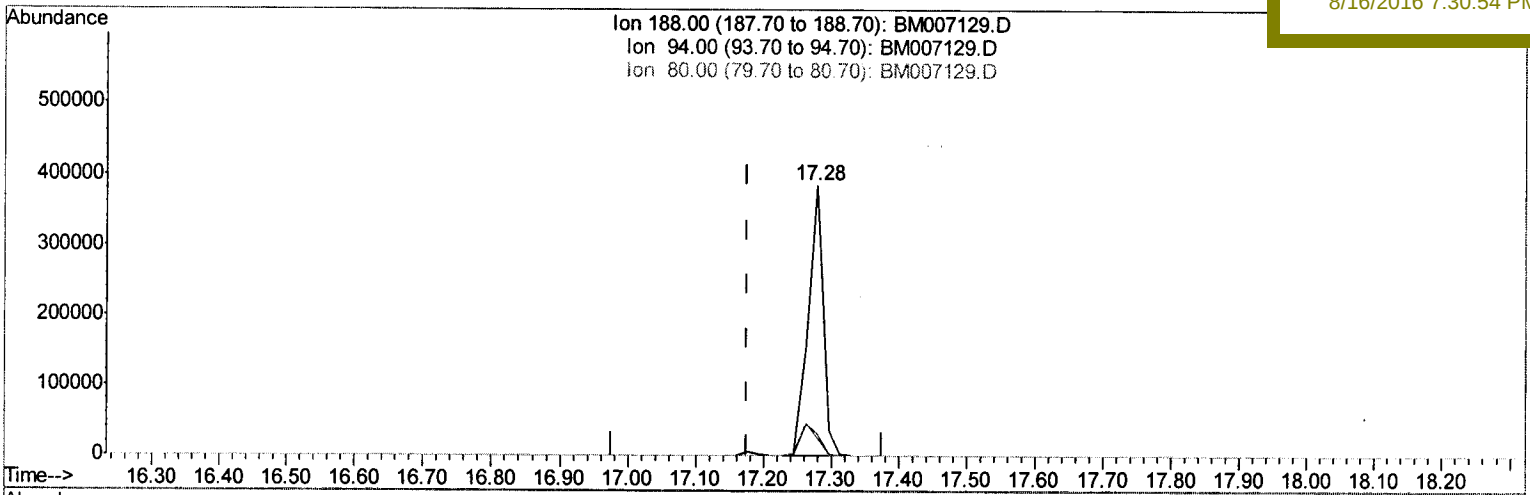

(10) Phenanthrene-d10 (I)
 17.279min (+0.103) 0.40ng/ul
 response 590477

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	8.17#
80.00	11.90	6.30#
0.00	0.00	0.00