




Data Path : Z:\HPCHEM1\BNA M\Data\BM081516\
 Data File : BM007133.D
 Acq On : 16 Aug 2016 01:08
 Operator : UM/SJ
 Sample : PB92717BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 16 03:56:08 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 16 01:54:24 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK17

Manual Integrations
 APPROVED

umangi
 8/16/2016 7:31:02 PM

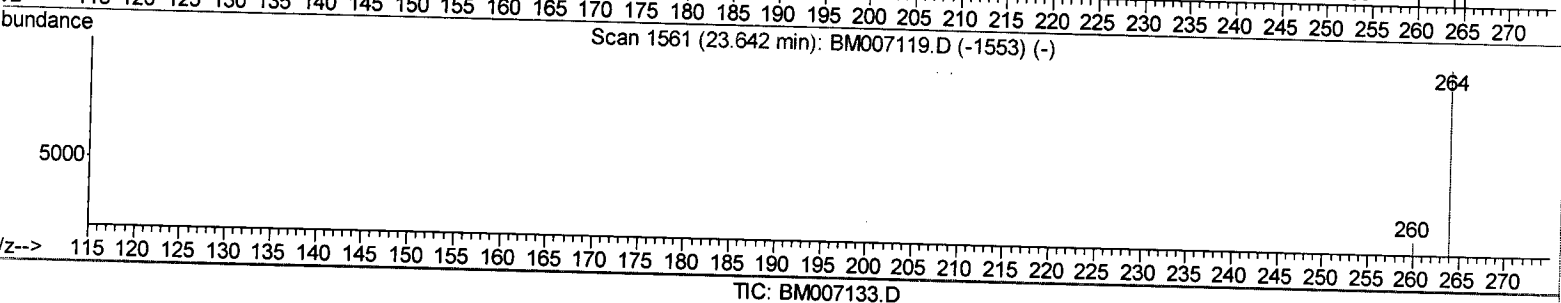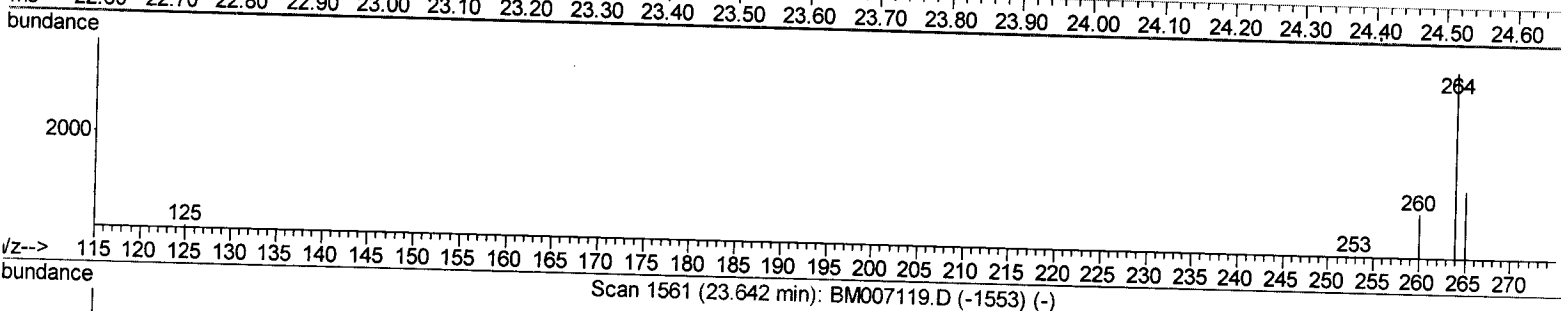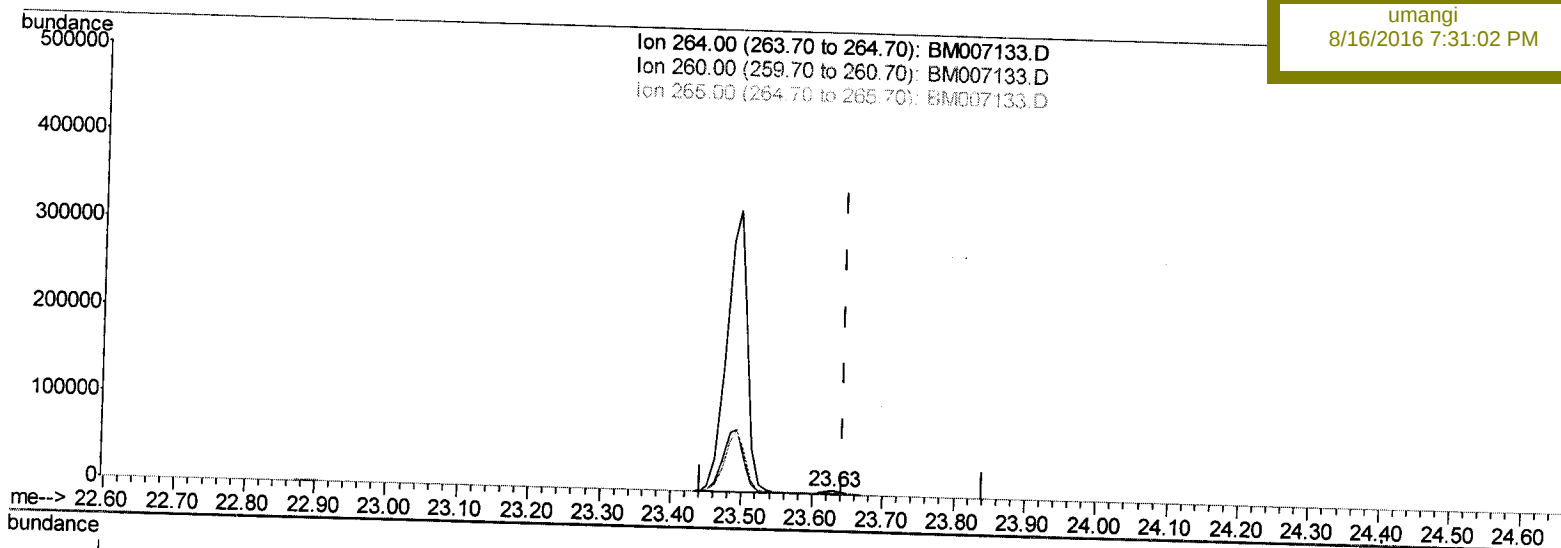

(20) Perylene-d12 (I)

23.628min (-0.014) 0.40ng/ul m

response 7668

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	27.28
265.00	38.20	39.54
0.00	0.00	0.00

U.M
 08/17/16




Data Path : Z:\HPCHEM1\BNA M\Data\BM081516\
 Data File : BM007133.D
 Acq On : 16 Aug 2016 01:08
 Operator : UM/SJ
 Sample : PB92717BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 16 03:56:08 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 16 01:54:24 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK17

Manual Integrations
 APPROVED

umangi
 8/16/2016 7:31:02 PM

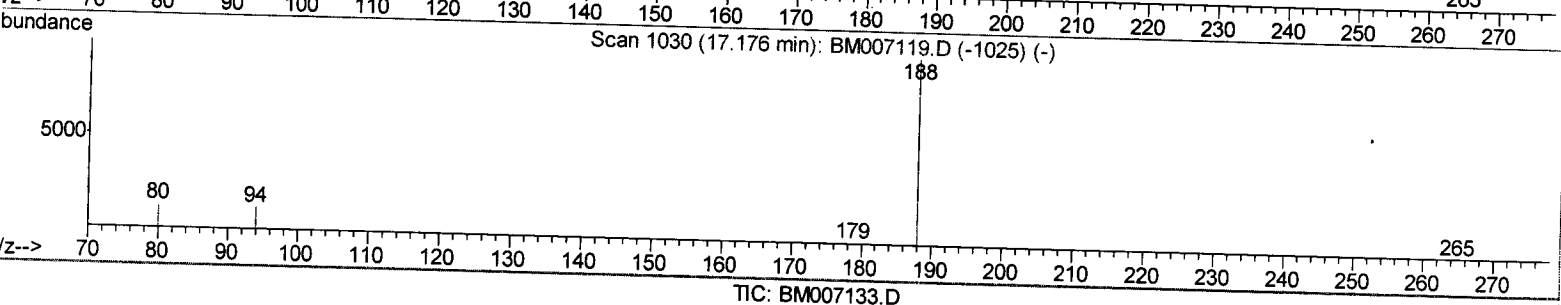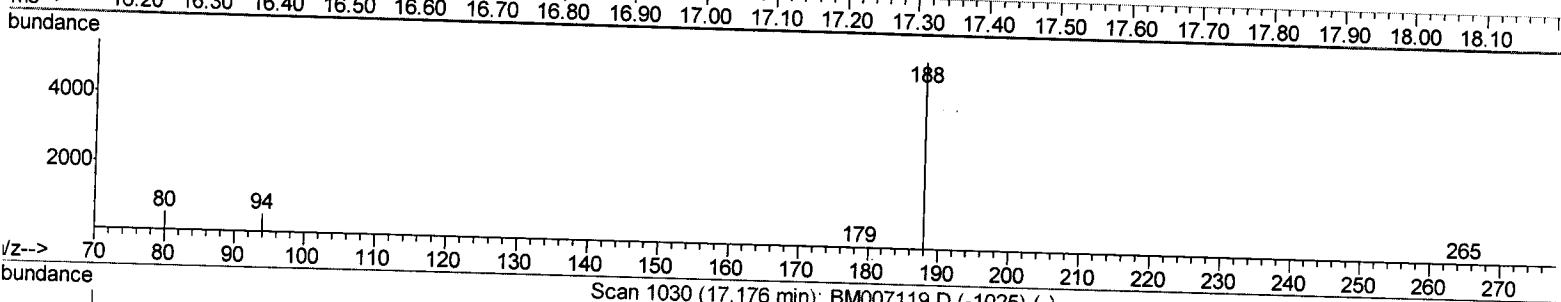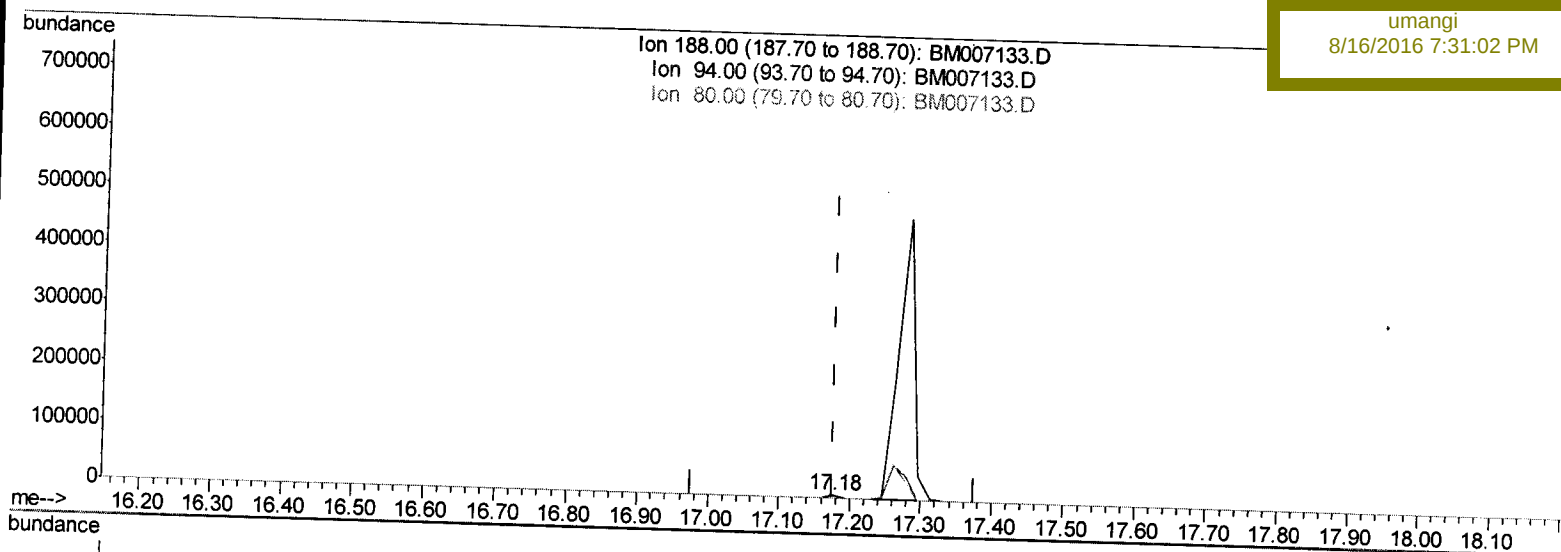

(10) Phenanthrene-d10 (I)

17.176min (+0.000) 0.40ng/ul m

response 7873

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	10.25
80.00	11.90	10.35
0.00	0.00	0.00

U.M
08/17/16




Data Path : Z:\HPCHEM1\BNA M\Data\BM081516\
Data File : BM007133.D
Acq On : 16 Aug 2016 01:08
Operator : UM/SJ
Sample : PB92717BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 17 04:31:34 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 01:54:24 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK17

Manual Integrations
APPROVED

umangi
8/16/2016 7:31:02 PM

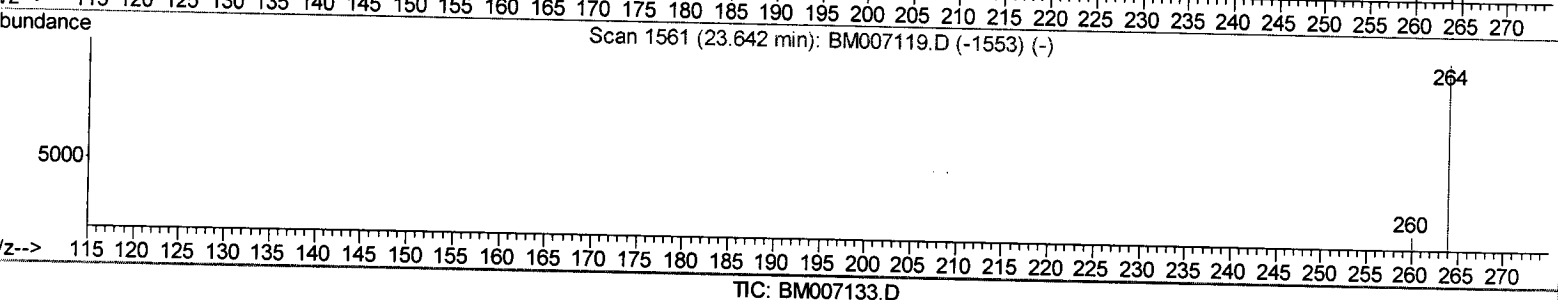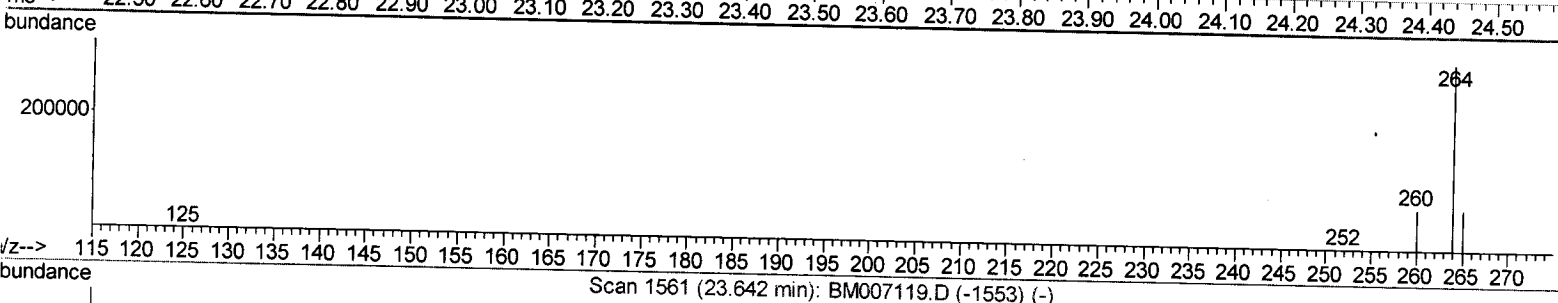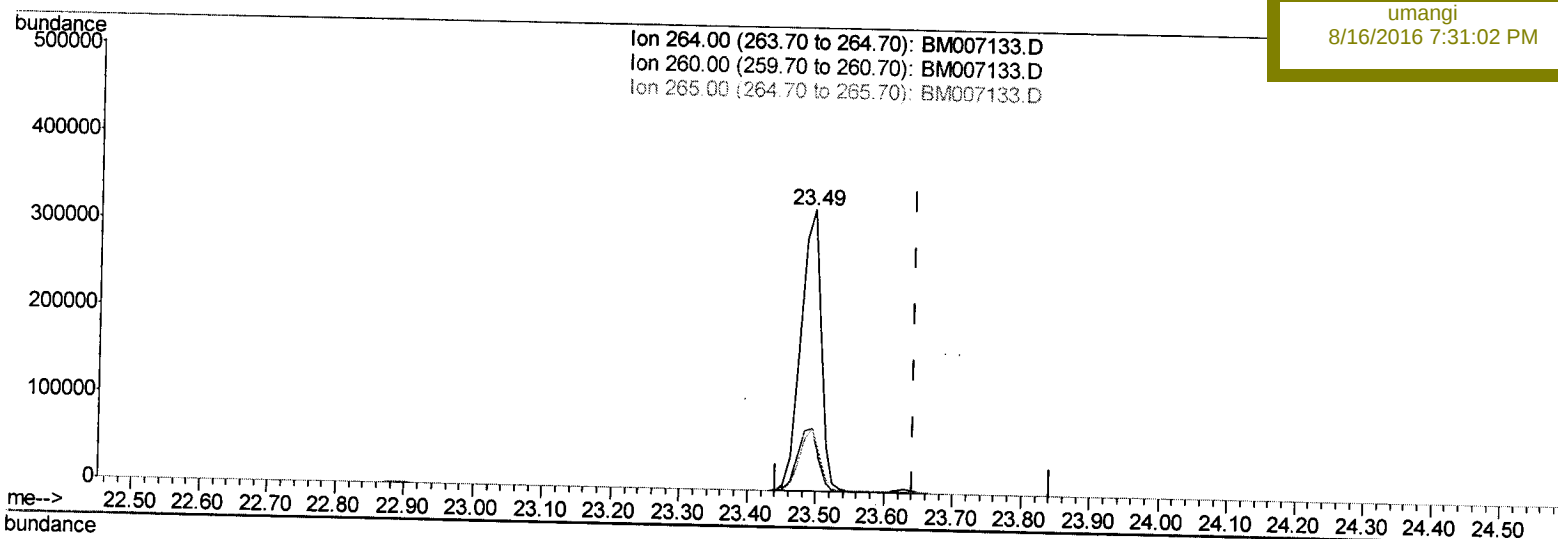

TIC: BM007133.D

(20) Perylene-d12 (I)

23.493min (-0.149) 0.40ng/ul

response 650280

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	22.15
265.00	38.20	21.76#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM081516\
Data File : BM007133.D
Acq On : 16 Aug 2016 01:08
Operator : UM/SJ
Sample : PB92717BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 16 03:56:08 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 01:54:24 2016
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
SBLK17

Manual Integrations
APPROVED
umangi
8/16/2016 7:31:02 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	1929	0.40	ng/ul	0.00
2) Naphthalene-d8	10.60	136	6877	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.43	164	3775	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.18	188	7873m	0.40	ng/ul	0.00
16) Chrysene-d12	21.36	240	7083	0.40	ng/ul	-0.01
20) Perylene-d12	23.63	264	7668m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.18	152	4013	0.47	ng/ul	0.00
14) Fluoranthene-d10	19.21	212	8533	0.48	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

g u m
08/17/16

Data Path : Z:\HPCHEM1\BNA M\Data\BM081516\
Data File : BM007133.D
Acq On : 16 Aug 2016 01:08
Operator : UM/SJ
Sample : PB92717BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 16 03:56:08 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 16 01:54:24 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK17

Manual Integrations
APPROVED

umangi
8/16/2016 7:31:02 PM

