
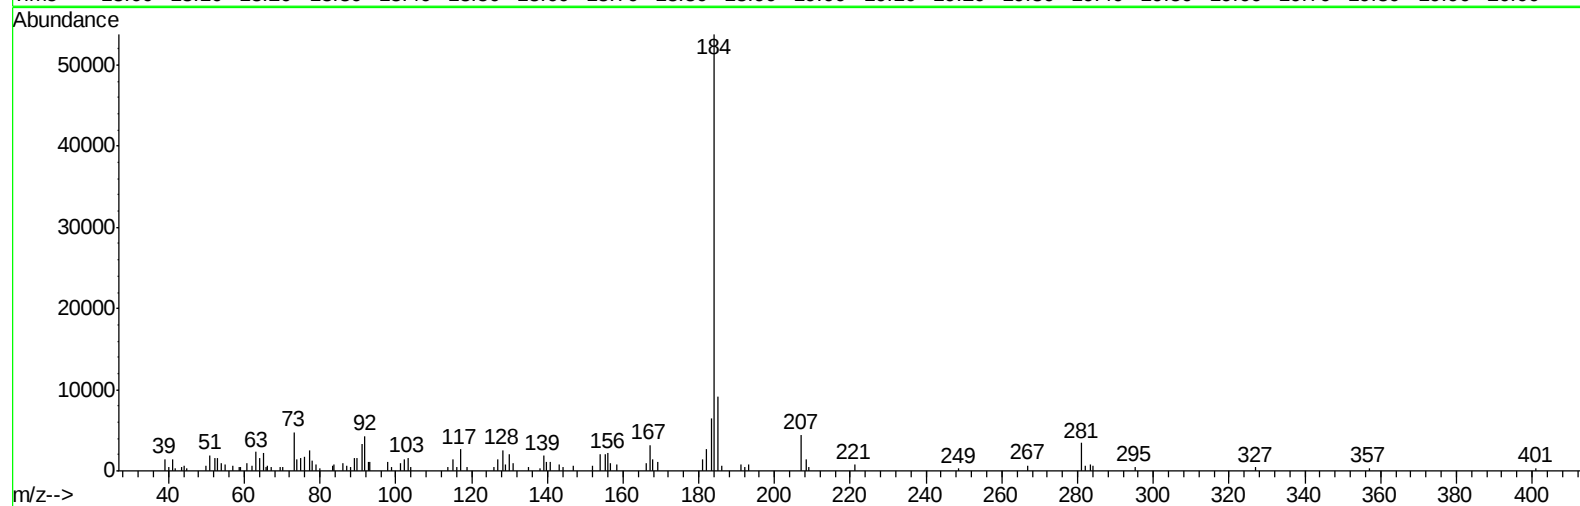


Data Path : Z:\HPCHEM1\BNA M\Data\BM081517\
Data File : BM011237.D
Acq On : 15 Aug 2017 16:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 03:18:53 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

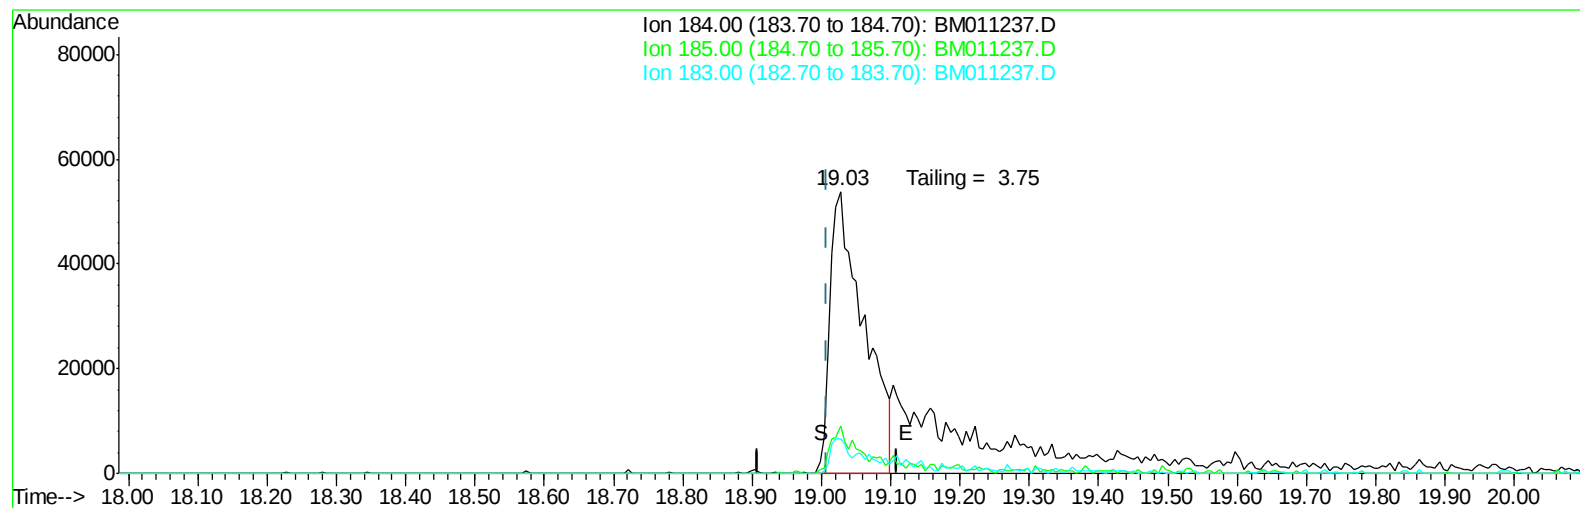

TIC: BM011237.D

(76) Benzidine



19.027min (+0.018) 26585.69ng

response 181261

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	17.03#
183.00	11.10	12.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM081517\
Data File : BM011237.D
Acq On : 15 Aug 2017 16:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 03:18:53 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

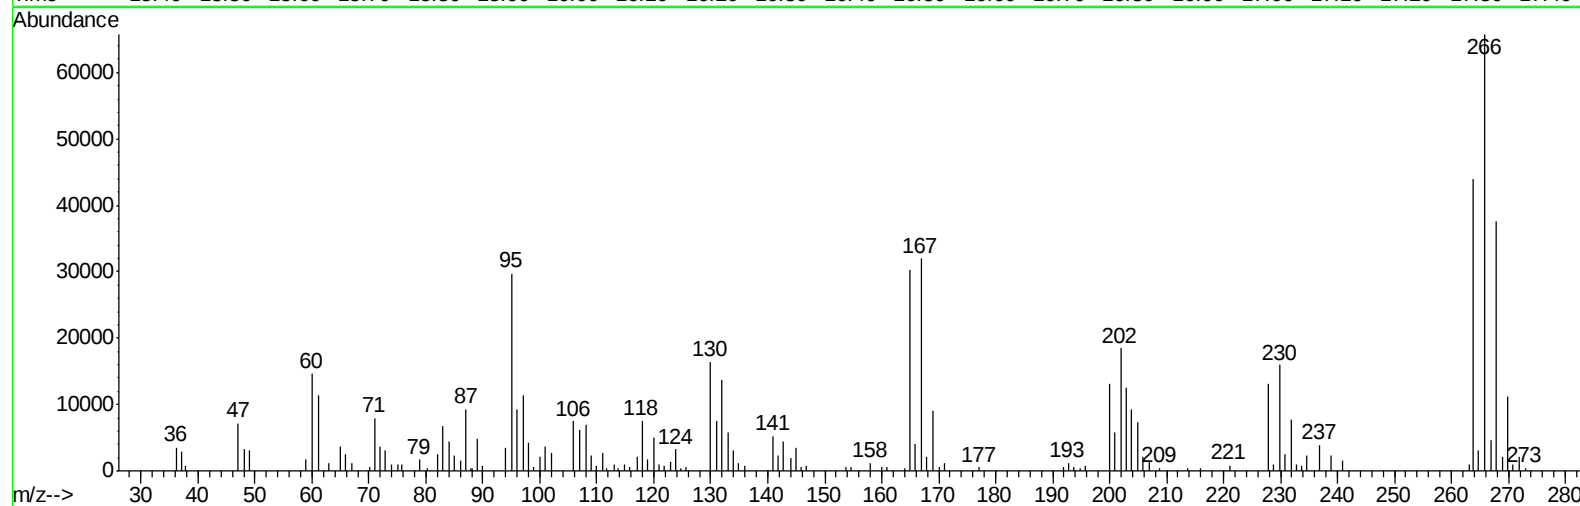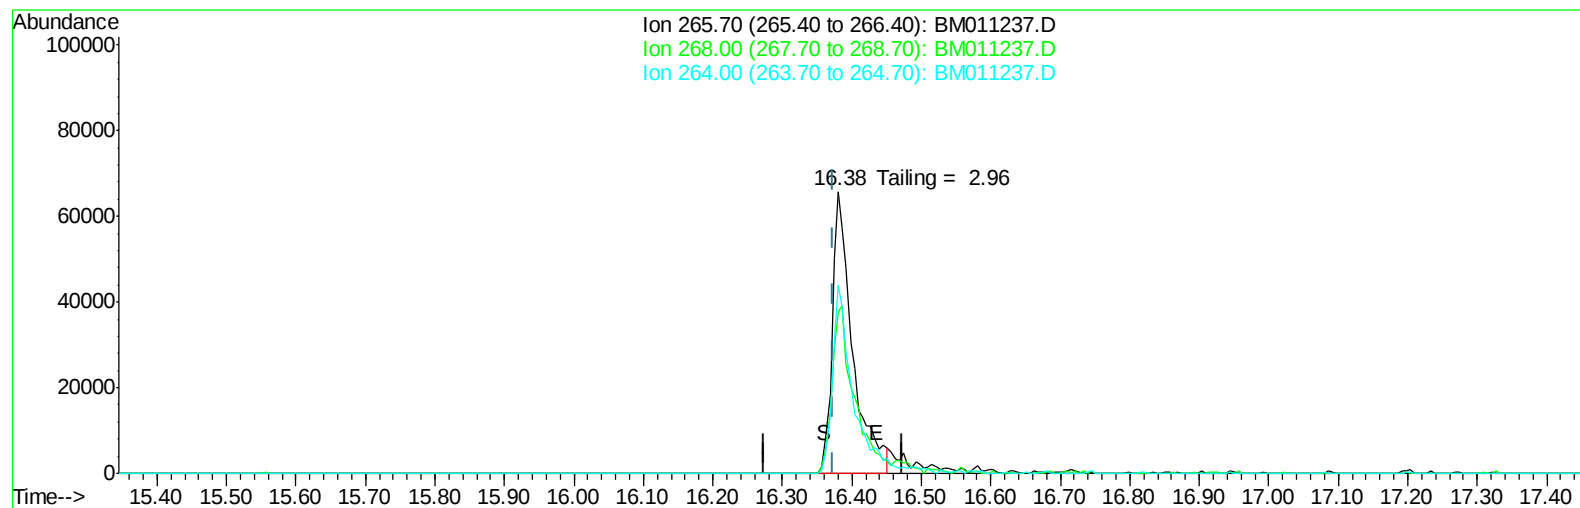

TIC: BM011237.D

(69) Pentachlorophenol (C)

16.380min (+0.006) 0.00ng

response 134020

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	57.11
264.00	61.20	66.79
0.00	0.00	0.00