


Data Path : Z:\HPCHEM1\BNA M\Data\BM081517\  
 Data File : BM011237.D  
 Acq On : 15 Aug 2017 16:14  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-BM072617.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Aug 16 02:25:04 2017

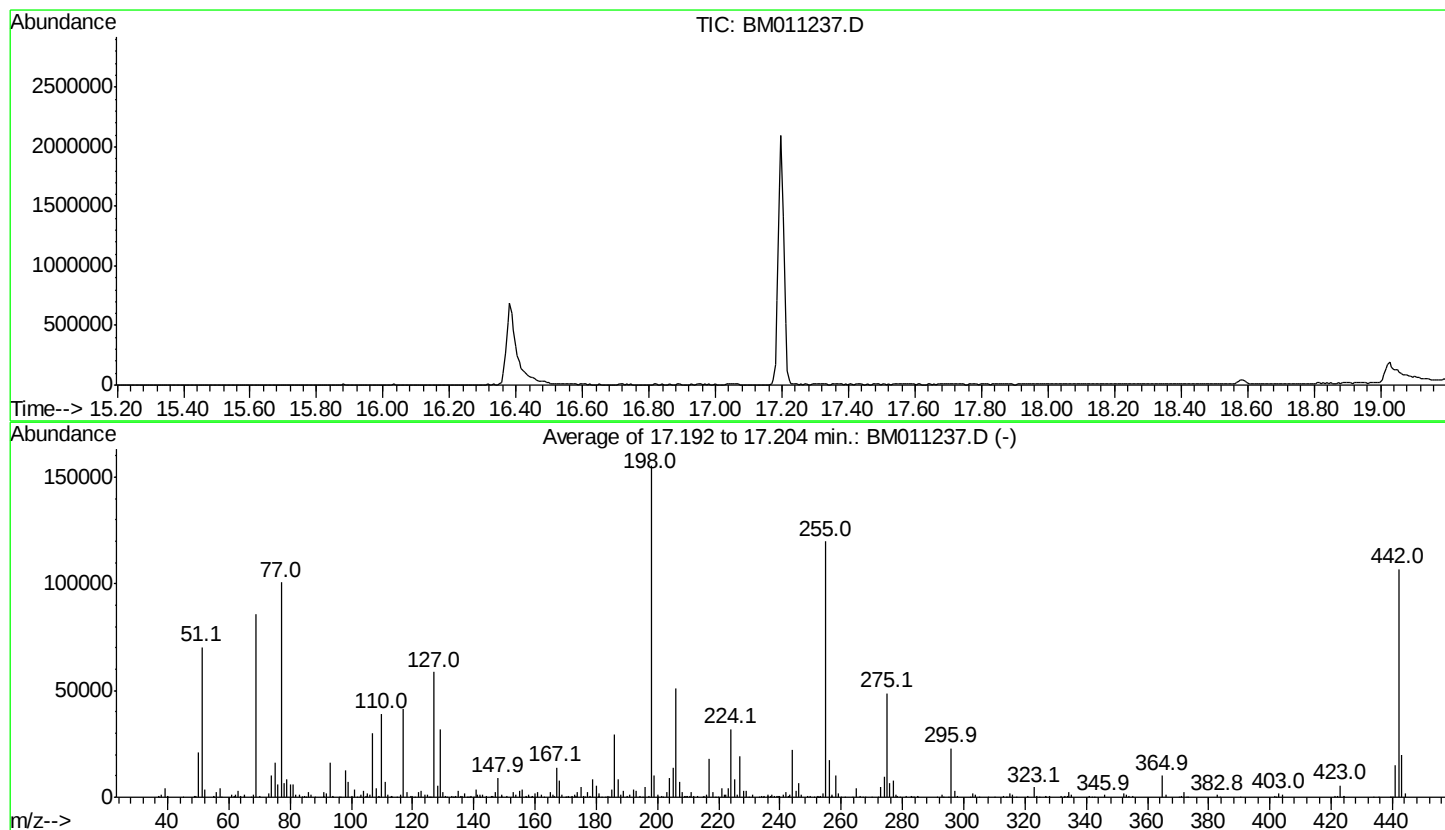

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 45.3      | 70501   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 1334    | PASS             |
| 69          | 198          | 0.00         | 100          | 55.1      | 85669   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 325     | PASS             |
| 127         | 198          | 10           | 80           | 37.7      | 58544   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 404     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 155469  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 10427   | PASS             |
| 275         | 198          | 10           | 60           | 31.3      | 48645   | PASS             |
| 365         | 198          | 1            | 100          | 6.5       | 10104   | PASS             |
| 441         | 443          | 0.01         | 100          | 77.5      | 15295   | PASS             |
| 442         | 198          | 50           | 100          | 68.8      | 107008  | PASS             |
| 443         | 442          | 15           | 24           | 18.4      | 19725   | PASS             |