




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036287.D
Acq On : 15 Aug 2022 15:21
Operator : CG/JU
Sample : N3951-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/16/2022
Supervised By :Sohil Jodhani 08/16/2022

Quant Time: Aug 15 15:56:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 14 23:34:05 2022
Response via : Initial Calibration

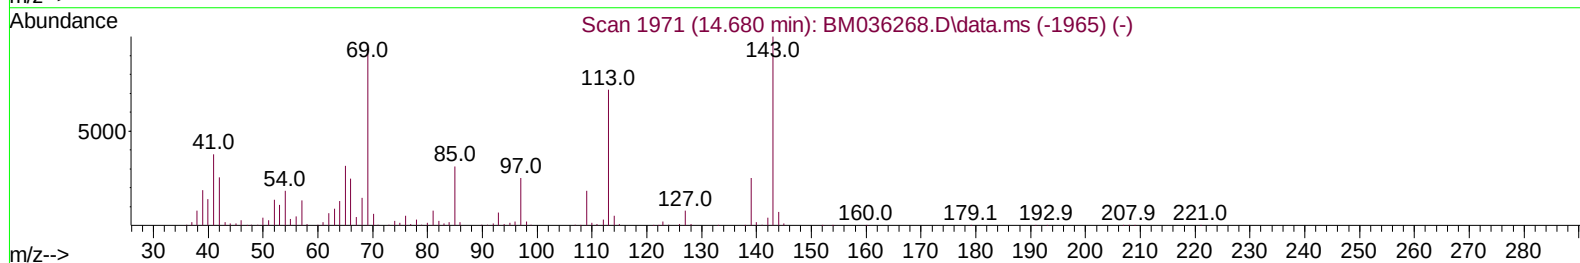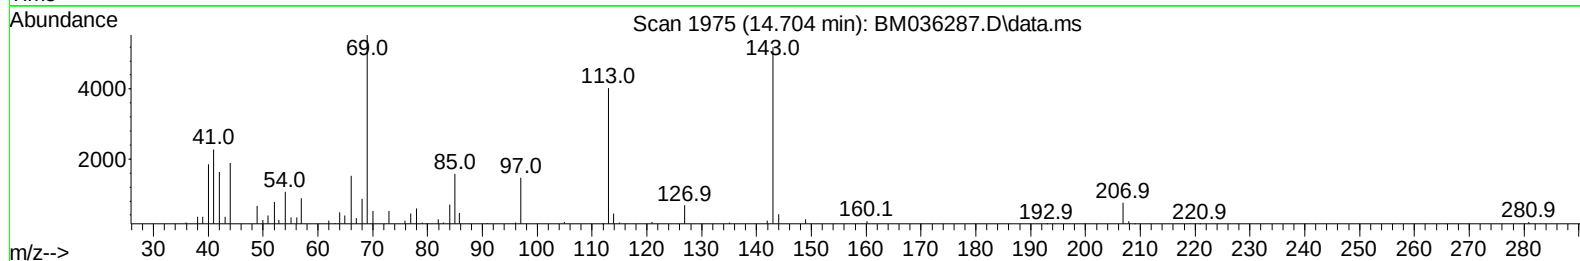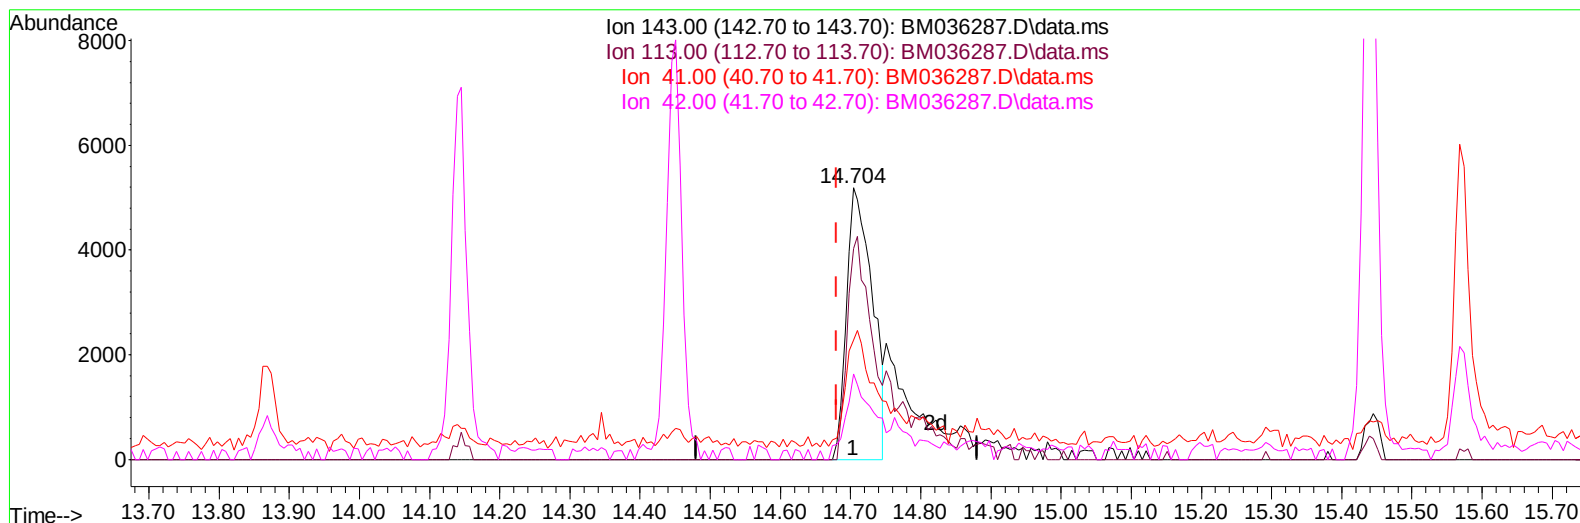

TIC: BM036287.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.704min (+ 0.023) 2.26 ng/ul

response 13208

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	77.62#
41.00	41.00	43.88
42.00	29.30	31.41




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036287.D
Acq On : 15 Aug 2022 15:21
Operator : CG/JU
Sample : N3951-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF8

Manual IntegrationsAPPROVED

Quant Time: Aug 15 15:56:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 14 23:34:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/16/2022
Supervised By :Sohil Jodhani 08/16/2022

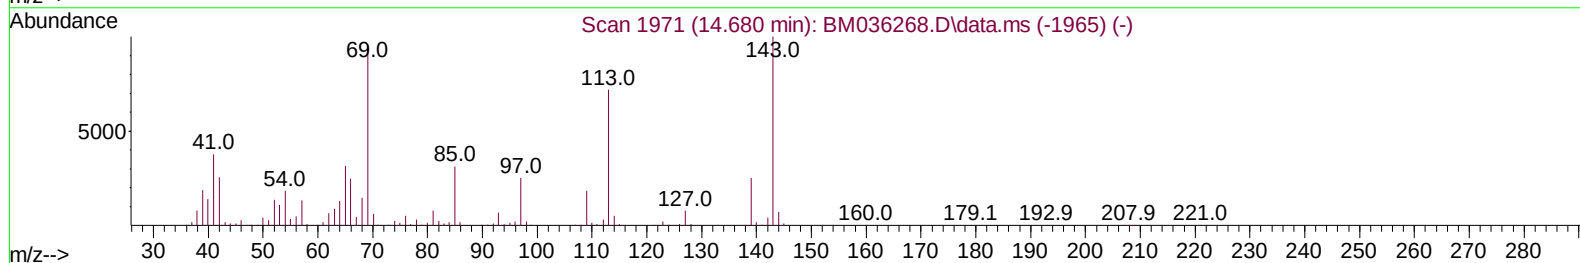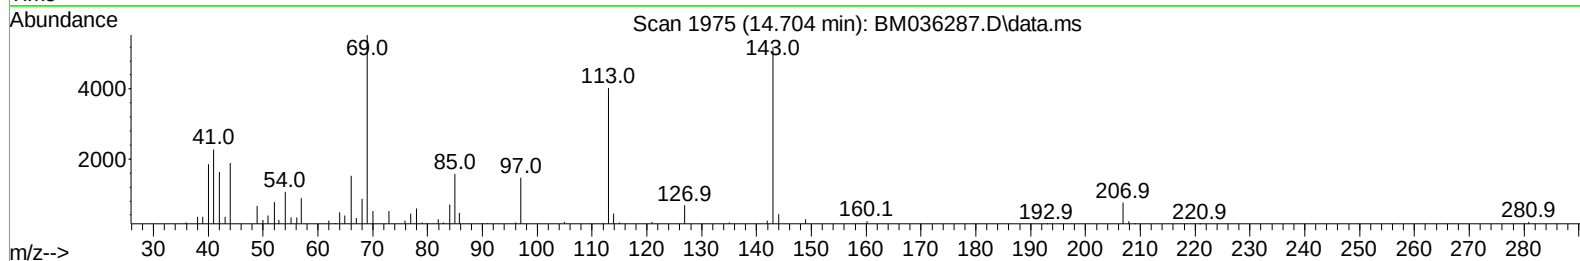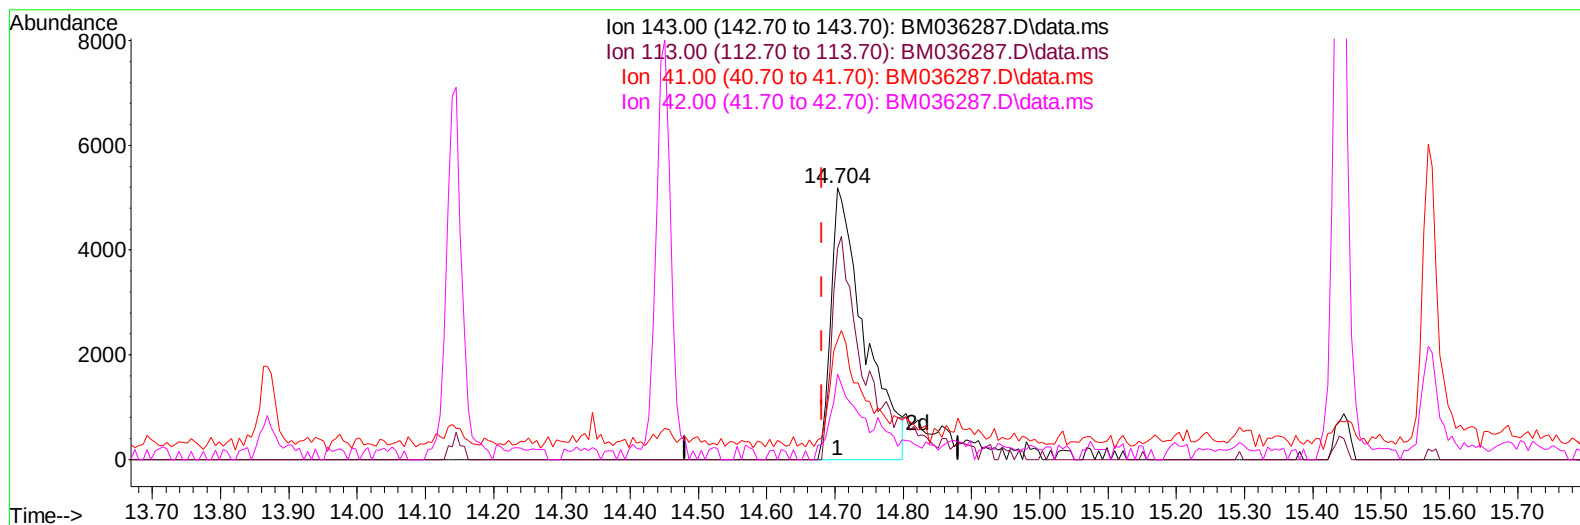

TIC: BM036287.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.704min (+ 0.023) 3.01 ng/ul m

response 17578

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	77.62#
41.00	41.00	43.88
42.00	29.30	31.41

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036287.D
 Acq On : 15 Aug 2022 15:21
 Operator : CG/JU
 Sample : N3951-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/16/2022
 Supervised By :Sohil Jodhani 08/16/2022

Quant Time: Aug 15 15:56:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 14 23:34:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	187772	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	751786	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	417326	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	839445	20.000	ng/ul	0.00
79) Chrysene-d12	21.374	240	904542	20.000	ng/ul	0.00
88) Perylene-d12	23.703	264	1021100	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	19579	3.924	ng/uL	0.00
4) Pyridine-d5	3.652	84	58890	4.308	ng/ul	0.01
7) Phenol-d5	6.993	99	74431	4.727	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.146	67	248273	23.651	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	243461	18.627	ng/ul	0.00
15) 4-Methylphenol-d8	8.534	113	135466	10.619	ng/ul	0.00
21) Nitrobenzene-d5	8.975	128	159141	26.714	ng/ul	0.00
24) 2-Nitrophenol-d4	9.698	143	154199	26.568	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.239	165	227714	21.693	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	182552	10.273	ng/ul	0.00
46) Dimethylphthalate-d6	13.869	166	764308	26.886	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	963035	26.552	ng/ul	0.00
54) 4-Nitrophenol-d4	14.704	143	17578m	3.011	ng/ul	0.02
60) Fluorene-d10	15.439	176	714099	27.799	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.574	200	99336	22.015	ng/ul	0.00
73) Anthracene-d10	17.292	188	1168302	30.784	ng/ul	0.00
81) Pyrene-d10	19.586	212	1420525	28.336	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.556	264	1594467	30.757	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036287.D
Acq On : 15 Aug 2022 15:21
Operator : CG/JU
Sample : N3951-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/16/2022
Supervised By :Sohil Jodhani 08/16/2022

Quant Time: Aug 15 15:56:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 14 23:34:05 2022
Response via : Initial Calibration

