

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036279.D
 Acq On : 15 Aug 2022 10:30
 Operator : CG/JU
 Sample : PB146648BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK648

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	29	rVB	62054	78863	2.11%	0.205%
2	3.640	91	94	113	rBV	568833	844918	22.59%	2.193%
3	3.963	145	149	154	rVB	15448	19253	0.51%	0.050%
4	6.992	657	664	678	rBV	683310	1156017	30.91%	3.000%
5	7.145	683	690	704	rVB	611702	965436	25.82%	2.506%
6	7.339	716	723	735	rBV	756207	1195609	31.97%	3.103%
7	7.804	796	802	813	rBV	632917	977116	26.13%	2.536%
8	8.533	919	926	941	rBV	817171	1383814	37.00%	3.592%
9	8.975	994	1001	1015	rBV	666674	1090096	29.15%	2.829%
10	9.698	1116	1124	1139	rBV	493305	842956	22.54%	2.188%
11	9.822	1142	1145	1149	rVB6	2994	3835	0.10%	0.010%
12	10.239	1209	1216	1239	rBV	703035	1287366	34.42%	3.341%
13	10.604	1271	1278	1290	rBV	815197	1369813	36.63%	3.555%
14	10.757	1296	1304	1330	rBV	798874	1571232	42.01%	4.078%
15	12.221	1545	1553	1564	rBV3	8633	22336	0.60%	0.058%
16	13.427	1754	1758	1764	rBV7	2433	4854	0.13%	0.013%
17	13.868	1827	1833	1850	rVB	1227180	1694459	45.31%	4.398%
18	14.145	1872	1880	1898	rBV	1485242	2205903	58.98%	5.725%
19	14.451	1925	1932	1945	rBV	1110570	1633556	43.68%	4.240%
20	14.680	1966	1971	1998	rBV	313548	774474	20.71%	2.010%
21	15.439	2092	2100	2112	rBV	1939370	2729465	72.98%	7.084%
22	15.568	2116	2122	2137	rBV	411126	671933	17.97%	1.744%
23	15.680	2138	2141	2146	rVB2	19207	26701	0.71%	0.069%
24	16.115	2209	2215	2217	rBV7	1776	3768	0.10%	0.010%
25	16.221	2230	2233	2237	rVB6	4175	6716	0.18%	0.017%
26	16.656	2304	2307	2313	rVB5	4082	7559	0.20%	0.020%
27	16.986	2360	2363	2366	rVB5	3316	3991	0.11%	0.010%
28	17.192	2392	2398	2408	rBV	1263224	1783458	47.69%	4.629%
29	17.292	2408	2415	2433	rVV	1979015	2918668	78.04%	7.575%
30	17.750	2492	2493	2497	rBV4	2980	4393	0.12%	0.011%
31	19.150	2727	2731	2735	rBV4	21039	29264	0.78%	0.076%
32	19.227	2741	2744	2748	rVB2	16617	18953	0.51%	0.049%
33	19.586	2799	2805	2815	rBV	2581059	3336648	89.22%	8.660%
34	20.586	2973	2975	2981	rVB4	37537	40665	1.09%	0.106%
35	21.374	3105	3109	3118	rBV	1395499	1944664	52.00%	5.047%
36	23.556	3474	3480	3496	rVB2	1941583	3739770	100.00%	9.707%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036279.D
Acq On : 15 Aug 2022 10:30
Operator : CG/JU
Sample : PB146648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	23.709	3500	3506	3523	rvB2	1046322	2139445	57.21%	5.553%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 38527967

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036279.D
Acq On : 15 Aug 2022 10:30
Operator : CG/JU
Sample : PB146648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

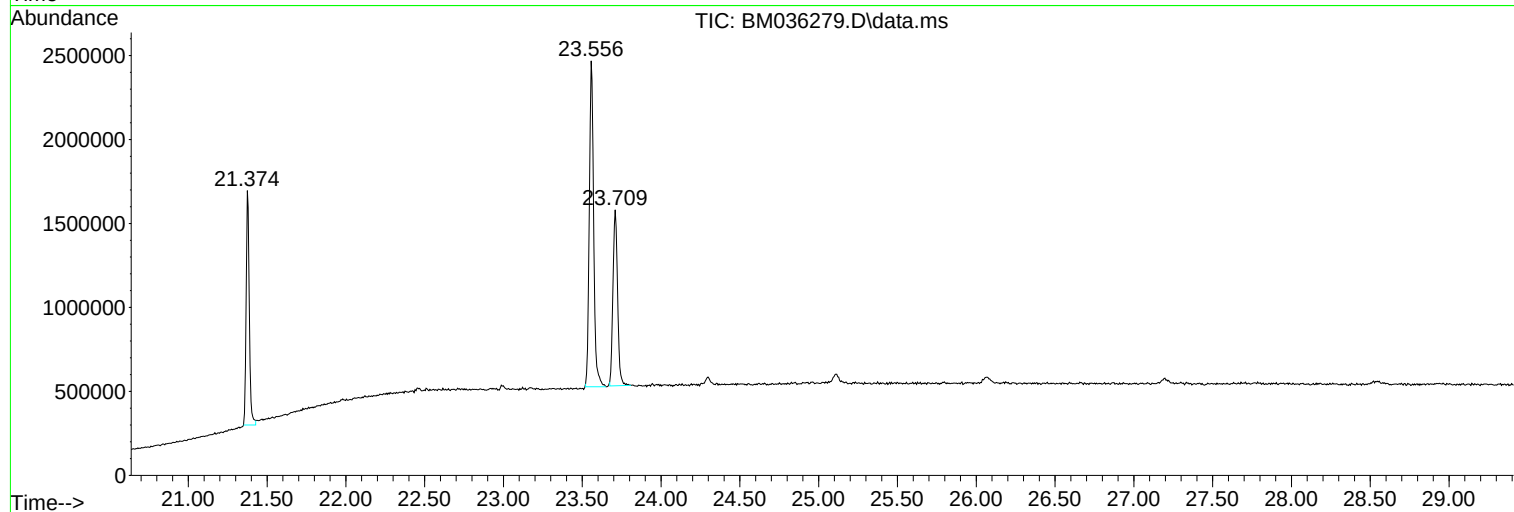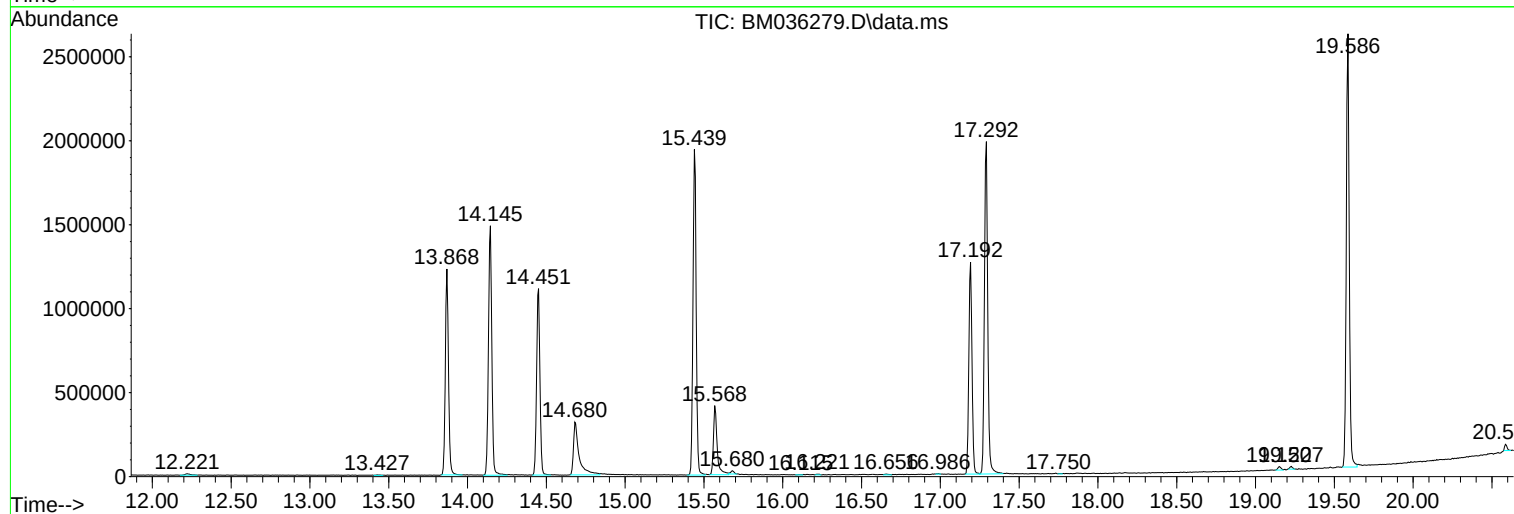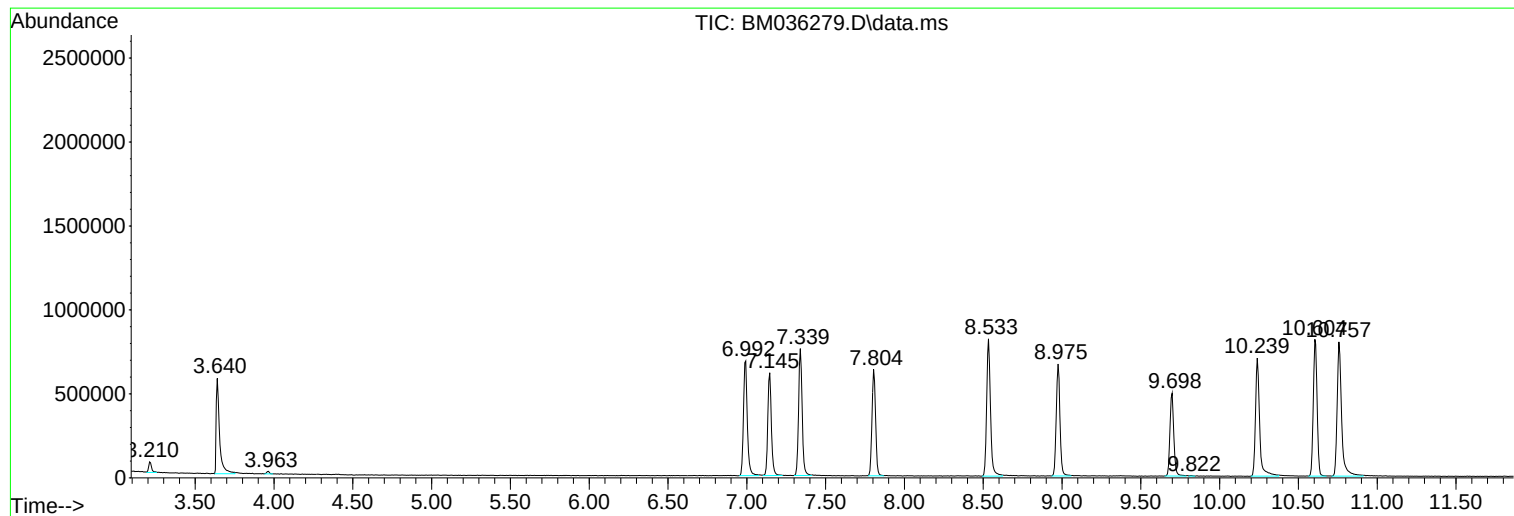

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036279.D
Acq On : 15 Aug 2022 10:30
Operator : CG/JU
Sample : PB146648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036279.D
Acq On : 15 Aug 2022 10:30
Operator : CG/JU
Sample : PB146648BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK648

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc