

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036281.D
 Acq On : 15 Aug 2022 11:42
 Operator : CG/JU
 Sample : PB146921BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK921

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	27	rBV	65446	77111	1.97%	0.196%
2	3.640	90	94	113	rBV	592477	894894	22.82%	2.272%
3	3.957	145	148	153	rVB2	16091	21127	0.54%	0.054%
4	6.992	657	664	675	rBV	734032	1222812	31.18%	3.104%
5	7.145	683	690	700	rBV	641598	995983	25.40%	2.528%
6	7.340	714	723	738	rBV	799816	1273534	32.47%	3.233%
7	7.804	794	802	813	rBV	652848	1032805	26.34%	2.622%
8	8.534	919	926	943	rBV	871189	1462157	37.28%	3.712%
9	8.975	994	1001	1017	rBV	698004	1156921	29.50%	2.937%
10	9.698	1115	1124	1133	rBV	515019	888571	22.66%	2.256%
11	10.239	1208	1216	1237	rBV	716239	1351651	34.47%	3.431%
12	10.604	1271	1278	1290	rBV	850882	1437564	36.66%	3.649%
13	10.757	1296	1304	1326	rBV	506358	1047604	26.71%	2.660%
14	12.222	1548	1553	1559	rVV3	9932	21743	0.55%	0.055%
15	13.868	1825	1833	1845	rBV	1258921	1737039	44.29%	4.410%
16	14.145	1872	1880	1892	rBV	1548405	2279668	58.13%	5.787%
17	14.451	1925	1932	1940	rBV	1155864	1667299	42.52%	4.233%
18	14.510	1940	1942	1948	rVB7	3679	5356	0.14%	0.014%
19	14.680	1965	1971	1999	rBV	334028	829500	21.15%	2.106%
20	15.439	2093	2100	2112	rBV	1936845	2784664	71.01%	7.069%
21	15.568	2117	2122	2137	rVV	422918	698730	17.82%	1.774%
22	15.680	2137	2141	2146	rVB2	20354	34319	0.88%	0.087%
23	16.221	2230	2233	2237	rVB5	5669	7979	0.20%	0.020%
24	16.504	2275	2281	2285	rBV9	3109	6852	0.17%	0.017%
25	16.657	2304	2307	2310	rBV4	3932	5821	0.15%	0.015%
26	16.962	2354	2359	2360	rBV5	4698	6806	0.17%	0.017%
27	16.980	2360	2362	2367	rVB3	3506	6050	0.15%	0.015%
28	17.192	2392	2398	2408	rBV	1326287	1799136	45.88%	4.567%
29	17.292	2408	2415	2431	rVV	2052927	2930033	74.71%	7.438%
30	18.927	2691	2693	2696	rBV4	4453	6313	0.16%	0.016%
31	19.151	2728	2731	2736	rVB5	20336	29582	0.75%	0.075%
32	19.227	2739	2744	2749	rBV2	21523	35192	0.90%	0.089%
33	19.586	2799	2805	2815	rBV	2552903	3381149	86.22%	8.584%
34	20.586	2972	2975	2980	rBV	53101	63320	1.61%	0.161%
35	21.374	3104	3109	3119	rBV	1533908	2081572	53.08%	5.284%
36	23.556	3474	3480	3494	rVB2	2013508	3921617	100.00%	9.956%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036281.D
Acq On : 15 Aug 2022 11:42
Operator : CG/JU
Sample : PB146921BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK921

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	23.709	3500	3506	3518	rVB2	1093074	2188303	55.80%	5.555%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 39390777

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036281.D
Acq On : 15 Aug 2022 11:42
Operator : CG/JU
Sample : PB146921BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK921

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

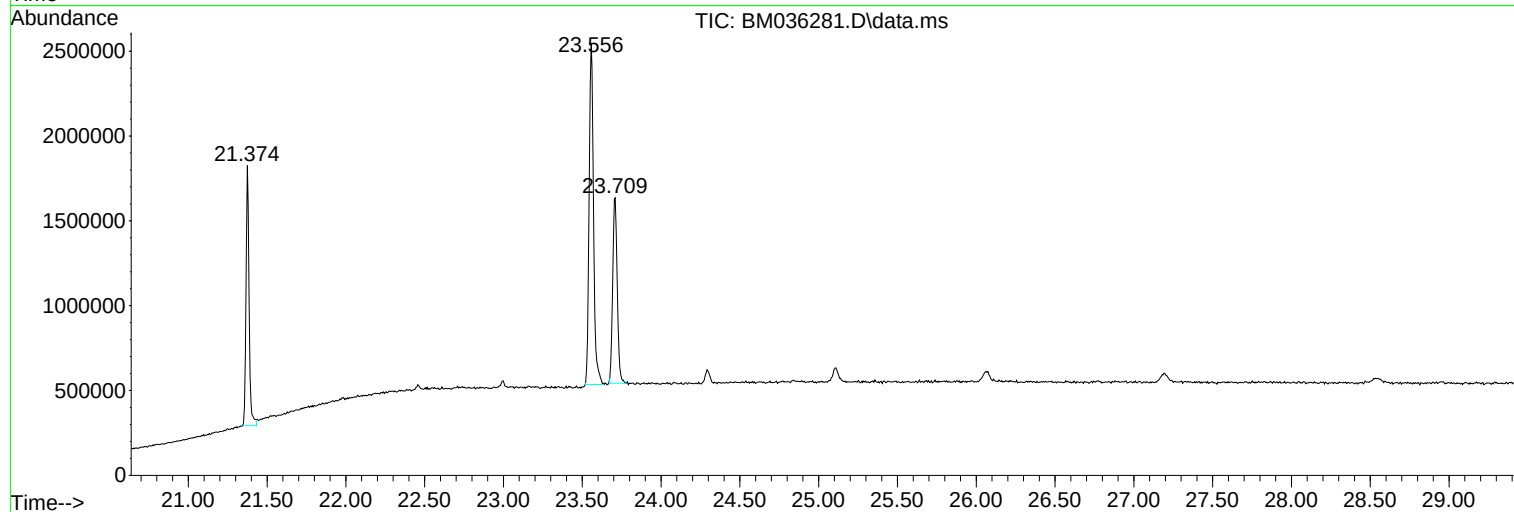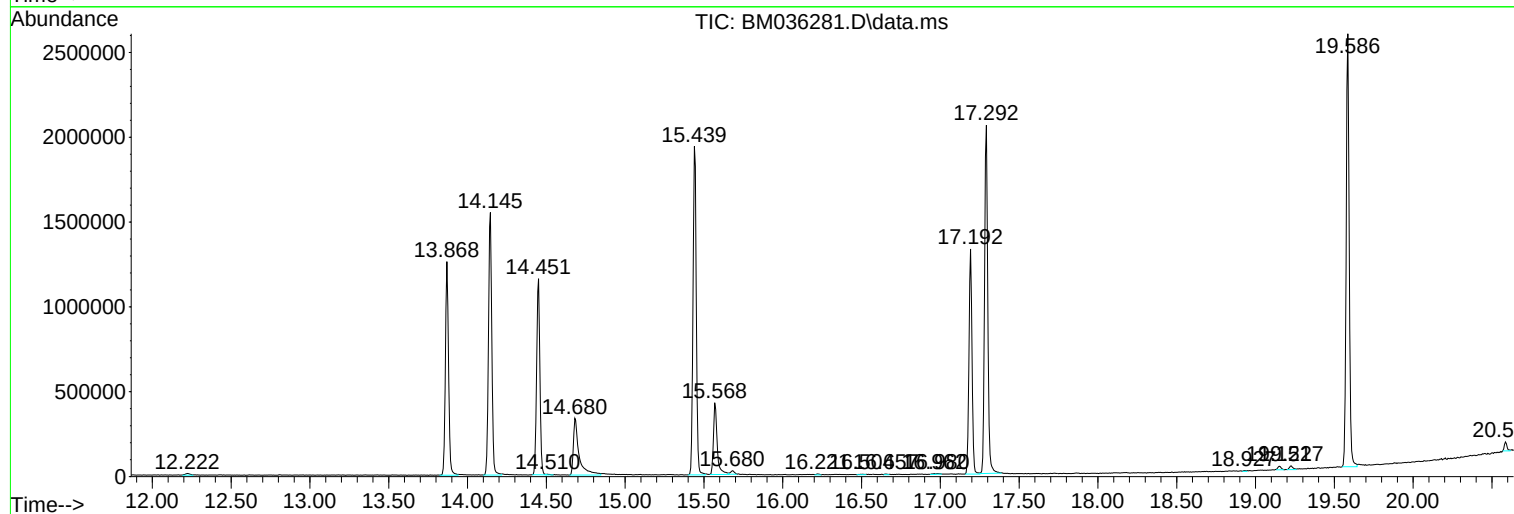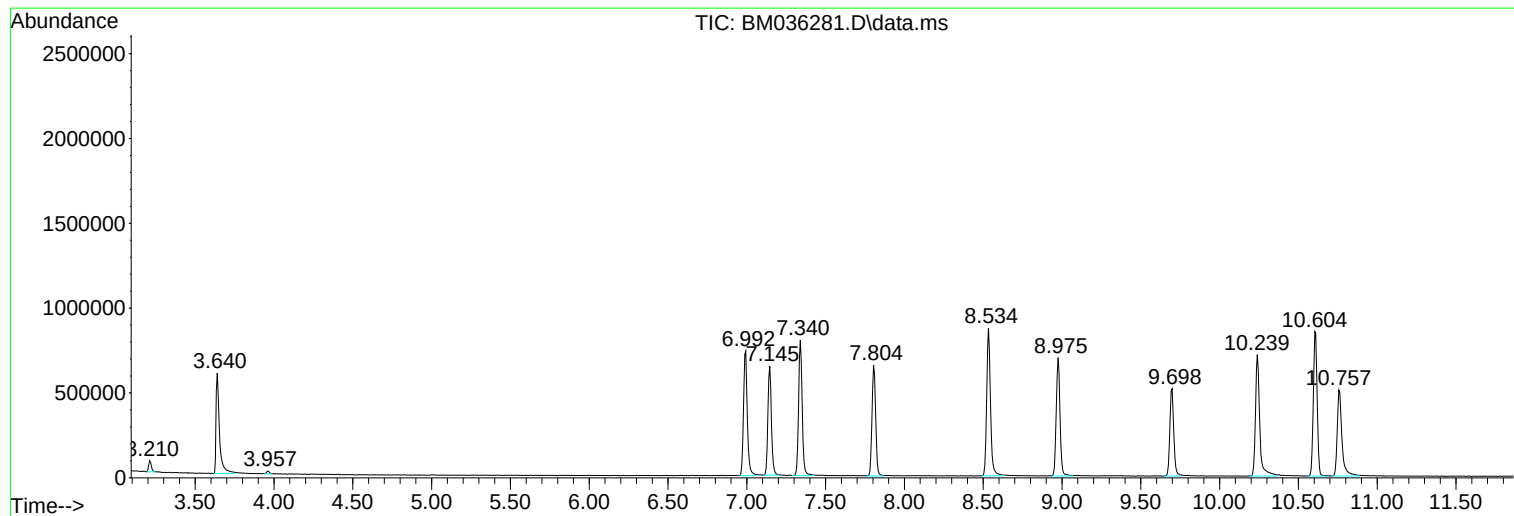

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036281.D
Acq On : 15 Aug 2022 11:42
Operator : CG/JU
Sample : PB146921BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK921

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036281.D
Acq On : 15 Aug 2022 11:42
Operator : CG/JU
Sample : PB146921BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK921

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc