

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036283.D
 Acq On : 15 Aug 2022 12:55
 Operator : CG/JU
 Sample : N3951-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COCA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	28	rVB	45559	56545	1.28%	0.151%
2	3.652	94	96	110	rBV	88064	155833	3.54%	0.416%
3	3.863	127	132	137	rVB	17910	29287	0.67%	0.078%
4	3.957	145	148	153	rVB	17555	22897	0.52%	0.061%
5	4.340	211	213	219	rBV7	2656	5115	0.12%	0.014%
6	4.410	220	225	231	rVB	31531	44372	1.01%	0.118%
7	5.016	325	328	332	rBV6	4584	6091	0.14%	0.016%
8	6.928	648	653	657	rVB2	13422	20104	0.46%	0.054%
9	6.993	658	664	677	rVB	118025	212558	4.83%	0.567%
10	7.145	683	690	701	rBV	590877	960153	21.82%	2.562%
11	7.340	717	723	734	rBV	545593	873829	19.86%	2.332%
12	7.804	796	802	812	rBV	718502	1134532	25.78%	3.027%
13	7.875	812	814	819	rVB4	6410	10783	0.25%	0.029%
14	8.534	920	926	945	rBV	345191	627056	14.25%	1.673%
15	8.975	994	1001	1017	rBV	650609	1113270	25.30%	2.971%
16	9.369	1062	1068	1075	rVB2	16087	24577	0.56%	0.066%
17	9.698	1117	1124	1134	rBV	467000	799856	18.17%	2.134%
18	10.239	1208	1216	1235	rBV	587327	1129206	25.66%	3.013%
19	10.610	1271	1279	1292	rVB	926211	1559054	35.43%	4.160%
20	10.763	1297	1305	1322	rBV	286682	634295	14.41%	1.693%
21	11.863	1487	1492	1498	rBV2	8842	13611	0.31%	0.036%
22	12.222	1546	1553	1559	rBV3	8254	18349	0.42%	0.049%
23	13.869	1823	1833	1849	rBV	1241501	1735458	39.43%	4.631%
24	14.145	1873	1880	1891	rBV	1522976	2190644	49.78%	5.845%
25	14.451	1925	1932	1944	rBV	1287256	1847048	41.97%	4.929%
26	14.704	1967	1975	1985	rBV4	30110	95202	2.16%	0.254%
27	15.204	2053	2060	2065	rBV2	8895	15774	0.36%	0.042%
28	15.286	2070	2074	2080	rVB5	2998	6427	0.15%	0.017%
29	15.439	2092	2100	2117	rBV	1933757	2770515	62.95%	7.393%
30	15.568	2117	2122	2133	rVV	447999	695820	15.81%	1.857%
31	15.686	2137	2142	2148	rVB	20567	34366	0.78%	0.092%
32	16.157	2219	2222	2227	rBV6	3694	5595	0.13%	0.015%
33	16.227	2229	2234	2238	rVB7	5907	7463	0.17%	0.020%
34	16.339	2250	2253	2258	rVB7	3054	4992	0.11%	0.013%
35	16.657	2303	2307	2313	rVB4	7432	11434	0.26%	0.031%
36	16.880	2342	2345	2348	rVB5	3710	4794	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036283.D
 Acq On : 15 Aug 2022 12:55
 Operator : CG/JU
 Sample : N3951-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COCA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.963	2355	2359	2360	rBV4	5646	6922	0.16%	0.018%
38	16.986	2360	2363	2368	rVB6	4405	7471	0.17%	0.020%
39	17.192	2392	2398	2405	rBV	1494493	2027105	46.06%	5.409%
40	17.292	2409	2415	2426	rVV	2245228	3107197	70.60%	8.291%
41	17.727	2485	2489	2493	rBV6	7387	10994	0.25%	0.029%
42	17.868	2507	2513	2519	rBV9	7259	18999	0.43%	0.051%
43	18.092	2547	2551	2560	rBV6	21750	40689	0.92%	0.109%
44	18.168	2561	2564	2567	rVB4	6172	7718	0.18%	0.021%
45	19.151	2727	2731	2736	rBV3	26403	40651	0.92%	0.108%
46	19.221	2740	2743	2748	rBV	25544	35358	0.80%	0.094%
47	19.586	2799	2805	2816	rBV	2864660	3718202	84.49%	9.921%
48	20.586	2972	2975	2979	rBV	54168	55295	1.26%	0.148%
49	21.374	3104	3109	3119	rBV	1909769	2460678	55.91%	6.566%
50	23.556	3474	3480	3496	rVB2	2314669	4400924	100.00%	11.743%
51	23.709	3499	3506	3519	rVB2	1336573	2661106	60.47%	7.101%




Sum of corrected areas: 37476214

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036283.D
Acq On : 15 Aug 2022 12:55
Operator : CG/JU
Sample : N3951-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COCA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

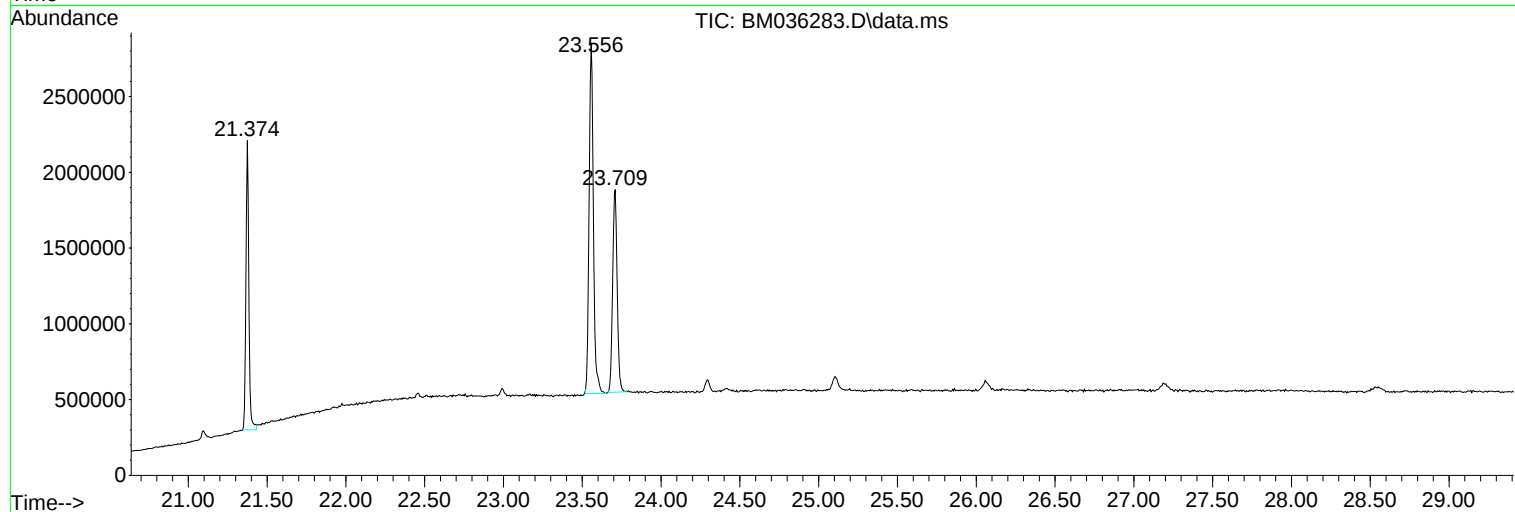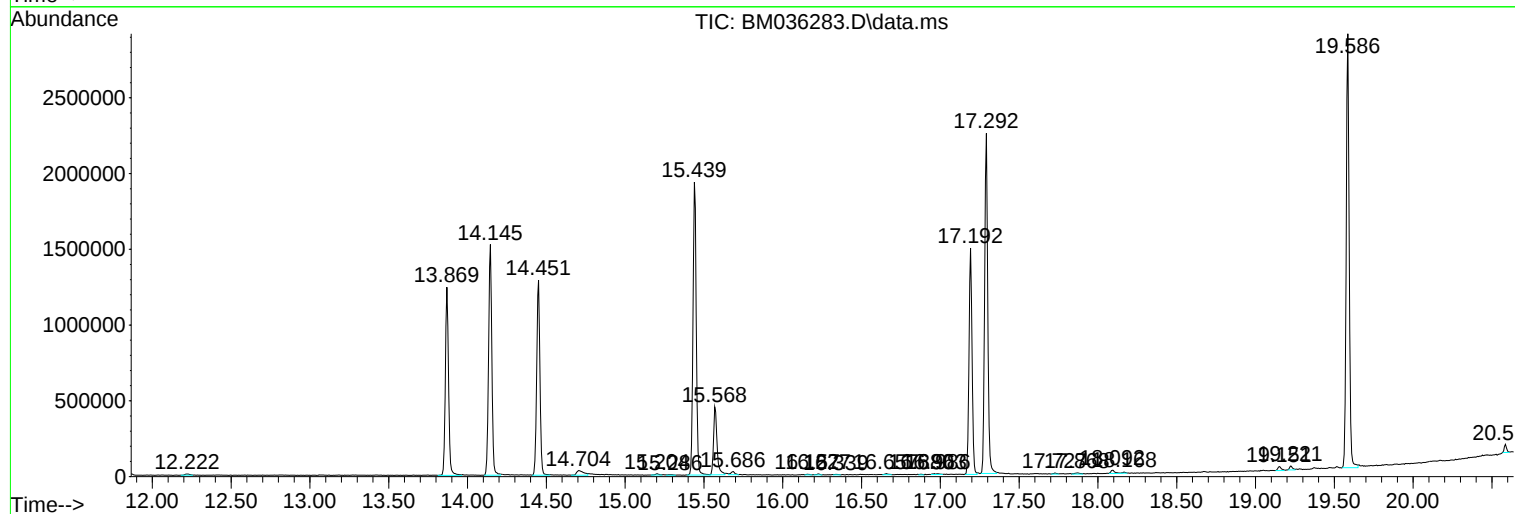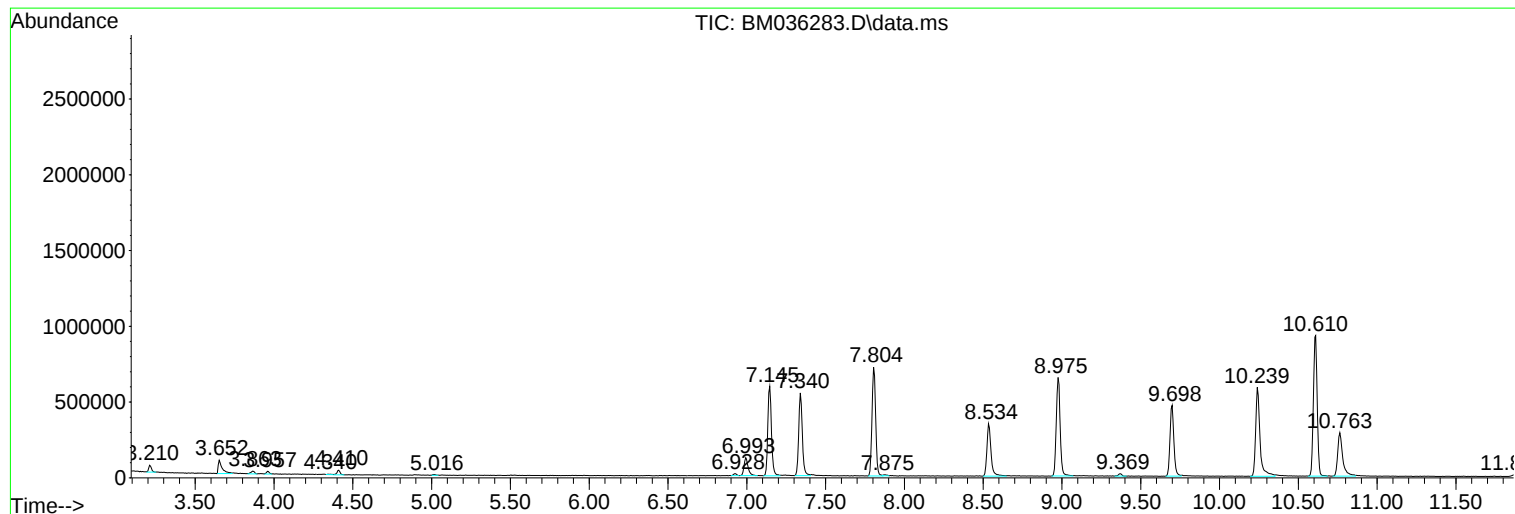

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036283.D
Acq On : 15 Aug 2022 12:55
Operator : CG/JU
Sample : N3951-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036283.D
Acq On : 15 Aug 2022 12:55
Operator : CG/JU
Sample : N3951-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc