

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036285.D
 Acq On : 15 Aug 2022 14:08
 Operator : CG/JU
 Sample : N3951-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COCA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	28	rVB	34102	43787	0.97%	0.120%
2	3.657	95	97	107	rBV	59944	104755	2.33%	0.287%
3	3.869	129	133	138	rVB	18723	27843	0.62%	0.076%
4	3.963	145	149	154	rVB2	14357	21081	0.47%	0.058%
5	4.410	221	225	230	rVB	26123	33951	0.76%	0.093%
6	5.016	324	328	332	rVB7	3919	4811	0.11%	0.013%
7	6.922	648	652	656	rBV	12619	17880	0.40%	0.049%
8	6.993	659	664	676	rBV	118281	212013	4.72%	0.580%
9	7.145	683	690	701	rBV	624799	983834	21.88%	2.693%
10	7.240	704	706	711	rVB5	5281	7231	0.16%	0.020%
11	7.340	716	723	735	rBV	542408	889090	19.78%	2.433%
12	7.416	735	736	740	rVB3	5821	5503	0.12%	0.015%
13	7.804	796	802	812	rBV	557848	897067	19.95%	2.455%
14	7.881	812	815	821	rVB5	6435	12335	0.27%	0.034%
15	8.534	919	926	940	rBV	363067	627910	13.97%	1.719%
16	8.975	993	1001	1014	rBV	685895	1147056	25.52%	3.139%
17	9.369	1064	1068	1074	rVB2	16213	23612	0.53%	0.065%
18	9.698	1117	1124	1142	rBV	479534	824338	18.34%	2.256%
19	10.239	1209	1216	1234	rBV	610778	1149155	25.56%	3.145%
20	10.610	1271	1279	1289	rBV	739800	1240507	27.59%	3.395%
21	10.763	1298	1305	1327	rBV	230317	502841	11.19%	1.376%
22	11.863	1486	1492	1500	rVB3	9368	14474	0.32%	0.040%
23	12.222	1546	1553	1562	rVB2	9029	21264	0.47%	0.058%
24	13.274	1728	1732	1739	rBV7	2790	5782	0.13%	0.016%
25	13.427	1754	1758	1764	rVB7	4603	8347	0.19%	0.023%
26	13.869	1826	1833	1849	rBV	1350857	1869492	41.59%	5.117%
27	14.145	1871	1880	1894	rBV	1640454	2353458	52.35%	6.441%
28	14.345	1911	1914	1920	rVB7	3214	5554	0.12%	0.015%
29	14.451	1925	1932	1945	rVB	1016581	1486704	33.07%	4.069%
30	14.704	1970	1975	1986	rBV3	33644	107504	2.39%	0.294%
31	15.439	2090	2100	2109	rBV	2075916	2979146	66.27%	8.154%
32	15.568	2117	2122	2136	rBV	499322	770366	17.14%	2.108%
33	15.686	2138	2142	2146	rVB	18710	28446	0.63%	0.078%
34	16.157	2214	2222	2226	rBV10	3740	8776	0.20%	0.024%
35	16.221	2230	2233	2240	rVB8	5522	10276	0.23%	0.028%
36	16.657	2304	2307	2312	rBV5	6145	8838	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036285.D
 Acq On : 15 Aug 2022 14:08
 Operator : CG/JU
 Sample : N3951-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.868	2341	2343	2349	rBV5	3036	4694	0.10%	0.013%
38	16.957	2353	2358	2360	rBV5	4048	6870	0.15%	0.019%
39	17.192	2391	2398	2408	rBV	1210036	1670582	37.16%	4.572%
40	17.292	2408	2415	2429	rVV	2406581	3347515	74.46%	9.162%
41	17.727	2487	2489	2492	rVB3	4521	5275	0.12%	0.014%
42	17.868	2508	2513	2515	rBV6	4841	5881	0.13%	0.016%
43	18.092	2546	2551	2558	rBV3	35538	64658	1.44%	0.177%
44	18.168	2562	2564	2568	rVB3	6095	6963	0.15%	0.019%
45	18.674	2648	2650	2654	rVB4	5952	5831	0.13%	0.016%
46	19.151	2727	2731	2737	rBV3	29783	41681	0.93%	0.114%
47	19.221	2740	2743	2747	rBV2	23157	31582	0.70%	0.086%
48	19.374	2766	2769	2775	rBV7	10271	19480	0.43%	0.053%
49	19.462	2782	2784	2785	rBV2	7258	6083	0.14%	0.017%
50	19.586	2799	2805	2813	rBV	3107991	3975070	88.42%	10.879%
51	20.586	2972	2975	2979	rBV	52055	57632	1.28%	0.158%
52	21.092	3057	3061	3072	rBV3	149178	319837	7.11%	0.875%
53	21.374	3104	3109	3116	rBV	1503166	1926932	42.86%	5.274%
54	23.556	3473	3480	3493	rBV	2350124	4495510	100.00%	12.304%
55	23.703	3499	3505	3515	rVB2	1085182	2090208	46.50%	5.721%




Sum of corrected areas: 36537311

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036285.D
Acq On : 15 Aug 2022 14:08
Operator : CG/JU
Sample : N3951-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

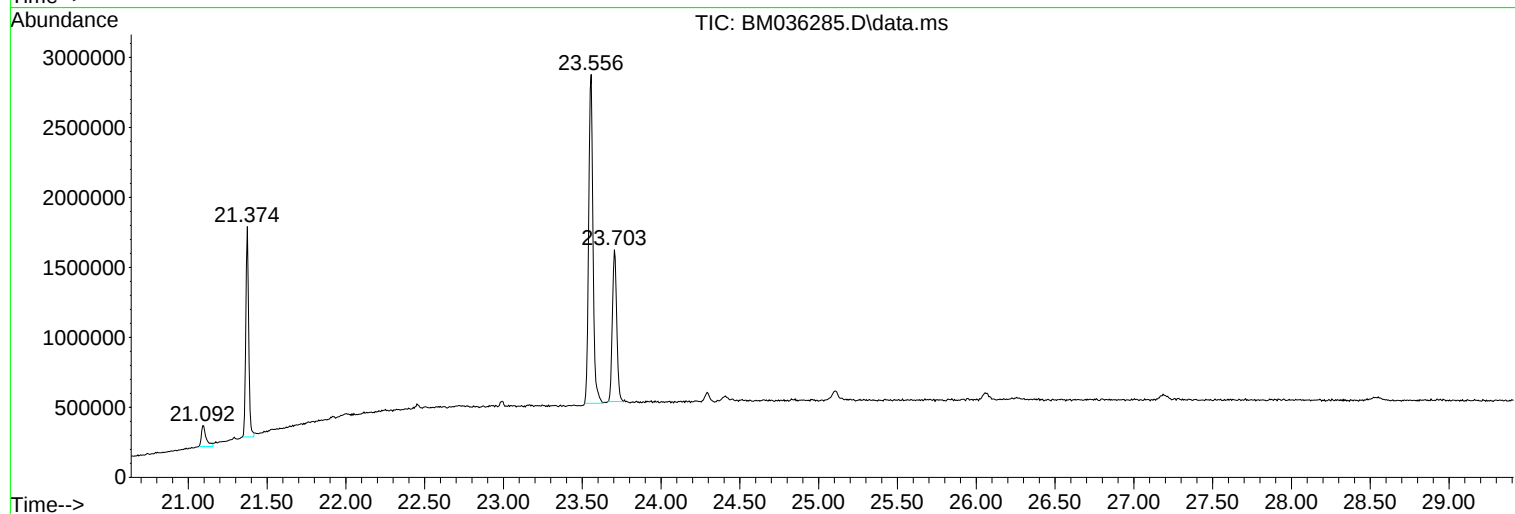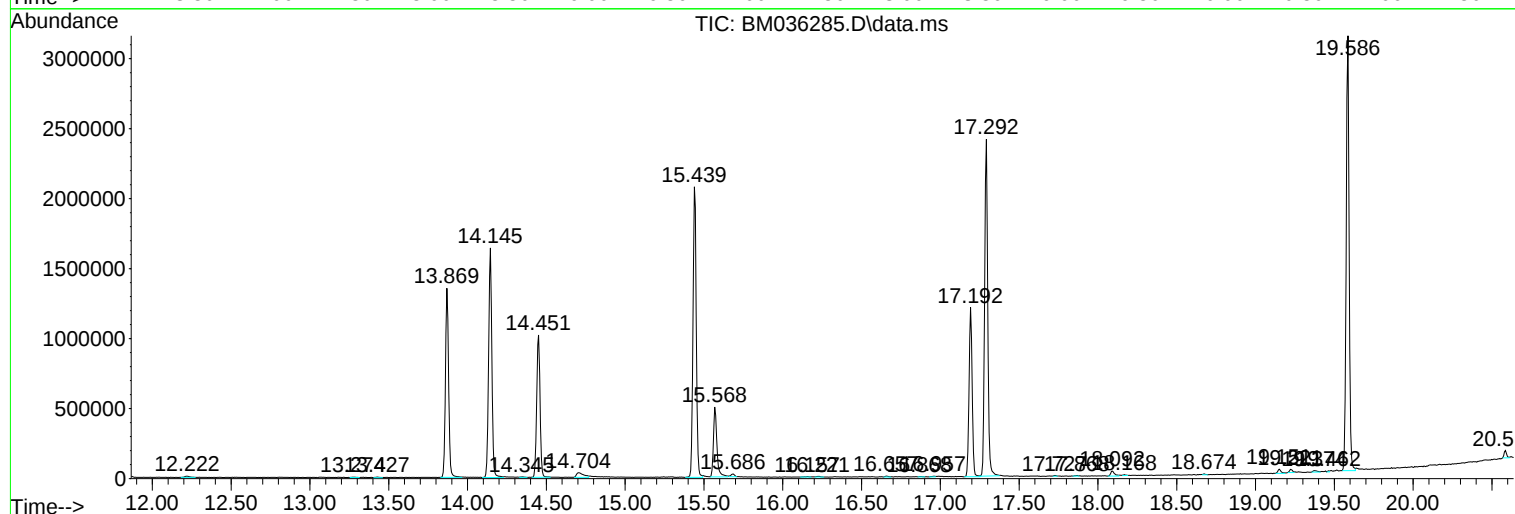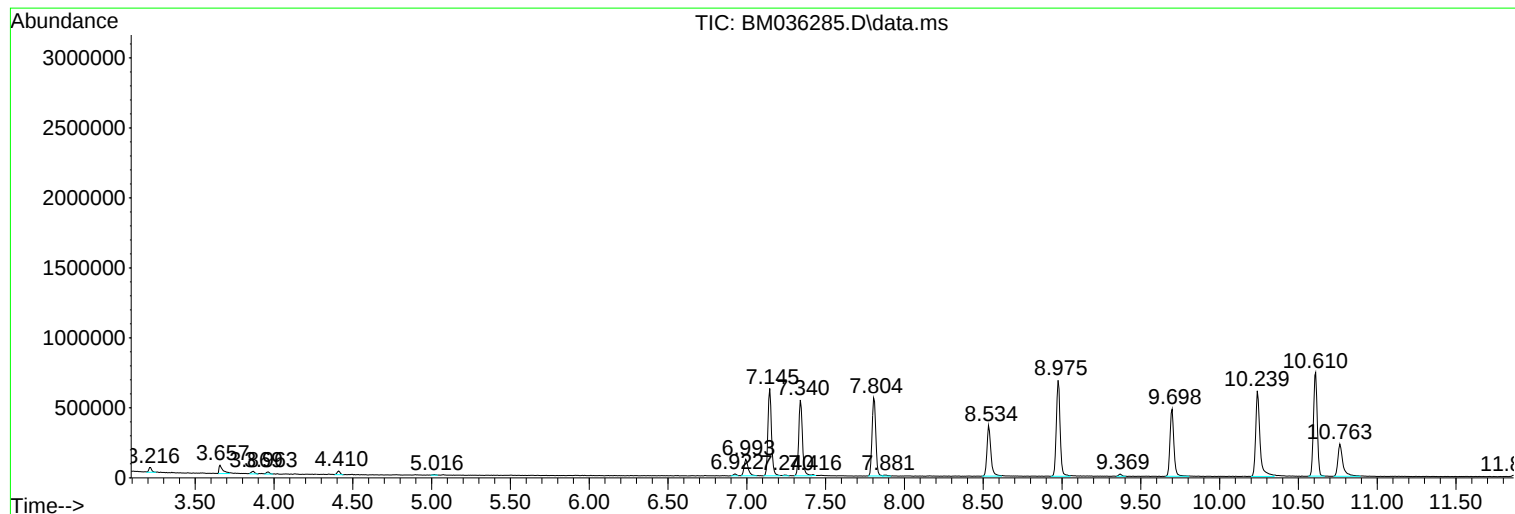

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036285.D
Acq On : 15 Aug 2022 14:08
Operator : CG/JU
Sample : N3951-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COCA6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Heneicosyl formate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	3.32 ng/ul	319837	Chrysene-d12	21.374

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Heneicosyl formate	340	C22H44O2	077899-03-7	91
2			Trichloroacetic acid, tetradecyl...	358	C16H29Cl3O2	074339-52-9	91
3			Cyclopentadecane	210	C15H30	000295-48-7	91
4			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	91
5			1-Hexacosene	364	C26H52	018835-33-1	91

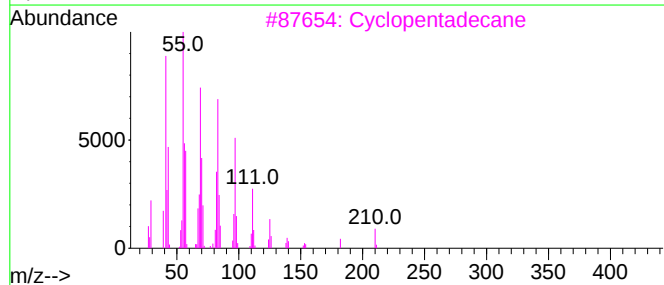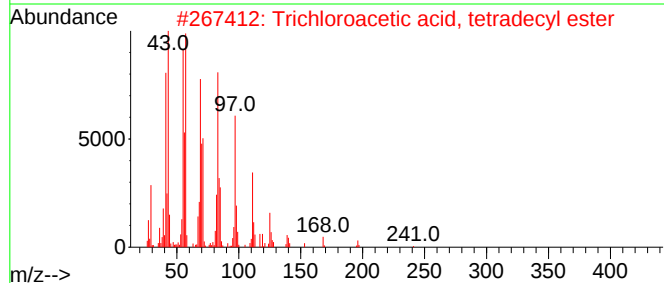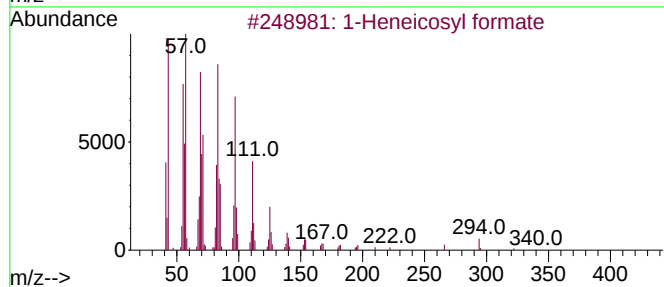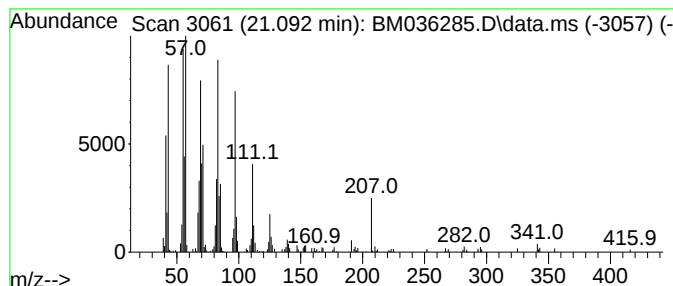

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036285.D
Acq On : 15 Aug 2022 14:08
Operator : CG/JU
Sample : N3951-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Heneicosyl fo...	21.092	3.3	ng/u1	319837	5	21.374	1926930	20.0