

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036287.D
 Acq On : 15 Aug 2022 15:21
 Operator : CG/JU
 Sample : N3951-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	26	rVB	43661	56284	1.26%	0.149%
2	3.652	93	96	108	rBV	98782	162084	3.64%	0.429%
3	3.869	128	133	138	rVB	18109	29807	0.67%	0.079%
4	3.963	146	149	155	rVB	15967	21434	0.48%	0.057%
5	4.410	220	225	230	rVB	30095	42931	0.96%	0.114%
6	5.004	325	326	331	rBV4	5138	6773	0.15%	0.018%
7	6.063	501	506	509	rBV6	3031	5697	0.13%	0.015%
8	6.828	632	636	638	rBV4	3385	4583	0.10%	0.012%
9	6.928	649	653	659	rBV3	12696	17436	0.39%	0.046%
10	6.993	659	664	675	rBV	113315	208288	4.68%	0.552%
11	7.146	683	690	701	rBV	563726	880210	19.77%	2.331%
12	7.240	703	706	712	rVB2	6762	11033	0.25%	0.029%
13	7.340	717	723	733	rBV	506855	827772	18.59%	2.192%
14	7.804	796	802	811	rVV	688012	1090133	24.48%	2.887%
15	8.534	920	926	941	rBV	335226	606709	13.62%	1.607%
16	8.975	994	1001	1016	rBV	628724	1044827	23.46%	2.767%
17	9.139	1026	1029	1034	rBV7	3583	5201	0.12%	0.014%
18	9.369	1063	1068	1073	rVB2	15472	25042	0.56%	0.066%
19	9.698	1116	1124	1138	rBV	457222	789740	17.73%	2.092%
20	10.239	1209	1216	1236	rBV	567150	1078643	24.22%	2.857%
21	10.610	1270	1279	1292	rBV	890007	1514538	34.01%	4.011%
22	10.763	1297	1305	1322	rBV	268443	582793	13.09%	1.543%
23	11.863	1488	1492	1497	rBV2	8422	12264	0.28%	0.032%
24	12.210	1544	1551	1559	rBV4	8297	20630	0.46%	0.055%
25	13.280	1726	1733	1738	rBV8	3122	8394	0.19%	0.022%
26	13.869	1827	1833	1848	rBV	1161938	1636188	36.74%	4.333%
27	14.145	1873	1880	1890	rBV	1444248	2087567	46.88%	5.529%
28	14.345	1910	1914	1918	rVB5	3502	5687	0.13%	0.015%
29	14.451	1923	1932	1939	rBV	1256726	1798330	40.38%	4.763%
30	14.504	1939	1941	1947	rVB7	4825	7939	0.18%	0.021%
31	14.704	1969	1975	1989	rBV4	35275	122565	2.75%	0.325%
32	15.204	2055	2060	2065	rBV2	13046	22315	0.50%	0.059%
33	15.439	2091	2100	2116	rBV	1857145	2682246	60.23%	7.104%
34	15.568	2116	2122	2137	rVV	463155	732018	16.44%	1.939%
35	15.680	2137	2141	2148	rVB2	18991	34082	0.77%	0.090%
36	16.157	2218	2222	2226	rVV7	4566	7263	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036287.D
 Acq On : 15 Aug 2022 15:21
 Operator : CG/JU
 Sample : N3951-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.221	2230	2233	2238	rVB6	6047	11336	0.25%	0.030%
38	16.339	2249	2253	2255	rVB5	3760	4657	0.10%	0.012%
39	16.663	2305	2308	2311	rVB5	7082	8746	0.20%	0.023%
40	16.951	2352	2357	2360	rBV6	6783	10511	0.24%	0.028%
41	17.192	2392	2398	2408	rBV	1508448	2060543	46.27%	5.457%
42	17.292	2408	2415	2429	rVV	2224793	3030663	68.05%	8.026%
43	17.492	2443	2449	2454	rBV8	3601	8041	0.18%	0.021%
44	17.733	2486	2490	2494	rVB7	6165	10698	0.24%	0.028%
45	17.868	2509	2513	2515	rBV5	9520	11802	0.27%	0.031%
46	18.092	2546	2551	2560	rBV3	59957	97286	2.18%	0.258%
47	18.168	2561	2564	2567	rVB2	6783	8533	0.19%	0.023%
48	18.445	2607	2611	2613	rBV5	5500	7781	0.17%	0.021%
49	18.674	2648	2650	2655	rVB6	6756	7656	0.17%	0.020%
50	19.151	2727	2731	2739	rBV5	26585	42978	0.97%	0.114%
51	19.221	2739	2743	2749	rBV2	29318	48464	1.09%	0.128%
52	19.586	2799	2805	2815	rBV	2832085	3725816	83.66%	9.867%
53	20.586	2972	2975	2978	rBV2	58311	63066	1.42%	0.167%
54	21.092	3057	3061	3069	rBV2	301791	516521	11.60%	1.368%
55	21.374	3104	3109	3117	rBV	2060473	2593887	58.25%	6.870%
56	23.556	3473	3480	3492	rBV2	2282122	4453346	100.00%	11.794%
57	23.703	3499	3505	3517	rVB2	1440136	2847500	63.94%	7.541%




Sum of corrected areas: 37759277

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036287.D
Acq On : 15 Aug 2022 15:21
Operator : CG/JU
Sample : N3951-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

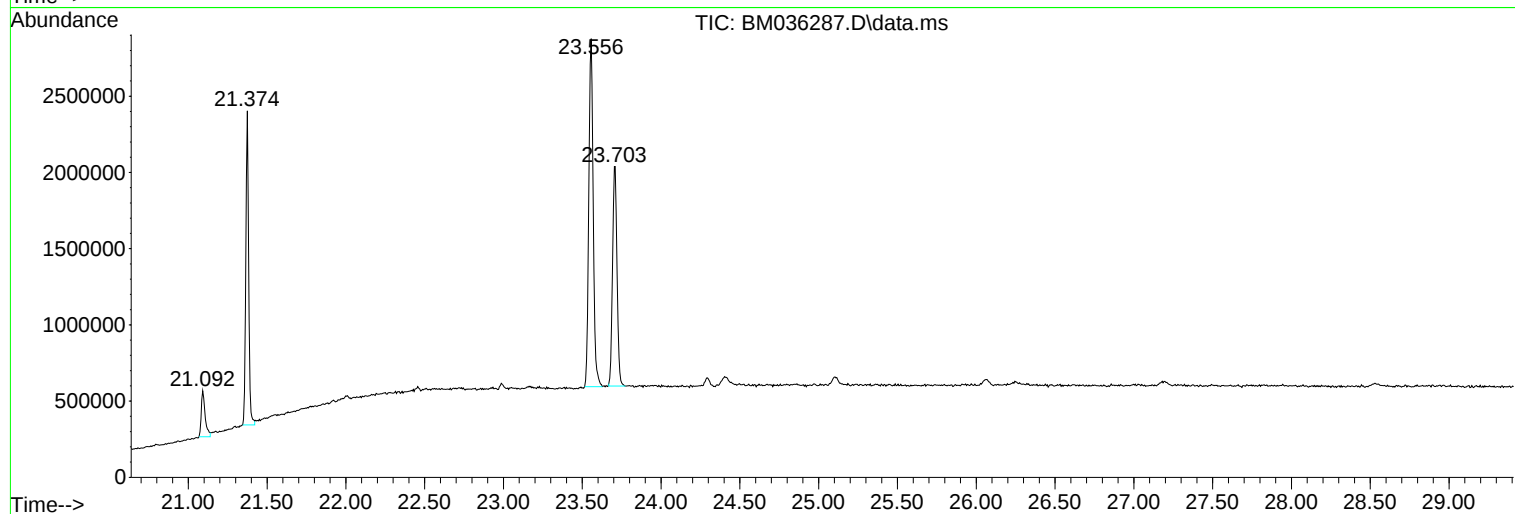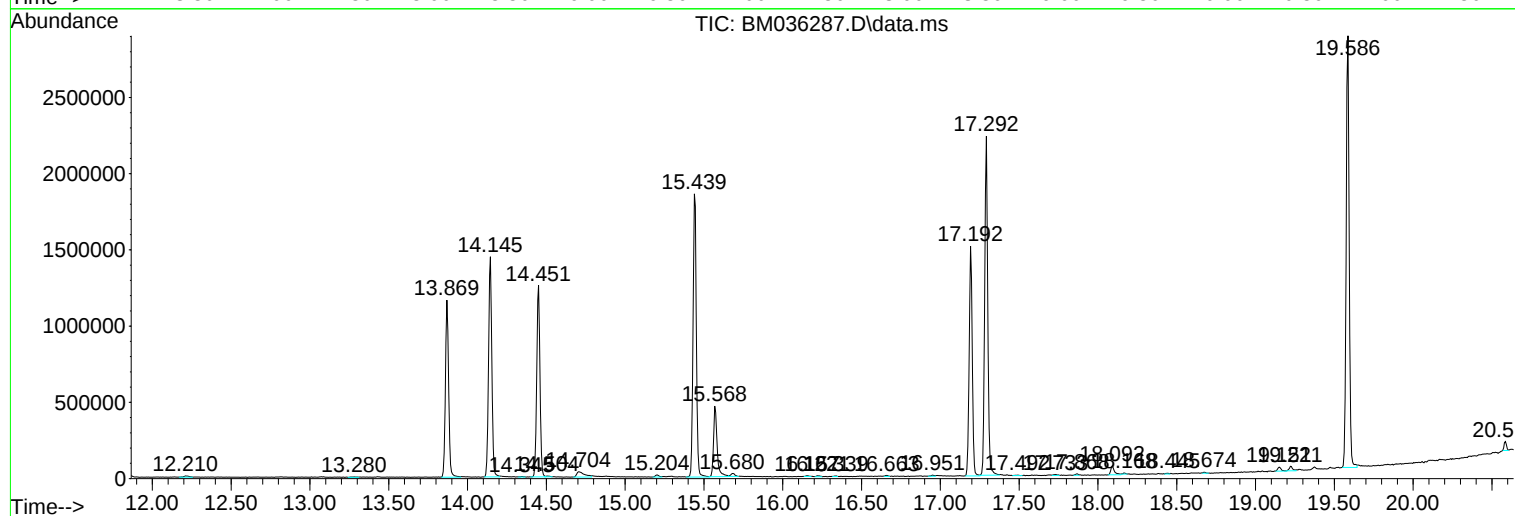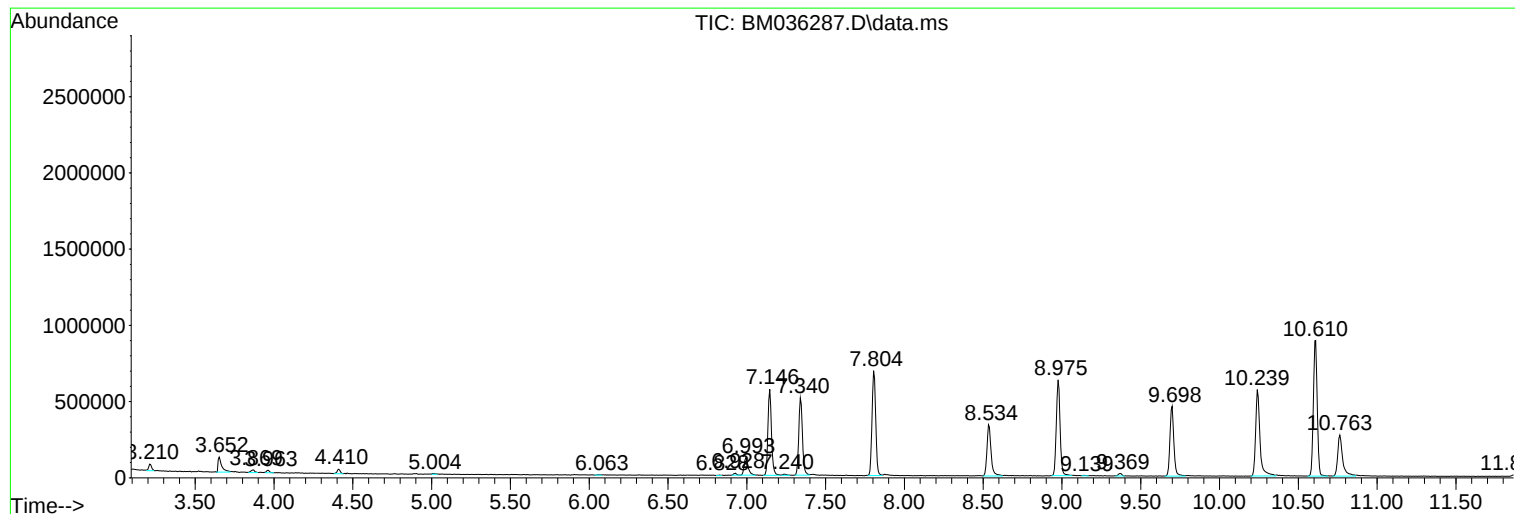

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036287.D
Acq On : 15 Aug 2022 15:21
Operator : CG/JU
Sample : N3951-07
Misc :
ALS Vial : 11 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
C0CF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.092	3.98 ng/ul	516521	Chrysene-d12	21.374	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentacos-1-ene	350	C25H50	016980-85-1	94
2	5-Octadecene, (E)-	252	C18H36	007206-21-5	93
3	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	93
4	Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	93
5	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	93

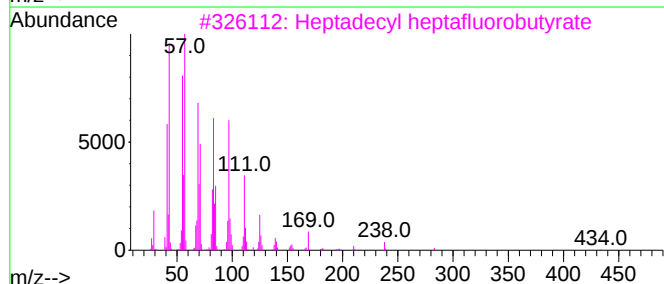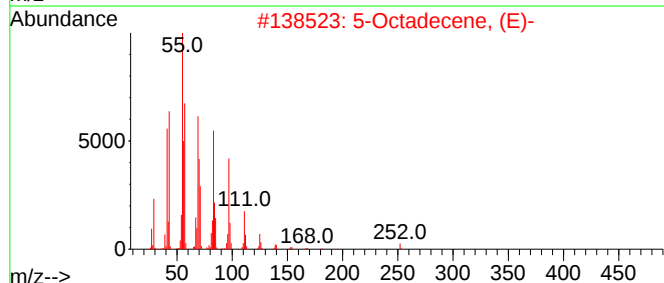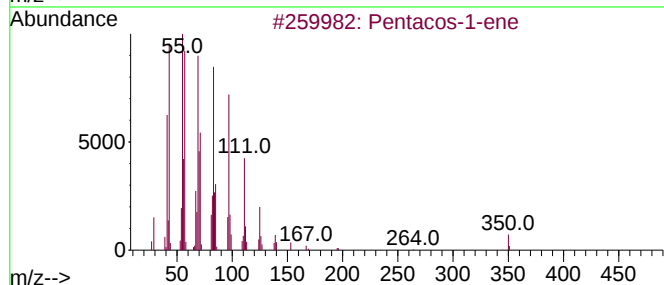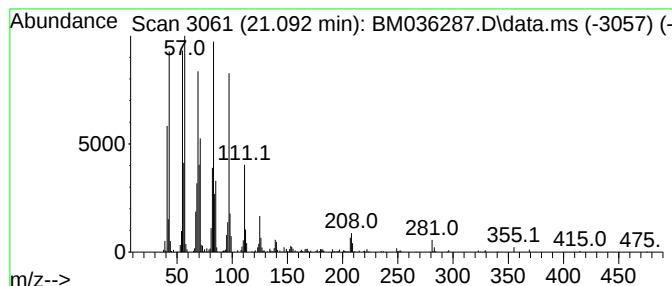

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036287.D
Acq On : 15 Aug 2022 15:21
Operator : CG/JU
Sample : N3951-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.092	4.0	ng/u1	516521	5	21.374	2593890	20.0