

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036288.D
 Acq On : 15 Aug 2022 15:58
 Operator : CG/JU
 Sample : N3951-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	18	22	28	rVB	42841	53442	0.92%	0.114%
2	3.646	93	95	115	rBV	179862	292190	5.01%	0.624%
3	3.863	130	132	137	rVB	18710	22762	0.39%	0.049%
4	3.963	145	149	156	rVB	17616	29034	0.50%	0.062%
5	4.410	221	225	232	rVB	33263	49231	0.84%	0.105%
6	6.922	648	652	658	rVB2	15409	20945	0.36%	0.045%
7	6.992	658	664	675	rBV	148168	251424	4.31%	0.537%
8	7.145	683	690	702	rBV	711828	1113612	19.10%	2.377%
9	7.340	716	723	733	rBV	633677	1006704	17.27%	2.148%
10	7.804	795	802	811	rBV	684614	1077964	18.49%	2.300%
11	7.875	812	814	819	rVB5	6456	9342	0.16%	0.020%
12	8.534	920	926	936	rBV	438254	747265	12.82%	1.595%
13	8.975	994	1001	1015	rBV	810454	1346537	23.10%	2.874%
14	9.369	1063	1068	1073	rVB	17839	25834	0.44%	0.055%
15	9.698	1116	1124	1142	rBV	591717	1010723	17.34%	2.157%
16	10.239	1209	1216	1239	rBV	748521	1404985	24.10%	2.998%
17	10.604	1271	1278	1286	rBV	923444	1552756	26.64%	3.314%
18	10.763	1296	1305	1324	rBV	366406	767996	13.18%	1.639%
19	11.863	1487	1492	1498	rVB3	12314	18486	0.32%	0.039%
20	12.216	1545	1552	1558	rBV3	11208	24471	0.42%	0.052%
21	13.869	1824	1833	1846	rBV	1680446	2328637	39.95%	4.969%
22	14.145	1873	1880	1895	rBV	1989884	2894803	49.66%	6.178%
23	14.339	1909	1913	1917	rBV6	5489	9379	0.16%	0.020%
24	14.451	1925	1932	1943	rBV	1372763	1989258	34.13%	4.245%
25	14.698	1968	1974	1992	rBV	56369	182639	3.13%	0.390%
26	15.292	2071	2075	2079	rVB7	6422	9631	0.17%	0.021%
27	15.439	2090	2100	2113	rBV	2541169	3704409	63.55%	7.905%
28	15.568	2116	2122	2136	rVV	709012	1054800	18.10%	2.251%
29	15.686	2137	2142	2150	rVB2	26564	47821	0.82%	0.102%
30	16.157	2219	2222	2229	rVB6	7578	12359	0.21%	0.026%
31	16.227	2229	2234	2239	rVB8	8057	14885	0.26%	0.032%
32	16.333	2247	2252	2256	rBV7	3653	7879	0.14%	0.017%
33	16.657	2303	2307	2313	rVB4	9318	14896	0.26%	0.032%
34	16.951	2353	2357	2361	rBV6	8393	16519	0.28%	0.035%
35	17.192	2392	2398	2405	rBV	1661836	2301800	39.49%	4.912%
36	17.292	2408	2415	2428	rVV	3068792	4236159	72.67%	9.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036288.D
 Acq On : 15 Aug 2022 15:58
 Operator : CG/JU
 Sample : N3951-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	17.604	2465	2468	2473	rBV6	4465	6512	0.11%	0.014%
38	17.727	2486	2489	2492	rBV3	7916	9720	0.17%	0.021%
39	17.868	2508	2513	2518	rBV8	7897	13352	0.23%	0.028%
40	18.092	2547	2551	2556	rBV5	20397	34803	0.60%	0.074%
41	18.168	2560	2564	2567	rVV2	6583	8947	0.15%	0.019%
42	18.668	2647	2649	2654	rVB6	7295	8673	0.15%	0.019%
43	19.151	2727	2731	2737	rBV2	34540	51879	0.89%	0.111%
44	19.221	2740	2743	2748	rBV	34068	47586	0.82%	0.102%
45	19.586	2799	2805	2813	rBV	3875044	5149145	88.34%	10.989%
46	20.586	2971	2975	2979	rBV	113570	126602	2.17%	0.270%
47	21.092	3058	3061	3068	rBV4	79051	122584	2.10%	0.262%
48	21.374	3104	3109	3117	rBV	2231977	2807870	48.17%	5.992%
49	23.556	3473	3480	3492	rBV2	3161070	5828986	100.00%	12.439%
50	23.703	3499	3505	3518	rVB2	1510484	2990532	51.30%	6.382%




Sum of corrected areas: 46858768

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036288.D
Acq On : 15 Aug 2022 15:58
Operator : CG/JU
Sample : N3951-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

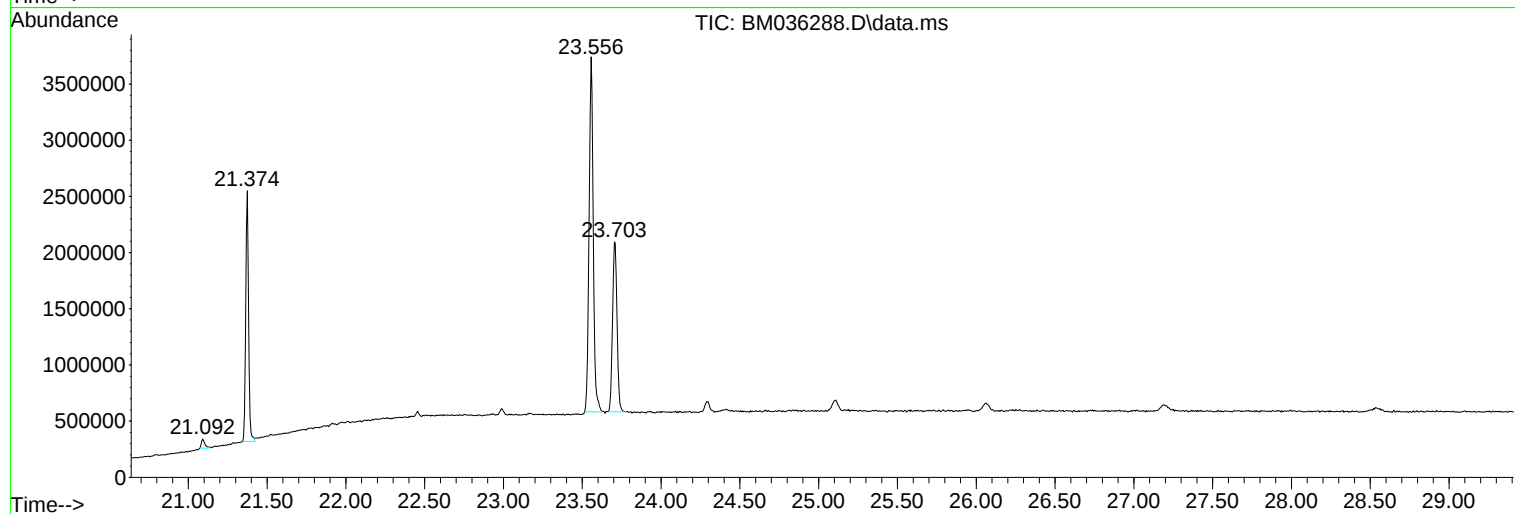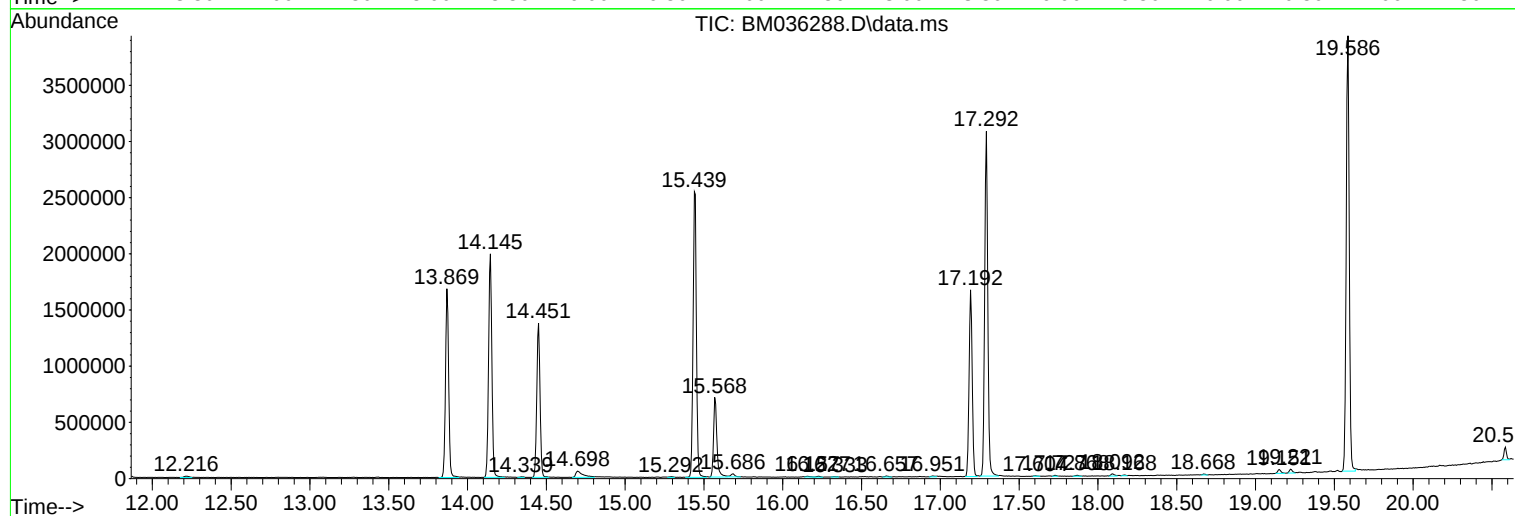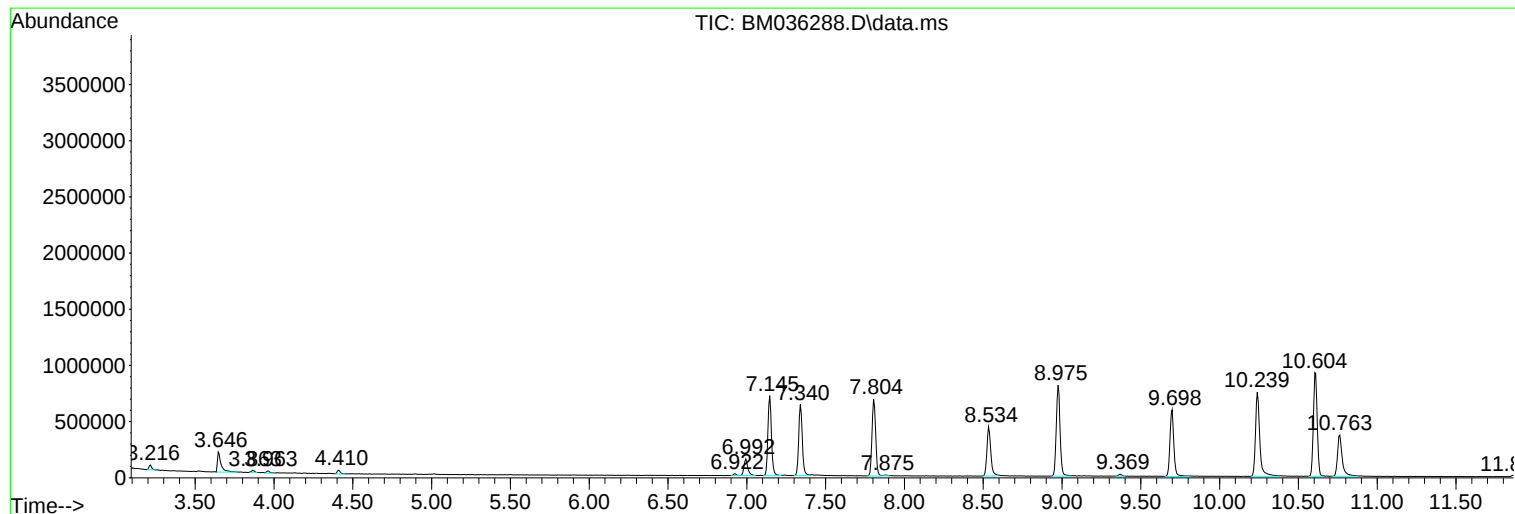

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036288.D
Acq On : 15 Aug 2022 15:58
Operator : CG/JU
Sample : N3951-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036288.D
Acq On : 15 Aug 2022 15:58
Operator : CG/JU
Sample : N3951-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc