

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036289.D
 Acq On : 15 Aug 2022 16:35
 Operator : CG/JU
 Sample : N4065-01DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.663	97	98	108	rBV	26662	49643	1.92%	0.222%
2	3.963	145	149	153	rVB2	17237	23663	0.92%	0.106%
3	4.199	185	189	195	rBV	45701	61343	2.37%	0.274%
4	4.410	221	225	231	rVB3	10194	15968	0.62%	0.071%
5	4.616	256	260	265	rBV	28681	38222	1.48%	0.171%
6	7.004	660	666	672	rBV	22564	45500	1.76%	0.203%
7	7.145	683	690	703	rBV	97885	172399	6.67%	0.770%
8	7.345	717	724	734	rBV	82402	154734	5.99%	0.691%
9	7.804	795	802	812	rBV	616463	1002859	38.82%	4.481%
10	8.545	922	928	936	rBV	58002	116954	4.53%	0.523%
11	8.981	996	1002	1009	rBV	104729	186971	7.24%	0.835%
12	9.275	1046	1052	1056	rBV6	6954	12615	0.49%	0.056%
13	9.698	1118	1124	1135	rBV	64315	131343	5.08%	0.587%
14	10.022	1172	1179	1188	rBV	12520	34629	1.34%	0.155%
15	10.251	1207	1218	1227	rBV	83712	182923	7.08%	0.817%
16	10.610	1270	1279	1293	rVV	801489	1378681	53.36%	6.160%
17	10.769	1300	1306	1319	rVV	78952	204298	7.91%	0.913%
18	10.898	1325	1328	1337	rVB7	6777	12354	0.48%	0.055%
19	11.210	1375	1381	1391	rVB2	25397	50627	1.96%	0.226%
20	11.657	1447	1457	1463	rBV6	11640	30128	1.17%	0.135%
21	11.727	1463	1469	1473	rVV	27243	50566	1.96%	0.226%
22	11.933	1497	1504	1508	rBV8	4910	11435	0.44%	0.051%
23	12.027	1515	1520	1528	rBV3	18302	28465	1.10%	0.127%
24	12.163	1535	1543	1548	rBV5	25126	56616	2.19%	0.253%
25	12.333	1567	1572	1576	rBV5	8732	12846	0.50%	0.057%
26	12.445	1587	1591	1610	rVB10	26321	85179	3.30%	0.381%
27	12.633	1614	1623	1626	rBV7	22164	42914	1.66%	0.192%
28	12.669	1626	1629	1631	rVV4	10051	12435	0.48%	0.056%
29	12.704	1631	1635	1643	rVB8	10115	21171	0.82%	0.095%
30	12.804	1643	1652	1656	rBV9	10841	21733	0.84%	0.097%
31	12.880	1661	1665	1672	rVB6	7995	15356	0.59%	0.069%
32	12.974	1672	1681	1686	rBV6	15095	28688	1.11%	0.128%
33	13.274	1722	1732	1736	rBV8	18367	50545	1.96%	0.226%
34	13.510	1767	1772	1777	rVB3	61694	98701	3.82%	0.441%
35	13.604	1782	1788	1789	rBV5	13051	19151	0.74%	0.086%
36	13.645	1790	1795	1800	rVB4	19167	42629	1.65%	0.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036289.D
 Acq On : 15 Aug 2022 16:35
 Operator : CG/JU
 Sample : N4065-01DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	13.786	1813	1819	1827	rBV8	17906	46759	1.81%	0.209%
38	13.869	1827	1833	1840	rBV	230321	336742	13.03%	1.505%
39	14.004	1851	1856	1859	rBV	41313	58424	2.26%	0.261%
40	14.039	1859	1862	1870	rVB	36391	56786	2.20%	0.254%

41	14.145	1874	1880	1883	rBV	264654	401015	15.52%	1.792%
42	14.174	1883	1885	1893	rVB3	88655	133581	5.17%	0.597%
43	14.257	1895	1899	1903	rBV5	16759	27625	1.07%	0.123%
44	14.451	1925	1932	1937	rBV	1127689	1596683	61.80%	7.134%
45	14.516	1937	1943	1951	rVV	1775129	2583516	100.00%	11.543%

46	14.598	1951	1957	1962	rVB3	12301	25856	1.00%	0.116%
47	14.757	1974	1984	1990	rBV	44789	94952	3.68%	0.424%
48	14.851	1996	2000	2006	rVB2	20084	30383	1.18%	0.136%
49	14.927	2010	2013	2017	rVV6	9346	13651	0.53%	0.061%
50	15.068	2031	2037	2045	rBV6	20590	44618	1.73%	0.199%

51	15.327	2076	2081	2087	rVB2	23629	40405	1.56%	0.181%
52	15.439	2090	2100	2105	rBV	380489	542870	21.01%	2.425%
53	15.498	2105	2110	2119	rVB	566624	804202	31.13%	3.593%
54	15.580	2119	2124	2128	rBV3	61957	124477	4.82%	0.556%
55	15.621	2128	2131	2134	rVB2	40460	47873	1.85%	0.214%

56	15.704	2142	2145	2149	rVB4	27253	38070	1.47%	0.170%
57	15.745	2150	2152	2157	rVB5	12266	16478	0.64%	0.074%
58	15.810	2159	2163	2169	rVB7	24039	44223	1.71%	0.198%
59	15.898	2172	2178	2180	rBV4	14924	25679	0.99%	0.115%
60	15.939	2180	2185	2194	rVB2	71957	153960	5.96%	0.688%

61	16.021	2194	2199	2204	rVB2	12956	26907	1.04%	0.120%
62	16.174	2220	2225	2236	rVB5	56268	114771	4.44%	0.513%
63	16.292	2240	2245	2252	rBV	45129	66119	2.56%	0.295%
64	16.368	2253	2258	2264	rBV4	34464	59311	2.30%	0.265%
65	16.462	2269	2274	2275	rBV5	13206	20910	0.81%	0.093%

66	16.498	2277	2280	2285	rVB3	30493	44326	1.72%	0.198%
67	16.551	2285	2289	2295	rBV6	11907	22142	0.86%	0.099%
68	16.651	2302	2306	2310	rVB3	18500	24999	0.97%	0.112%
69	16.733	2316	2320	2323	rBV6	10436	15444	0.60%	0.069%
70	16.839	2333	2338	2347	rVB8	21785	58762	2.27%	0.263%

71	16.986	2359	2363	2364	rBV	18248	20435	0.79%	0.091%
72	17.121	2379	2386	2389	rBV4	22015	41412	1.60%	0.185%
73	17.192	2389	2398	2403	rBV	1344530	1854716	71.79%	8.287%
74	17.233	2403	2405	2409	rVB2	29108	32761	1.27%	0.146%
75	17.292	2409	2415	2419	rBV	377407	563675	21.82%	2.518%

76	17.392	2429	2432	2437	rVB3	24494	35681	1.38%	0.159%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036289.D
 Acq On : 15 Aug 2022 16:35
 Operator : CG/JU
 Sample : N4065-01DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	17.574	2458	2463	2466	rBV	38382	58487	2.26%	0.261%
78	17.692	2479	2483	2484	rBV4	12086	15165	0.59%	0.068%
79	17.862	2508	2512	2516	rVB6	24355	38623	1.49%	0.173%
80	17.909	2517	2520	2524	rBV4	14502	17303	0.67%	0.077%
81	17.962	2524	2529	2532	rVV7	14055	23506	0.91%	0.105%
82	18.039	2538	2542	2546	rBV2	44995	64670	2.50%	0.289%
83	18.092	2548	2551	2552	rVV3	18755	20577	0.80%	0.092%
84	18.121	2552	2556	2560	rVB2	48069	70690	2.74%	0.316%
85	18.198	2565	2569	2575	rVB2	63328	92872	3.59%	0.415%
86	18.268	2575	2581	2590	rVB	112214	172544	6.68%	0.771%
87	18.356	2591	2596	2599	rBV2	25482	48131	1.86%	0.215%
88	18.462	2611	2614	2619	rVB5	15499	18500	0.72%	0.083%
89	18.515	2619	2623	2630	rBV3	26890	52285	2.02%	0.234%
90	18.574	2630	2633	2637	rBV3	18831	28909	1.12%	0.129%
91	18.621	2637	2641	2647	rBV5	20216	39861	1.54%	0.178%
92	18.792	2666	2670	2672	rBV5	11151	18384	0.71%	0.082%
93	19.251	2744	2748	2754	rVB	255624	331496	12.83%	1.481%
94	19.586	2799	2805	2808	rBV	563942	774048	29.96%	3.458%
95	19.998	2871	2875	2883	rBV	64130	107506	4.16%	0.480%
96	20.586	2972	2975	2979	rBV	64218	65923	2.55%	0.295%
97	20.709	2993	2996	3006	rBV2	71282	113612	4.40%	0.508%
98	21.374	3104	3109	3114	rBV	1837171	2342051	90.65%	10.464%
99	23.550	3475	3479	3485	rBV2	355251	603268	23.35%	2.695%
100	23.703	3499	3505	3515	rVB2	1273386	2468060	95.53%	11.027%




Sum of corrected areas: 22381954

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036289.D
Acq On : 15 Aug 2022 16:35
Operator : CG/JU
Sample : N4065-01DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

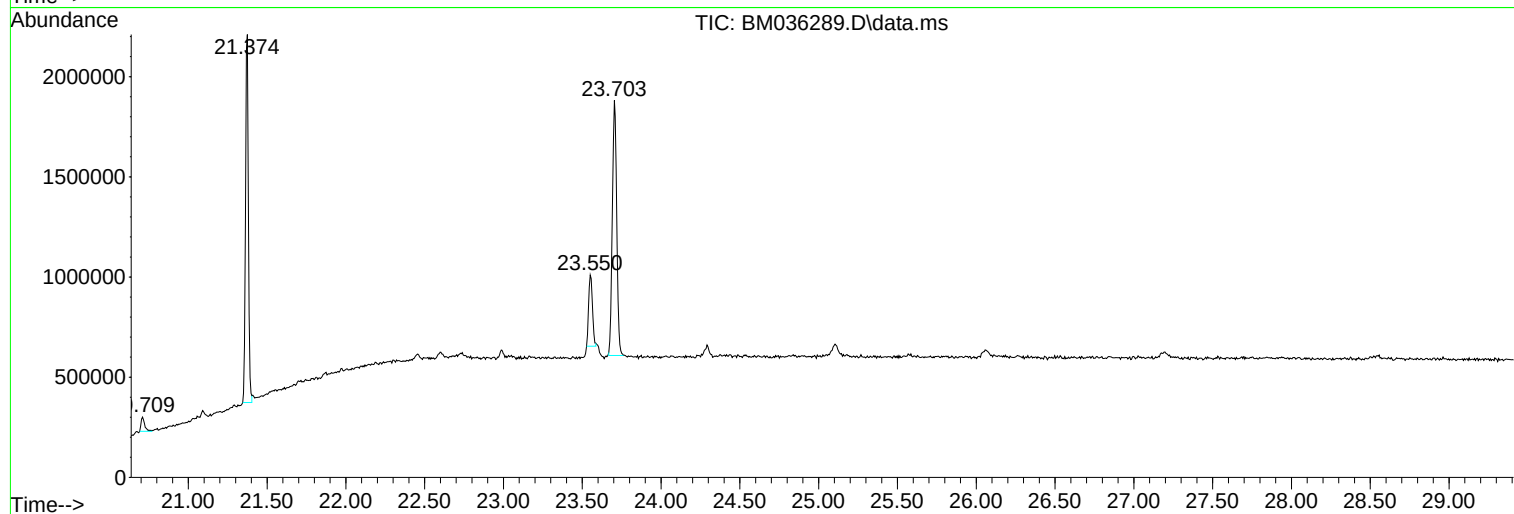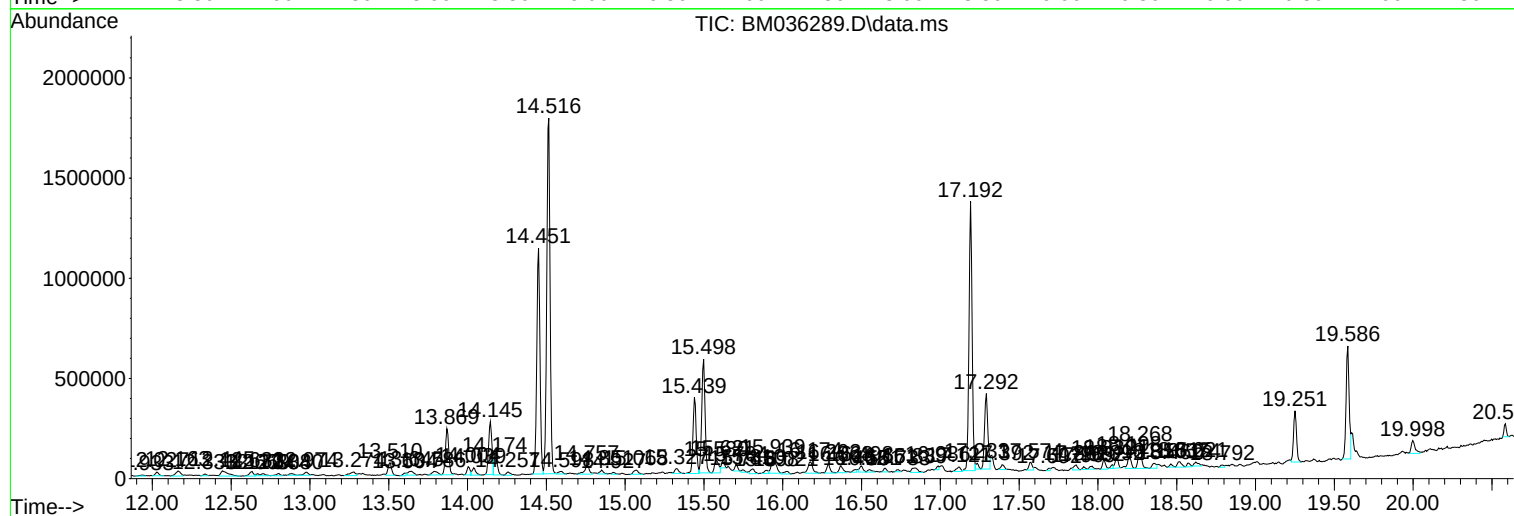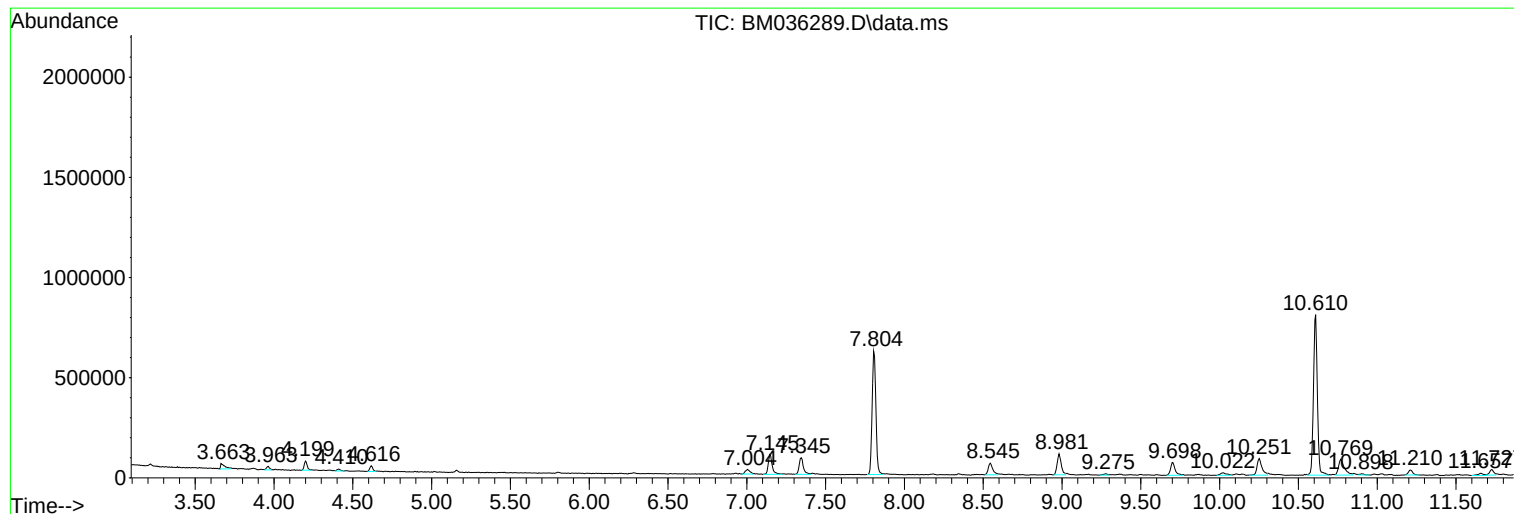

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036289.D
Acq On : 15 Aug 2022 16:35
Operator : CG/JU
Sample : N4065-01DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036289.D
Acq On : 15 Aug 2022 16:35
Operator : CG/JU
Sample : N4065-01DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc