

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
 Data File : BM036291.D
 Acq On : 15 Aug 2022 17:55
 Operator : CG/JU
 Sample : PB147022BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	30	rVB	72091	94162	2.06%	0.194%
2	3.640	90	94	114	rBV	801247	1210213	26.41%	2.492%
3	6.992	657	664	680	rBV	819931	1376758	30.05%	2.835%
4	7.145	683	690	705	rVB	738131	1153979	25.19%	2.377%
5	7.339	716	723	739	rBV	917252	1442816	31.49%	2.971%
6	7.804	796	802	816	rVB	726361	1131135	24.69%	2.329%
7	8.534	918	926	941	rBV	1008082	1682010	36.71%	3.464%
8	8.975	994	1001	1012	rBV	849060	1373912	29.99%	2.829%
9	9.692	1117	1123	1136	rBV	630360	1077034	23.51%	2.218%
10	10.239	1208	1216	1238	rBV	882701	1575919	34.40%	3.245%
11	10.604	1271	1278	1287	rBV	970782	1616337	35.28%	3.329%
12	10.757	1297	1304	1327	rBV	913418	1742609	38.03%	3.589%
13	12.222	1547	1553	1563	rBV4	11754	27332	0.60%	0.056%
14	13.421	1754	1757	1762	rBV6	3080	5656	0.12%	0.012%
15	13.868	1827	1833	1846	rBV	1667561	2247724	49.06%	4.629%
16	14.145	1873	1880	1892	rBV	1998314	2838613	61.96%	5.846%
17	14.451	1924	1932	1942	rBV	1374934	2025286	44.20%	4.171%
18	14.680	1965	1971	1994	rBV	500589	1061361	23.17%	2.186%
19	15.439	2094	2100	2114	rVB	2415899	3474282	75.83%	7.155%
20	15.568	2117	2122	2137	rBV	627224	968525	21.14%	1.995%
21	15.680	2137	2141	2148	rVB	30743	48520	1.06%	0.100%
22	16.009	2192	2197	2200	rBV7	3712	6295	0.14%	0.013%
23	16.227	2230	2234	2239	rVB6	9043	13372	0.29%	0.028%
24	16.868	2341	2343	2349	rVB6	4834	6005	0.13%	0.012%
25	16.962	2355	2359	2360	rBV5	3243	4785	0.10%	0.010%
26	16.980	2360	2362	2367	rVB6	4760	6384	0.14%	0.013%
27	17.192	2391	2398	2408	rBV	1696968	2314711	50.52%	4.767%
28	17.292	2408	2415	2428	rVV	2678231	3722239	81.24%	7.666%
29	19.150	2727	2731	2735	rBV4	30647	41371	0.90%	0.085%
30	19.221	2740	2743	2747	rVV	24794	31452	0.69%	0.065%
31	19.586	2799	2805	2815	rBV	3153791	4308847	94.05%	8.874%
32	20.586	2972	2975	2980	rBV	51463	55979	1.22%	0.115%
33	21.374	3104	3109	3119	rBV	1970304	2578204	56.27%	5.310%
34	23.556	3473	3480	3494	rVB	2397965	4581626	100.00%	9.436%
35	23.703	3499	3505	3518	rVB2	1326359	2711655	59.19%	5.584%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036291.D
Acq On : 15 Aug 2022 17:55
Operator : CG/JU
Sample : PB147022BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK022

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 48557108

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036291.D
Acq On : 15 Aug 2022 17:55
Operator : CG/JU
Sample : PB147022BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

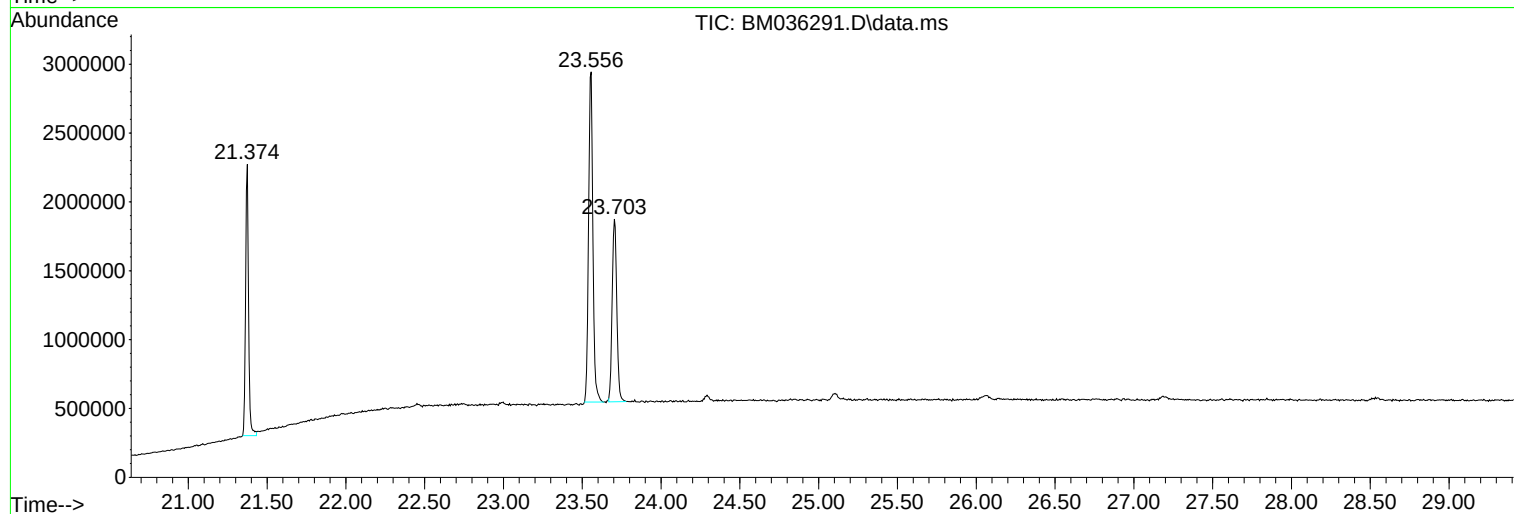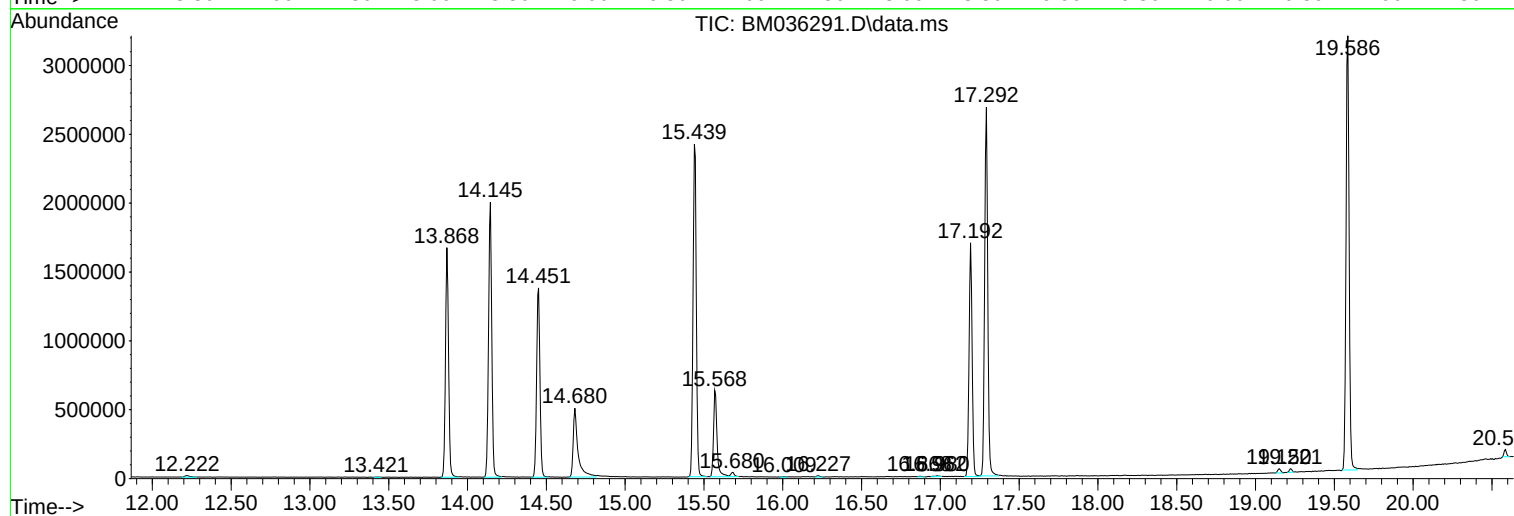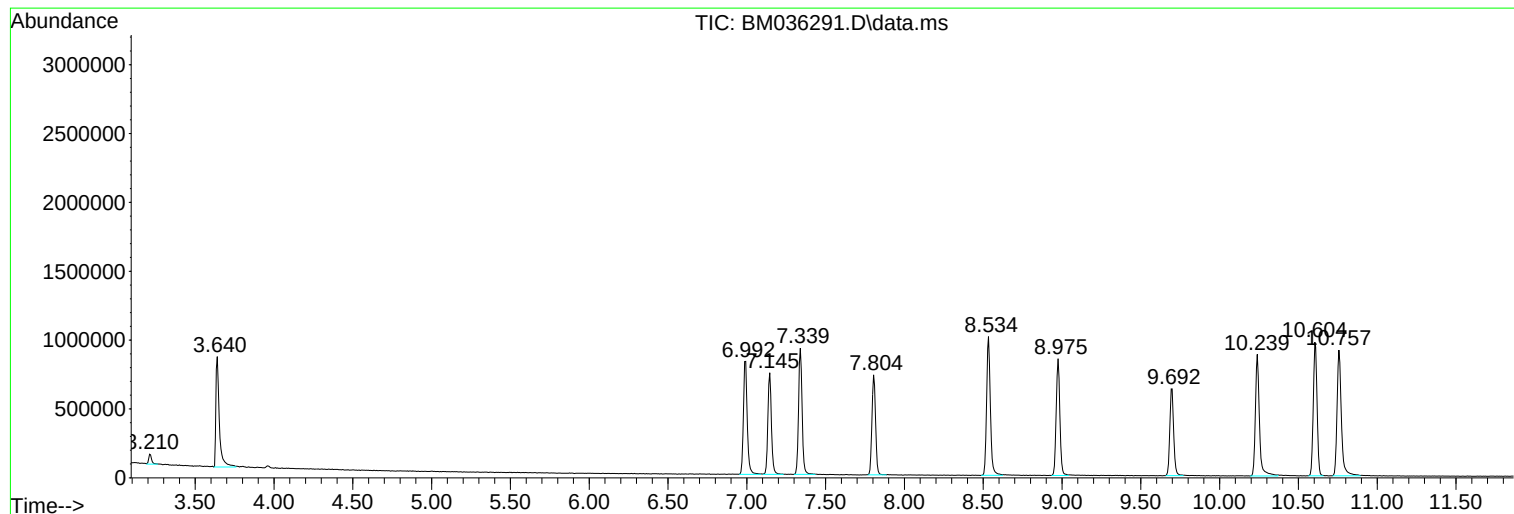

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036291.D
Acq On : 15 Aug 2022 17:55
Operator : CG/JU
Sample : PB147022BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081522\
Data File : BM036291.D
Acq On : 15 Aug 2022 17:55
Operator : CG/JU
Sample : PB147022BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc