
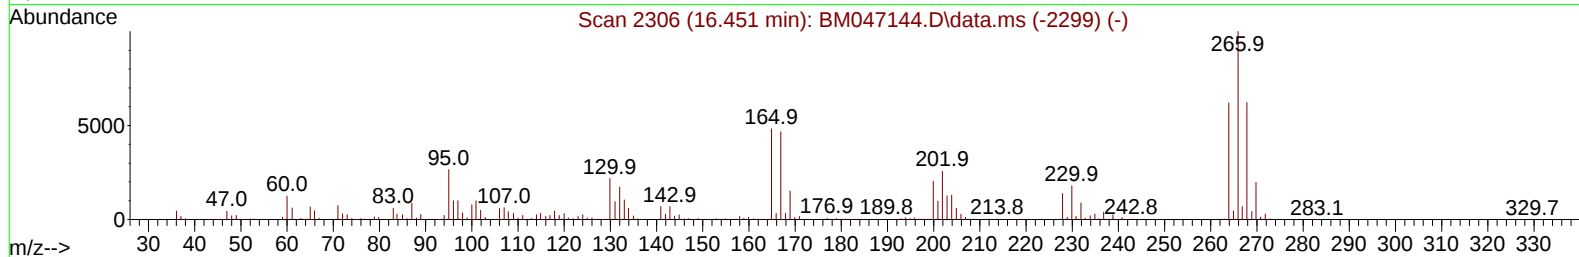
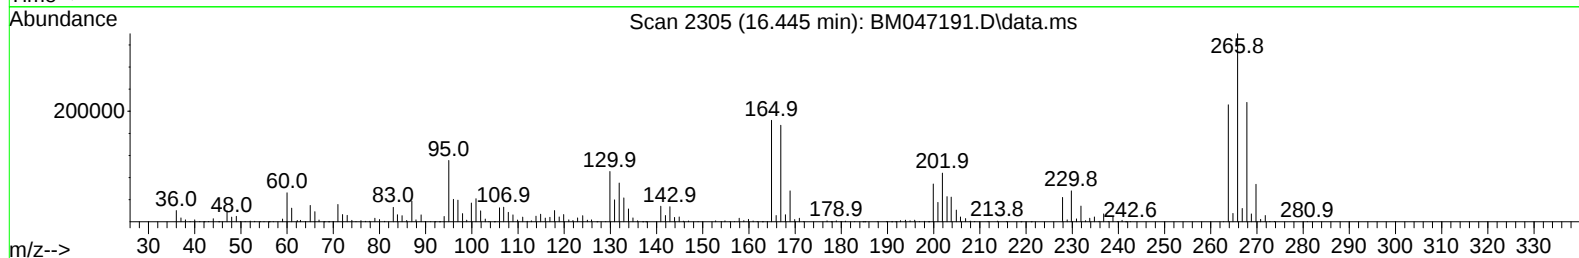


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047191.D
Acq On : 14 Aug 2024 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 17:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

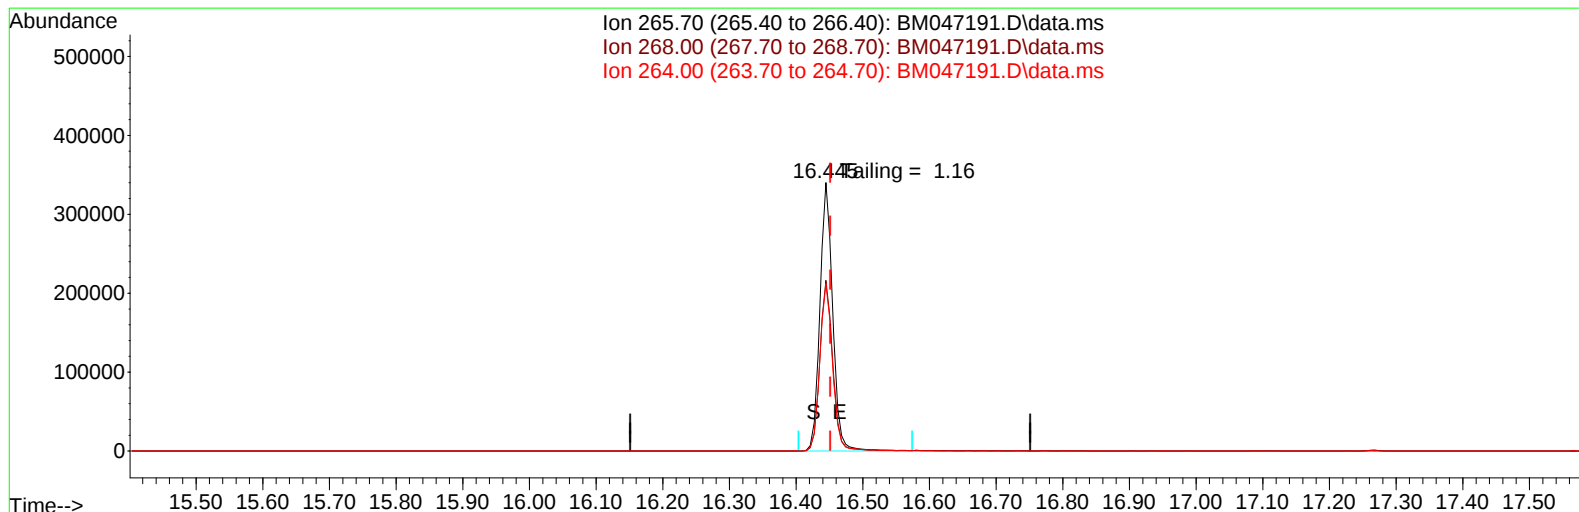

TIC: BM047191.D\data.ms

(70) Pentachlorophenol (C)




16.445min (-0.006) 414349.63 ng

response 455878

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.54
264.00	62.00	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047191.D
Acq On : 14 Aug 2024 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 17:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

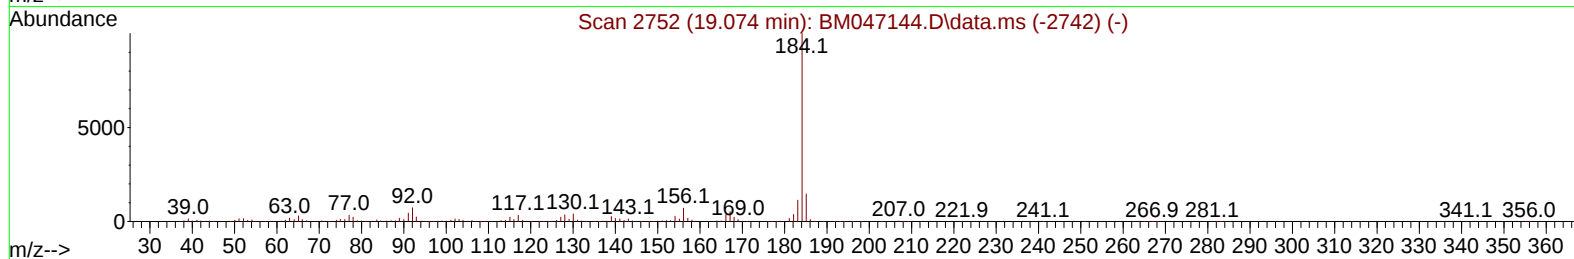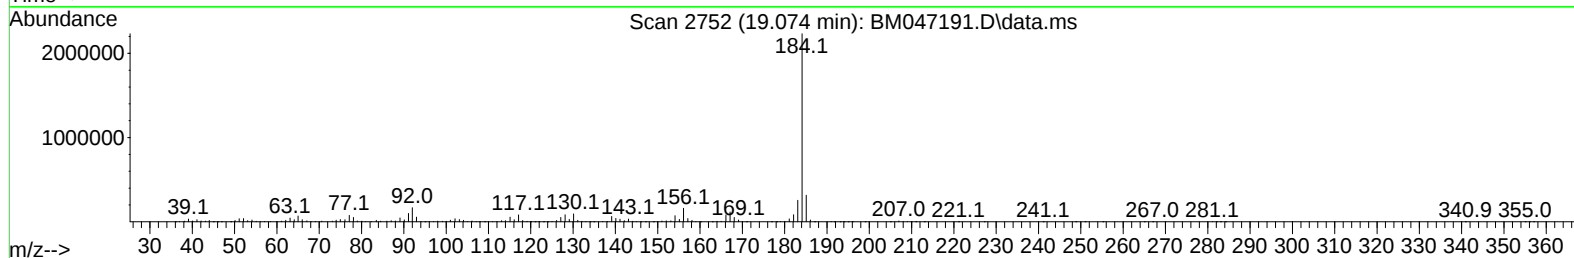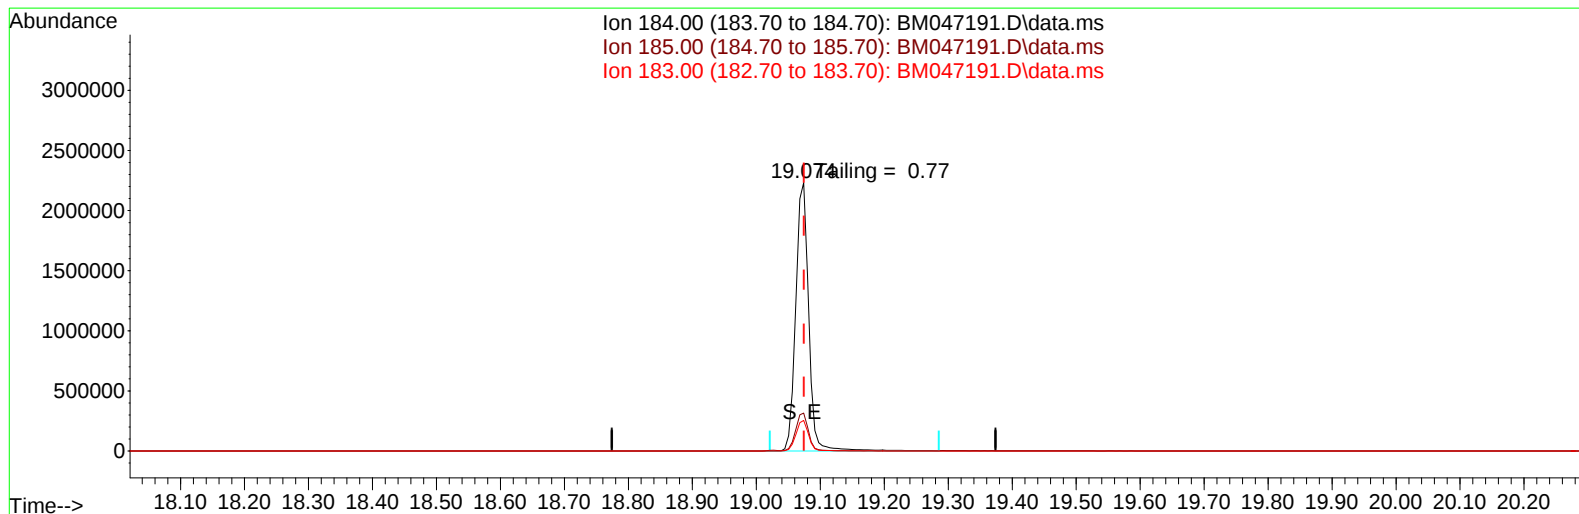

TIC: BM047191.D\data.ms

(77) Benzidine**19.074min (-0.000) 112139.60 ng****response 3139731**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.13
183.00	11.30	11.39
0.00	0.00	0.00