

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047194.D
 Acq On : 14 Aug 2024 16:50
 Operator : RC/JU
 Sample : P3519-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-16-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	61	64	72	rBV	248955	339023	2.58%	0.341%
2	4.575	280	287	297	rBV	539641	716295	5.45%	0.720%
3	5.022	356	363	376	rBV	3480587	5046011	38.38%	5.069%
4	6.581	618	628	642	rBV	3405582	5462046	41.54%	5.487%
5	7.369	754	762	772	rBV	1025112	1562888	11.89%	1.570%
6	8.516	947	957	965	rBV	2178510	3626040	27.58%	3.643%
7	10.122	1217	1230	1241	rBV	1332261	2174359	16.54%	2.184%
8	10.886	1353	1360	1371	rBV	196784	414106	3.15%	0.416%
9	12.633	1649	1657	1672	rBV	4222527	6113185	46.50%	6.141%
10	13.739	1835	1845	1851	rBV4	68065	155795	1.18%	0.157%
11	14.022	1887	1893	1902	rBV	1939747	2787665	21.20%	2.800%
12	14.263	1928	1934	1935	rBV	215676	264654	2.01%	0.266%
13	14.280	1935	1937	1946	rVB2	265049	416000	3.16%	0.418%
14	15.533	2143	2150	2162	rBV	4070738	5897169	44.85%	5.924%
15	16.786	2358	2363	2367	rBV	2432852	3277517	24.93%	3.292%
16	16.827	2367	2370	2374	rVB	300828	372386	2.83%	0.374%
17	16.916	2381	2385	2393	rVB2	152066	209919	1.60%	0.211%
18	17.498	2481	2484	2490	rVB2	114719	142907	1.09%	0.144%
19	17.727	2517	2523	2532	rBV2	1197405	1780854	13.55%	1.789%
20	17.992	2563	2568	2572	rBV	263300	383506	2.92%	0.385%
21	18.668	2680	2683	2690	rVB6	102693	229679	1.75%	0.231%
22	18.768	2697	2700	2707	rVB3	126822	216430	1.65%	0.217%
23	18.862	2711	2716	2721	rVV	944980	1254659	9.54%	1.260%
24	18.927	2725	2727	2732	rVB2	148223	191564	1.46%	0.192%
25	19.027	2739	2744	2753	rBV2	438436	706412	5.37%	0.710%
26	19.227	2770	2778	2785	rBV	806771	1258475	9.57%	1.264%
27	19.451	2811	2816	2827	rVB	7281142	9227908	70.19%	9.270%
28	20.109	2924	2928	2934	rVB3	496994	702967	5.35%	0.706%
29	20.280	2954	2957	2964	rBV2	114829	208373	1.58%	0.209%
30	20.774	3037	3041	3051	rVB2	784001	1365871	10.39%	1.372%
31	21.021	3077	3083	3087	rBV3	3027820	4410008	33.54%	4.430%
32	21.062	3087	3090	3101	rVB	449571	703749	5.35%	0.707%
33	21.756	3204	3208	3212	rBV	731295	993191	7.55%	0.998%
34	22.486	3329	3332	3339	rVB	332526	505303	3.84%	0.508%
35	22.874	3394	3398	3404	rBV	297074	659606	5.02%	0.663%
36	22.997	3413	3419	3427	rVB	2527426	4856721	36.94%	4.879%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047194.D
Acq On : 14 Aug 2024 16:50
Operator : RC/JU
Sample : P3519-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-16-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.715	3534	3541	3548	rBV	1497532	3366294	25.60%	3.382%
38	24.686	3698	3706	3716	rBV	1702001	4392233	33.41%	4.412%
39	28.115	4273	4289	4310	rVB6	2317528	13147614	100.00%	13.208%
40	29.003	4430	4440	4465	rVB3	1411914	7687999	58.47%	7.723%
41	29.768	4561	4570	4571	rBV	1047965	2318969	17.64%	2.330%




Sum of corrected areas: 99546350

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047194.D
Acq On : 14 Aug 2024 16:50
Operator : RC/JU
Sample : P3519-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-16-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

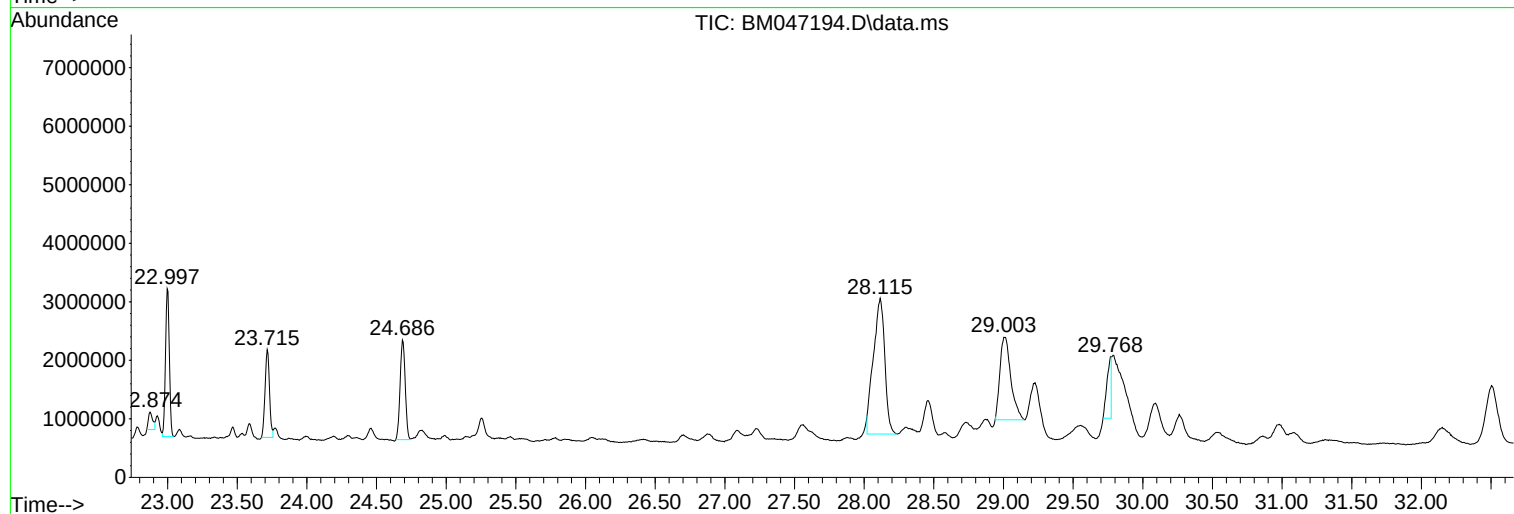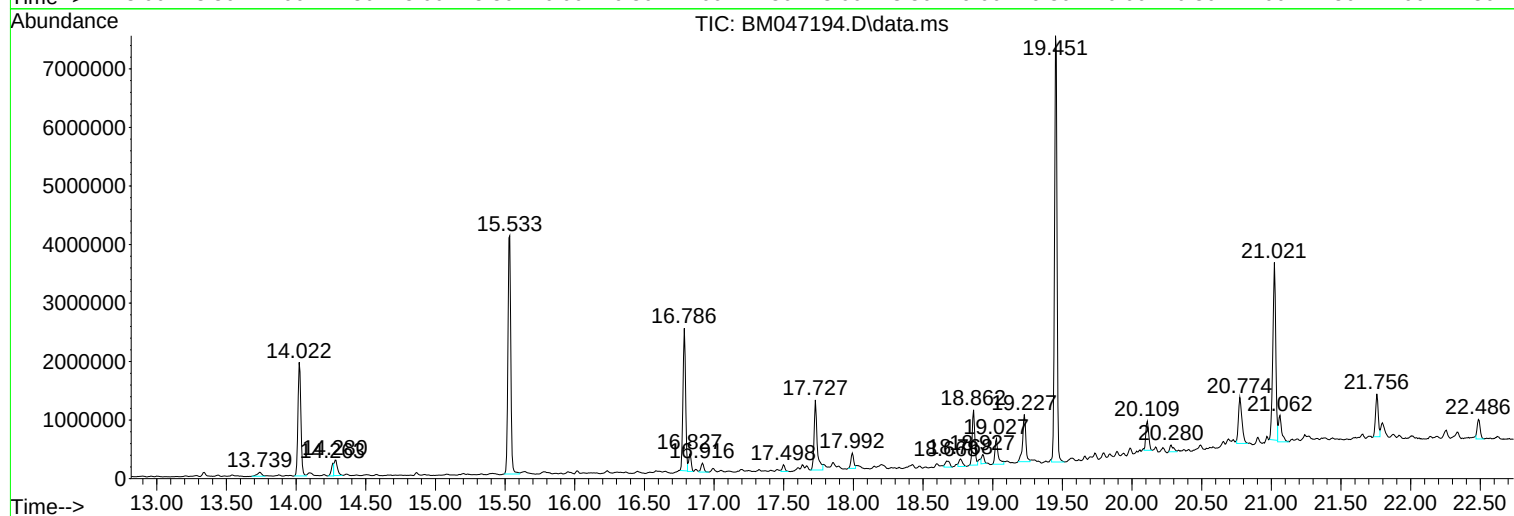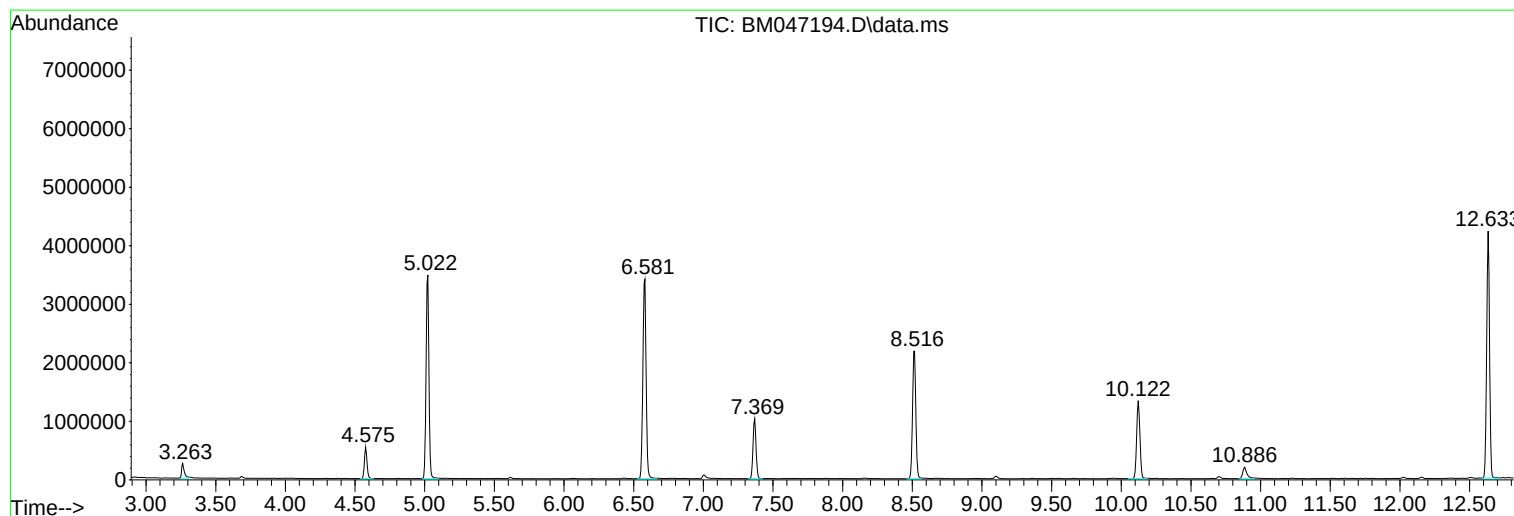

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047194.D
Acq On : 14 Aug 2024 16:50
Operator : RC/JU
Sample : P3519-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-16-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047194.D
Acq On : 14 Aug 2024 16:50
Operator : RC/JU
Sample : P3519-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-16-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------