

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047195.D
 Acq On : 14 Aug 2024 17:31
 Operator : RC/JU
 Sample : P3519-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-17-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	80	rVB	216004	309290	3.86%	0.336%
2	4.575	282	287	295	rBV	501132	654849	8.17%	0.711%
3	5.022	356	363	372	rBV	3424532	4813626	60.04%	5.230%
4	6.581	620	628	644	rBV	3202313	5102886	63.65%	5.544%
5	7.004	695	700	709	rBV	53488	108127	1.35%	0.117%
6	7.369	755	762	772	rBV	1327293	1971352	24.59%	2.142%
7	8.516	950	957	967	rBV	2114886	3415391	42.60%	3.711%
8	10.122	1223	1230	1237	rBV	1657468	2659919	33.18%	2.890%
9	10.886	1353	1360	1372	rBV	186249	398521	4.97%	0.433%
10	12.633	1649	1657	1667	rBV	4413410	6436007	80.28%	6.993%
11	13.339	1771	1777	1784	rBV2	69240	121586	1.52%	0.132%
12	13.739	1835	1845	1852	rBV2	73317	166318	2.07%	0.181%
13	14.027	1887	1894	1900	rBV	2471942	3612338	45.06%	3.925%
14	14.092	1900	1905	1915	rVB2	108955	213453	2.66%	0.232%
15	14.263	1927	1934	1935	rBV	97199	141332	1.76%	0.154%
16	14.286	1935	1938	1945	rVB5	135906	225201	2.81%	0.245%
17	15.086	2069	2074	2081	rBV	84431	130590	1.63%	0.142%
18	15.204	2086	2094	2099	rBV4	31461	82378	1.03%	0.090%
19	15.392	2122	2126	2139	rVB5	41080	112070	1.40%	0.122%
20	15.533	2143	2150	2163	rBV	4059389	5876915	73.31%	6.385%
21	15.774	2187	2191	2197	rBV4	45403	85404	1.07%	0.093%
22	16.015	2229	2232	2237	rBV4	60056	82904	1.03%	0.090%
23	16.233	2265	2269	2277	rVB8	55155	87345	1.09%	0.095%
24	16.445	2302	2305	2315	rVB2	52235	107393	1.34%	0.117%
25	16.539	2316	2321	2325	rBV5	45576	85167	1.06%	0.093%
26	16.604	2326	2332	2337	rVV	68690	138754	1.73%	0.151%
27	16.786	2357	2363	2367	rBV	3074013	4261687	53.16%	4.630%
28	16.827	2367	2370	2375	rVB	1448684	1786453	22.28%	1.941%
29	16.915	2381	2385	2393	rVB	448053	616686	7.69%	0.670%
30	16.992	2393	2398	2404	rBV6	43873	91900	1.15%	0.100%
31	17.198	2429	2433	2438	rVB	84063	123619	1.54%	0.134%
32	17.504	2482	2485	2494	rVB3	68183	105269	1.31%	0.114%
33	17.604	2497	2502	2504	rBV5	70316	111804	1.39%	0.121%
34	17.662	2509	2512	2516	rVB	188800	247993	3.09%	0.269%
35	17.727	2516	2523	2531	rBV2	1252949	2037421	25.41%	2.214%
36	17.857	2540	2545	2549	rBV2	254817	416513	5.20%	0.453%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047195.D
 Acq On : 14 Aug 2024 17:31
 Operator : RC/JU
 Sample : P3519-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-17-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.992	2564	2568	2572	rBV2	261063	350932	4.38%	0.381%
38	18.174	2596	2599	2603	rBV	93994	126843	1.58%	0.138%
39	18.598	2667	2671	2677	rBV3	96666	183988	2.30%	0.200%
40	18.668	2680	2683	2690	rVB6	109957	206920	2.58%	0.225%
41	18.739	2691	2695	2697	rBV	101982	141728	1.77%	0.154%
42	18.768	2697	2700	2709	rVB3	164276	276643	3.45%	0.301%
43	18.862	2711	2716	2721	rBV	2339037	3132389	39.07%	3.403%
44	19.027	2739	2744	2750	rBV2	422291	680940	8.49%	0.740%
45	19.227	2770	2778	2787	rVB	1990056	2986068	37.25%	3.244%
46	19.451	2811	2816	2827	rVB	6174879	8016866	100.00%	8.710%
47	19.733	2862	2864	2869	rVB	275554	323027	4.03%	0.351%
48	19.839	2879	2882	2886	rVB2	140452	172032	2.15%	0.187%
49	19.892	2888	2891	2896	rVV2	166467	228554	2.85%	0.248%
50	20.033	2912	2915	2916	rBV	120370	129805	1.62%	0.141%
51	20.109	2924	2928	2933	rVB3	503160	715974	8.93%	0.778%
52	20.280	2954	2957	2964	rBV2	116783	251249	3.13%	0.273%
53	20.774	3037	3041	3050	rVB2	773833	1362042	16.99%	1.480%
54	21.021	3077	3083	3087	rBV3	2985183	5034714	62.80%	5.470%
55	21.062	3087	3090	3099	rVB	805658	1166025	14.54%	1.267%
56	21.756	3204	3208	3212	rBV	655571	946338	11.80%	1.028%
57	22.880	3393	3399	3404	rBV	527702	1335636	16.66%	1.451%
58	23.003	3414	3420	3427	rVB	2307396	4244829	52.95%	4.612%
59	23.591	3515	3520	3530	rVB	470007	1035102	12.91%	1.125%
60	23.715	3535	3541	3548	rBV	1442032	3086072	38.49%	3.353%
61	24.685	3699	3706	3718	rVB	1539284	3882218	48.43%	4.218%
62	29.009	4432	4441	4466	rVB3	946916	5084386	63.42%	5.524%




Sum of corrected areas: 92039781

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047195.D
Acq On : 14 Aug 2024 17:31
Operator : RC/JU
Sample : P3519-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-17-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

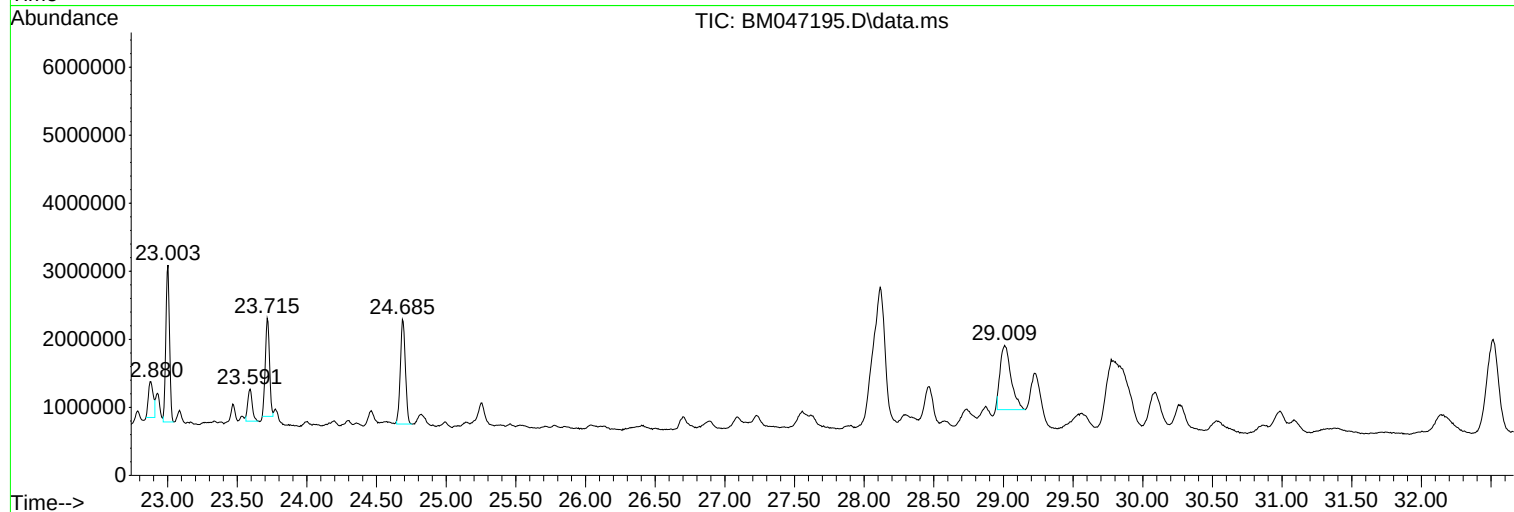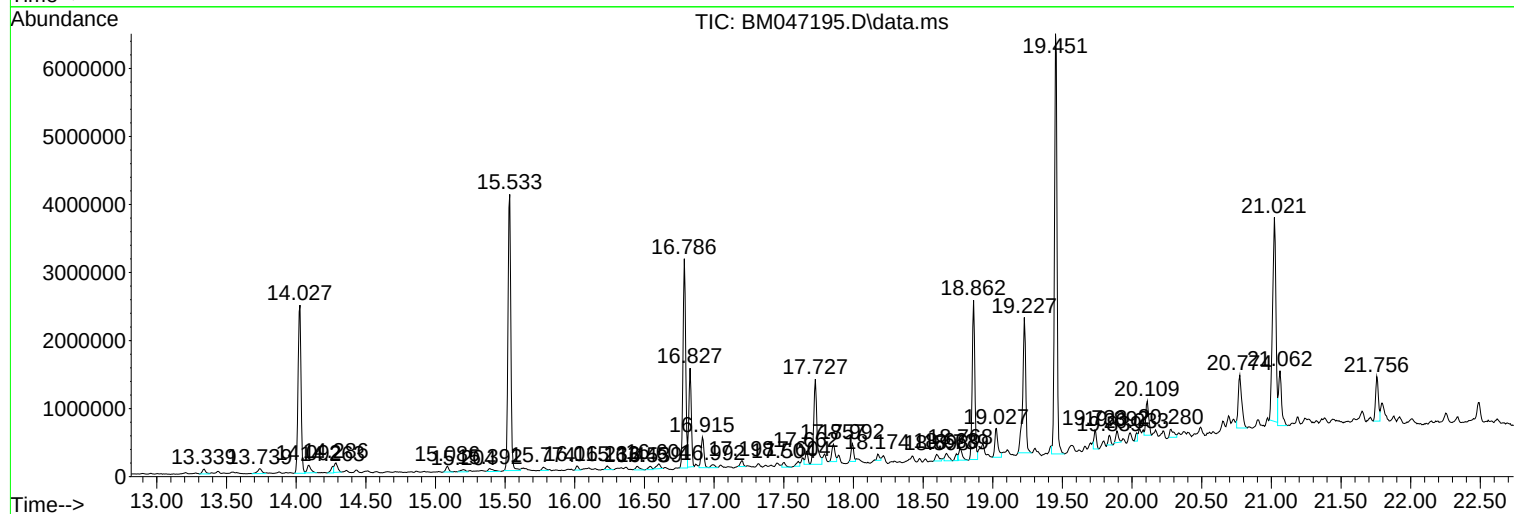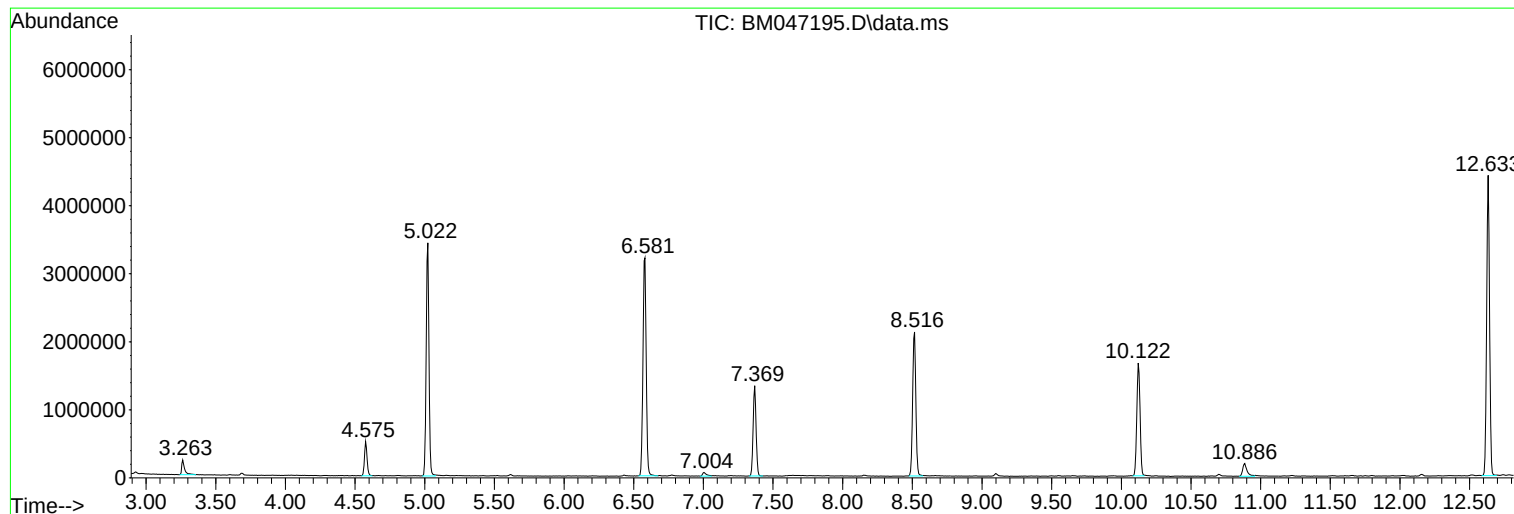

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047195.D
Acq On : 14 Aug 2024 17:31
Operator : RC/JU
Sample : P3519-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-17-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047195.D
Acq On : 14 Aug 2024 17:31
Operator : RC/JU
Sample : P3519-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-17-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------