

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047196.D
 Acq On : 14 Aug 2024 18:11
 Operator : RC/JU
 Sample : P3519-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-18-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	71	rBV	244025	311589	3.82%	0.391%
2	4.575	280	287	294	rBV	524663	710242	8.72%	0.892%
3	5.022	357	363	378	rBV	3654016	5114775	62.77%	6.421%
4	6.581	618	628	642	rBV	3632935	5531575	67.88%	6.944%
5	7.004	695	700	712	rBV	57528	115990	1.42%	0.146%
6	7.369	754	762	772	rBV	1353084	2040584	25.04%	2.562%
7	8.516	949	957	968	rBV	2298806	3731351	45.79%	4.684%
8	10.122	1223	1230	1246	rBV	1699222	2839014	34.84%	3.564%
9	10.886	1352	1360	1370	rBV	183197	395006	4.85%	0.496%
10	12.633	1650	1657	1666	rBV	4918542	7002309	85.93%	8.791%
11	13.339	1771	1777	1785	rBV2	51397	102924	1.26%	0.129%
12	13.739	1837	1845	1852	rBV2	76574	159385	1.96%	0.200%
13	14.027	1886	1894	1901	rBV	2546602	3766113	46.22%	4.728%
14	14.092	1901	1905	1915	rVB3	66758	148843	1.83%	0.187%
15	14.263	1927	1934	1935	rBV3	113227	166634	2.04%	0.209%
16	14.286	1935	1938	1946	rVB4	156108	255559	3.14%	0.321%
17	15.533	2143	2150	2159	rBV	4332074	6150803	75.48%	7.722%
18	15.774	2185	2191	2198	rBV8	40658	114239	1.40%	0.143%
19	16.604	2325	2332	2336	rBV4	37132	85005	1.04%	0.107%
20	16.786	2357	2363	2367	rBV	3045757	4245082	52.09%	5.329%
21	16.827	2367	2370	2375	rVB	777679	981339	12.04%	1.232%
22	16.915	2381	2385	2392	rVB	235860	350028	4.30%	0.439%
23	17.633	2505	2507	2510	rVV2	67622	81656	1.00%	0.103%
24	17.662	2510	2512	2516	rVB	102926	131695	1.62%	0.165%
25	17.727	2517	2523	2531	rBV2	1219640	1887996	23.17%	2.370%
26	17.856	2541	2545	2549	rBV2	160502	239929	2.94%	0.301%
27	17.992	2564	2568	2572	rBV	229091	307196	3.77%	0.386%
28	18.598	2668	2671	2675	rBV3	68162	102354	1.26%	0.128%
29	18.762	2697	2699	2709	rVB5	113929	194331	2.38%	0.244%
30	18.862	2711	2716	2721	rBV	1703998	2323585	28.51%	2.917%
31	18.927	2725	2727	2732	rVB3	140884	193710	2.38%	0.243%
32	19.027	2739	2744	2751	rBV2	412609	653925	8.02%	0.821%
33	19.227	2770	2778	2787	rBV	1345085	2096999	25.73%	2.633%
34	19.450	2811	2816	2825	rVB	6567433	8148992	100.00%	10.230%
35	19.733	2861	2864	2869	rVB	174966	244125	3.00%	0.306%
36	19.839	2879	2882	2886	rBV	124079	143812	1.76%	0.181%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047196.D
Acq On : 14 Aug 2024 18:11
Operator : RC/JU
Sample : P3519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-18-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.892	2888	2891	2895	rBV3	107662	176610	2.17%	0.222%
38	20.109	2924	2928	2933	rVB4	362802	493387	6.05%	0.619%
39	20.768	3037	3040	3050	rVB2	669677	1113860	13.67%	1.398%
40	21.021	3076	3083	3087	rBV2	2787035	4451204	54.62%	5.588%
41	21.062	3087	3090	3098	rVB	580191	846439	10.39%	1.063%
42	21.756	3204	3208	3211	rBV	520871	699193	8.58%	0.878%
43	22.486	3328	3332	3339	rVB	371500	601150	7.38%	0.755%
44	22.874	3394	3398	3403	rBV	350153	720093	8.84%	0.904%
45	22.997	3413	3419	3426	rVB	1855492	3353349	41.15%	4.210%
46	23.715	3534	3541	3548	rBV	1382413	3058722	37.53%	3.840%
47	24.685	3699	3706	3717	rVB	1216720	3074962	37.73%	3.860%




Sum of corrected areas: 79657663

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047196.D
Acq On : 14 Aug 2024 18:11
Operator : RC/JU
Sample : P3519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-18-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

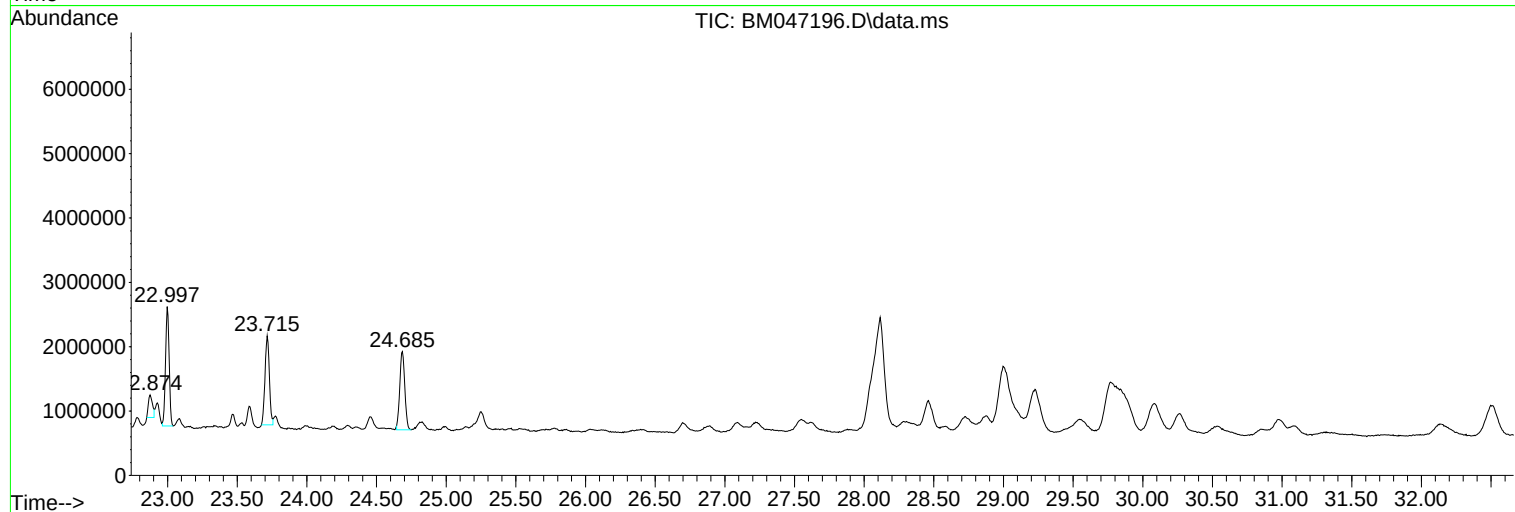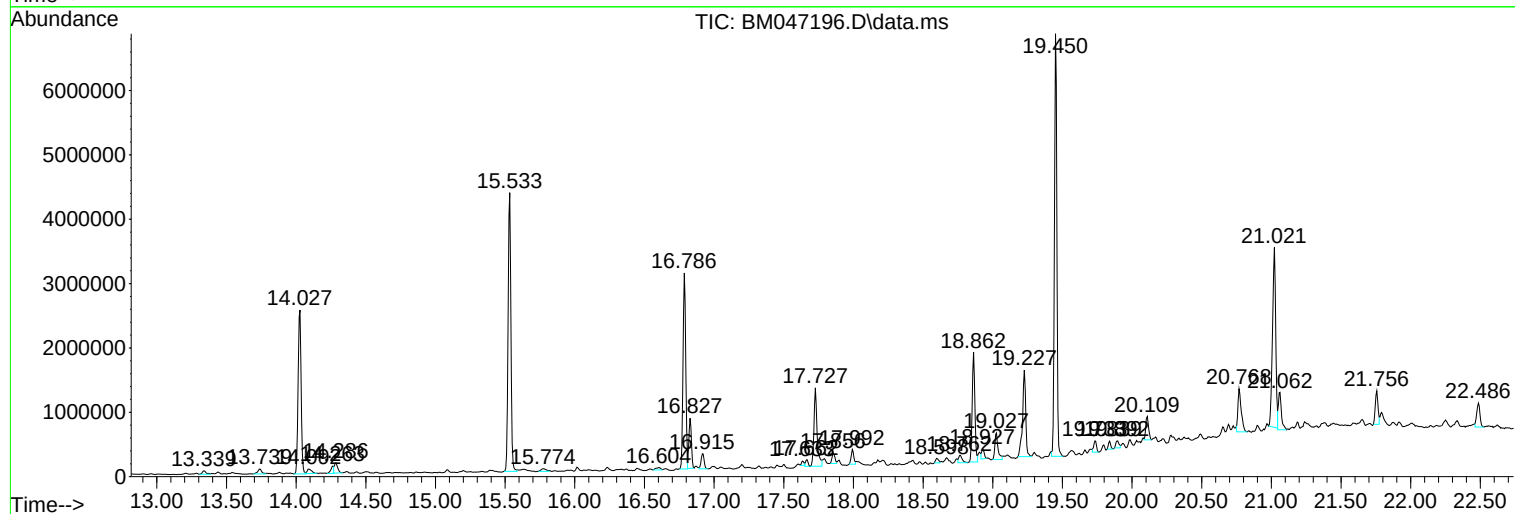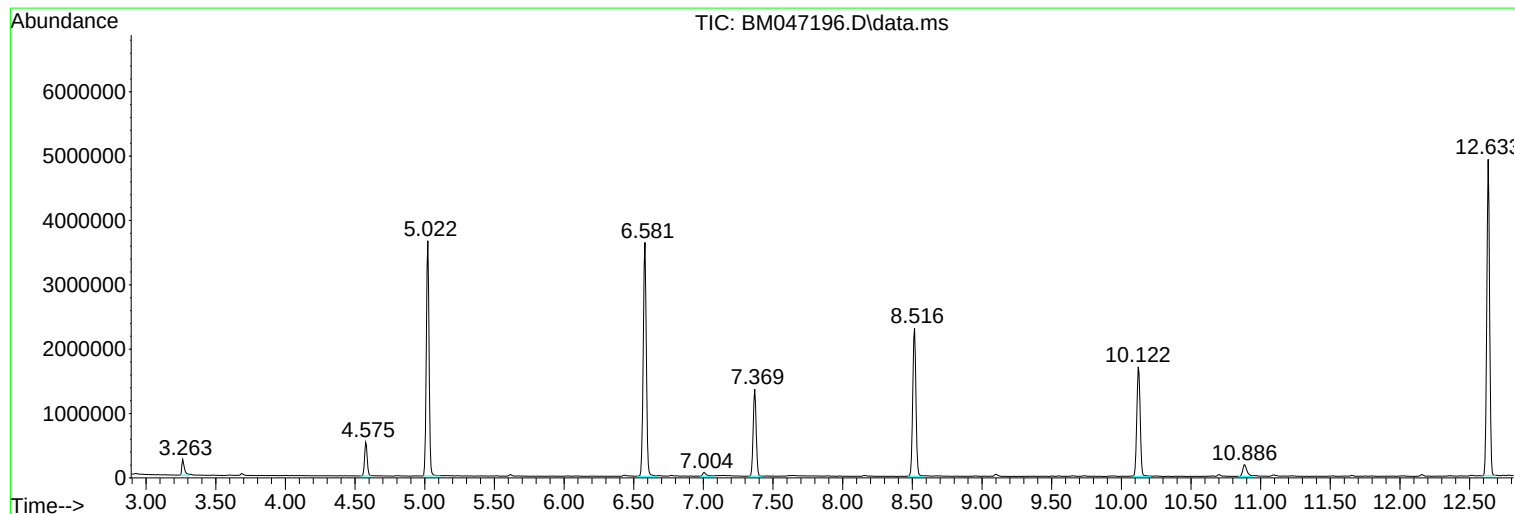

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047196.D
Acq On : 14 Aug 2024 18:11
Operator : RC/JU
Sample : P3519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-18-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047196.D
Acq On : 14 Aug 2024 18:11
Operator : RC/JU
Sample : P3519-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-18-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------