

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047198.D
 Acq On : 14 Aug 2024 19:31
 Operator : RC/JU
 Sample : P3519-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-20-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	77	rBV	317182	418796	5.15%	0.506%
2	4.575	281	287	295	rBV	576565	777790	9.56%	0.940%
3	5.022	356	363	380	rBV	4156678	5827945	71.65%	7.047%
4	6.581	614	628	643	rBV	4071671	6288100	77.31%	7.603%
5	6.998	694	699	712	rBV	124777	243826	3.00%	0.295%
6	7.369	752	762	771	rBV	1320819	1979882	24.34%	2.394%
7	8.516	949	957	968	rBV	2625196	4175521	51.34%	5.049%
8	10.122	1223	1230	1238	rBV	1642688	2675790	32.90%	3.236%
9	10.886	1352	1360	1369	rBV	294785	601225	7.39%	0.727%
10	12.633	1650	1657	1667	rBV	4709997	6945862	85.40%	8.399%
11	13.739	1835	1845	1851	rBV2	58582	132398	1.63%	0.160%
12	14.027	1887	1894	1902	rBV	2357196	3546094	43.60%	4.288%
13	14.268	1927	1935	1936	rBV	3439489	4500038	55.33%	5.441%
14	14.286	1936	1938	1947	rVB	4317620	5152781	63.35%	6.231%
15	15.533	2143	2150	2162	rBV	5029875	6854283	84.27%	8.288%
16	15.633	2163	2167	2177	rVB	43086	103426	1.27%	0.125%
17	16.786	2357	2363	2368	rBV	2980507	4091974	50.31%	4.948%
18	16.827	2368	2370	2375	rVB	257572	293071	3.60%	0.354%
19	16.921	2381	2386	2391	rVB2	135921	192765	2.37%	0.233%
20	17.498	2481	2484	2492	rVB	94601	128982	1.59%	0.156%
21	17.727	2517	2523	2532	rBV2	1013249	1600101	19.67%	1.935%
22	17.856	2541	2545	2549	rBV2	75384	107353	1.32%	0.130%
23	17.992	2564	2568	2572	rBV	175923	252903	3.11%	0.306%
24	18.686	2683	2686	2690	rVB3	192640	246205	3.03%	0.298%
25	18.862	2712	2716	2721	rBV	994631	1336855	16.44%	1.617%
26	19.027	2740	2744	2752	rBV2	362155	539821	6.64%	0.653%
27	19.227	2771	2778	2788	rVB	886755	1312499	16.14%	1.587%
28	19.456	2811	2817	2826	rVB	6632992	8133723	100.00%	9.835%
29	20.109	2925	2928	2934	rVB2	254986	366961	4.51%	0.444%
30	20.774	3037	3041	3051	rVB2	687190	1160252	14.26%	1.403%
31	21.021	3077	3083	3088	rBV2	2573863	4109682	50.53%	4.969%
32	21.062	3088	3090	3098	rVB	402474	494860	6.08%	0.598%
33	21.756	3205	3208	3211	rBV	333831	438420	5.39%	0.530%
34	22.997	3414	3419	3426	rVB	1350295	2488643	30.60%	3.009%
35	23.715	3535	3541	3549	rBV	1292097	2858340	35.14%	3.456%
36	24.685	3700	3706	3718	rVB	902552	2323171	28.56%	2.809%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047198.D
Acq On : 14 Aug 2024 19:31
Operator : RC/JU
Sample : P3519-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-20-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 82700338

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047198.D
Acq On : 14 Aug 2024 19:31
Operator : RC/JU
Sample : P3519-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-20-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

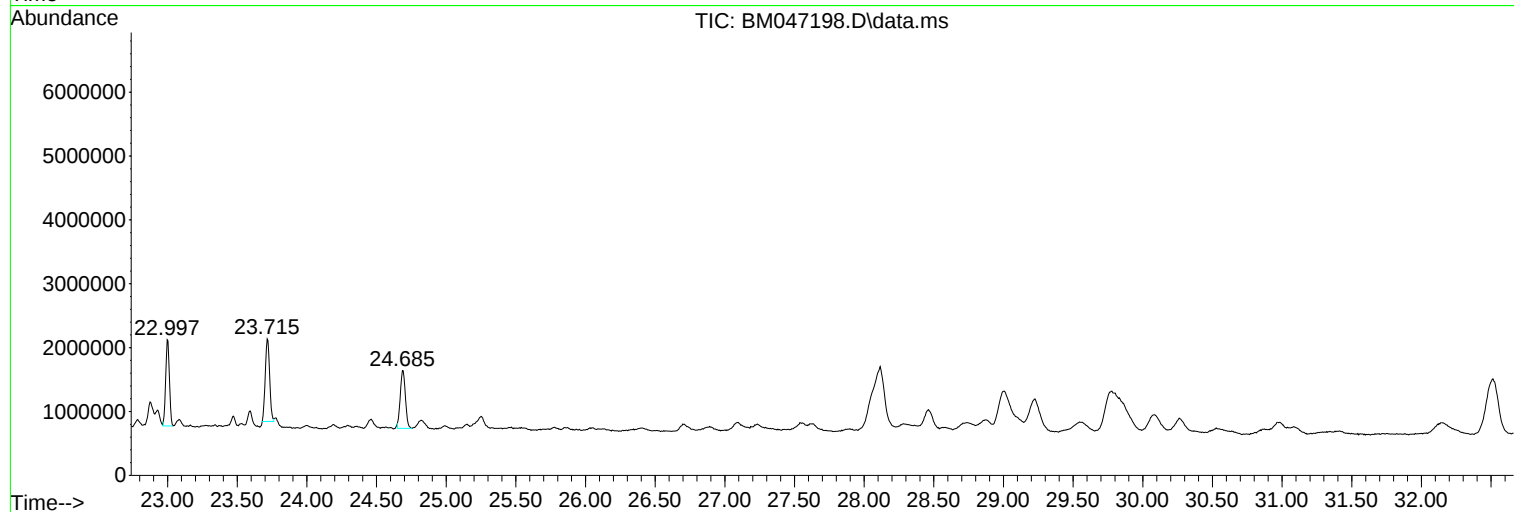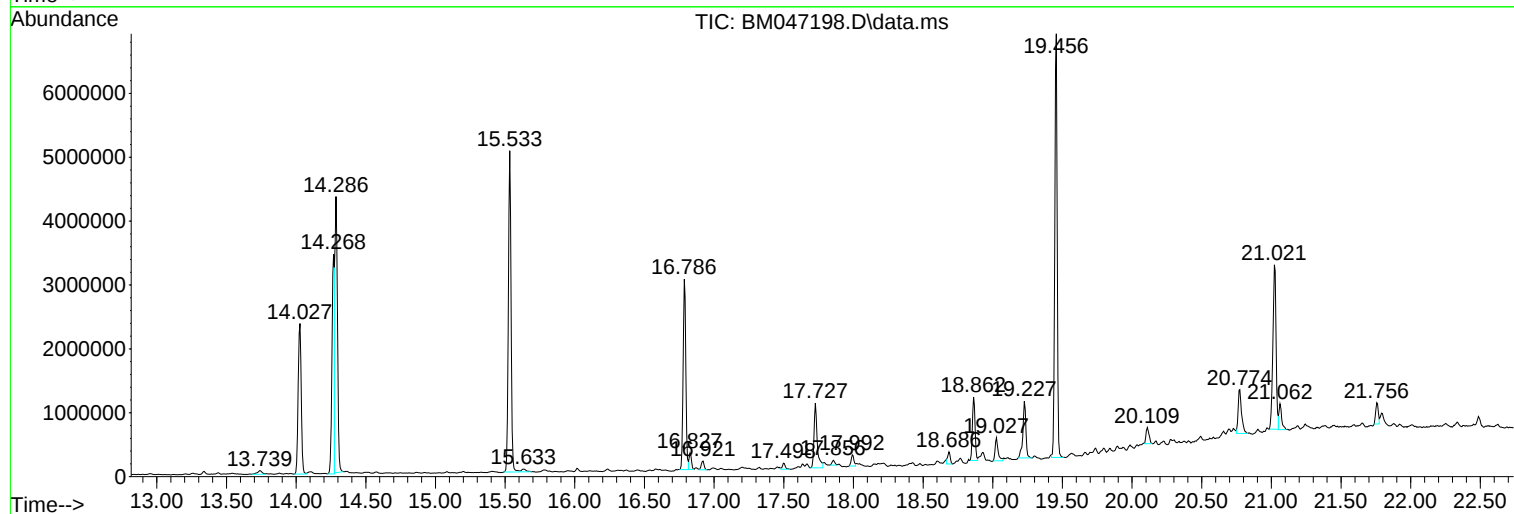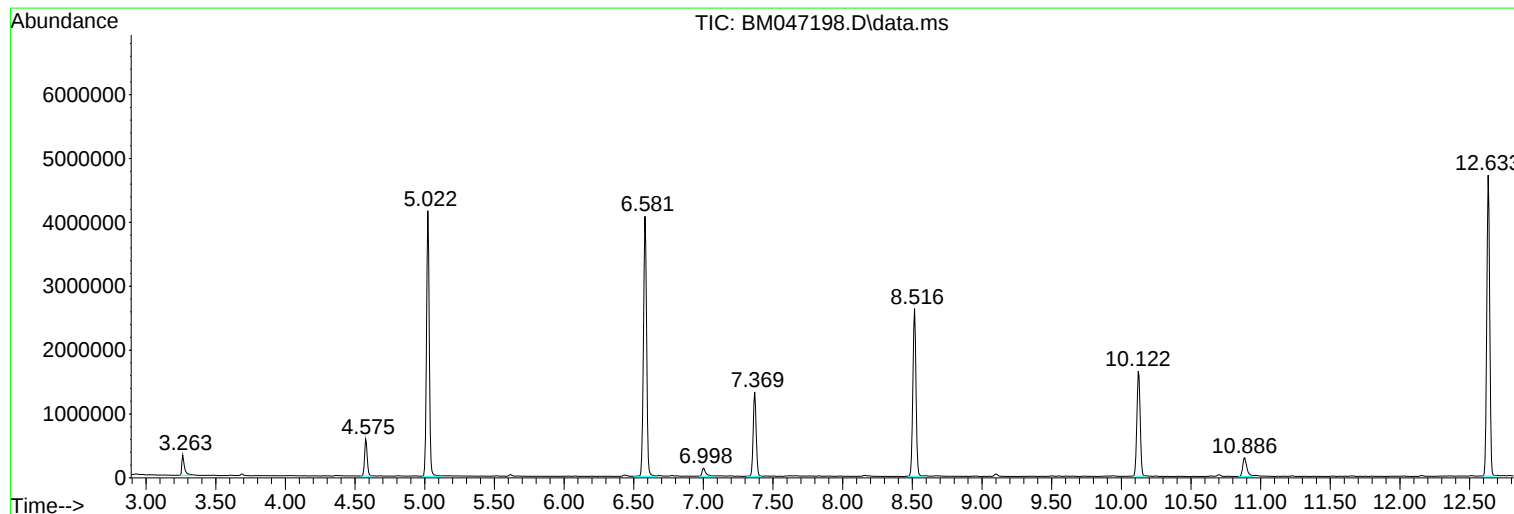

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047198.D
Acq On : 14 Aug 2024 19:31
Operator : RC/JU
Sample : P3519-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-20-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047198.D
Acq On : 14 Aug 2024 19:31
Operator : RC/JU
Sample : P3519-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-20-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------