

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047199.D
 Acq On : 14 Aug 2024 20:11
 Operator : RC/JU
 Sample : P3519-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-21-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	72	rBV	376894	482891	5.01%	0.532%
2	4.575	282	287	297	rVB	675165	917203	9.52%	1.011%
3	5.022	356	363	374	rBV	4777206	6746465	70.01%	7.435%
4	6.581	618	628	642	rBV	4757457	7422045	77.02%	8.180%
5	6.998	694	699	710	rBV	149008	267166	2.77%	0.294%
6	7.369	753	762	769	rBV	1362583	2052340	21.30%	2.262%
7	8.516	948	957	973	rBV	3024692	4898440	50.83%	5.398%
8	10.122	1223	1230	1239	rBV	1728483	2791178	28.97%	3.076%
9	10.886	1352	1360	1370	rBV	324941	659905	6.85%	0.727%
10	12.633	1649	1657	1673	rBV	5700165	8328394	86.43%	9.178%
11	13.739	1836	1845	1851	rBV	78567	175272	1.82%	0.193%
12	14.027	1887	1894	1901	rBV	2592710	3691968	38.31%	4.069%
13	14.263	1928	1934	1935	rBV	1542581	1764475	18.31%	1.945%
14	15.533	2143	2150	2159	rBV	5758476	8079943	83.85%	8.905%
15	15.633	2163	2167	2177	rVB7	51818	116831	1.21%	0.129%
16	16.786	2357	2363	2367	rBV	3075583	4186031	43.44%	4.613%
17	16.827	2367	2370	2375	rVB	854119	1044922	10.84%	1.152%
18	16.915	2381	2385	2392	rVB	206277	298566	3.10%	0.329%
19	17.504	2481	2485	2492	rVB3	139894	206755	2.15%	0.228%
20	17.668	2509	2513	2517	rVB	131328	166446	1.73%	0.183%
21	17.727	2517	2523	2531	rBV2	1242083	1933602	20.07%	2.131%
22	17.857	2540	2545	2549	rBV2	211489	346938	3.60%	0.382%
23	17.892	2549	2551	2556	rVB	103013	134060	1.39%	0.148%
24	17.992	2564	2568	2572	rBV3	156482	239145	2.48%	0.264%
25	18.215	2603	2606	2612	rVB2	179872	260001	2.70%	0.287%
26	18.604	2667	2672	2676	rBV	127335	222320	2.31%	0.245%
27	18.686	2684	2686	2691	rVB3	224509	253023	2.63%	0.279%
28	18.739	2692	2695	2697	rBV	95806	117494	1.22%	0.129%
29	18.862	2711	2716	2721	rBV	2299424	3060269	31.76%	3.373%
30	18.933	2725	2728	2732	rVB4	129849	167260	1.74%	0.184%
31	19.027	2740	2744	2749	rBV2	371451	501951	5.21%	0.553%
32	19.227	2770	2778	2787	rBV	1934446	2962283	30.74%	3.265%
33	19.415	2807	2810	2811	rBV2	97044	101599	1.05%	0.112%
34	19.451	2811	2816	2827	rVB	7659920	9636267	100.00%	10.620%
35	19.733	2862	2864	2869	rVB	228133	277454	2.88%	0.306%
36	19.839	2879	2882	2886	rBV2	130726	149244	1.55%	0.164%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047199.D
Acq On : 14 Aug 2024 20:11
Operator : RC/JU
Sample : P3519-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-21-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.892	2889	2891	2895	rVB2	139808	169555	1.76%	0.187%
38	20.109	2925	2928	2933	rVB4	218244	329659	3.42%	0.363%
39	20.768	3036	3040	3051	rVB3	1158247	2001791	20.77%	2.206%
40	21.021	3077	3083	3087	rBV2	2601565	4411314	45.78%	4.862%
41	21.062	3087	3090	3101	rVB	918752	1334118	13.84%	1.470%
42	22.880	3393	3399	3404	rBV	612214	1498295	15.55%	1.651%
43	22.997	3414	3419	3426	rVB	1062925	1863369	19.34%	2.054%
44	23.721	3535	3542	3548	rBV	1286824	2817784	29.24%	3.105%
45	24.686	3701	3706	3717	rVB	716856	1652729	17.15%	1.821%




Sum of corrected areas: 90738760

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047199.D
Acq On : 14 Aug 2024 20:11
Operator : RC/JU
Sample : P3519-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-21-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

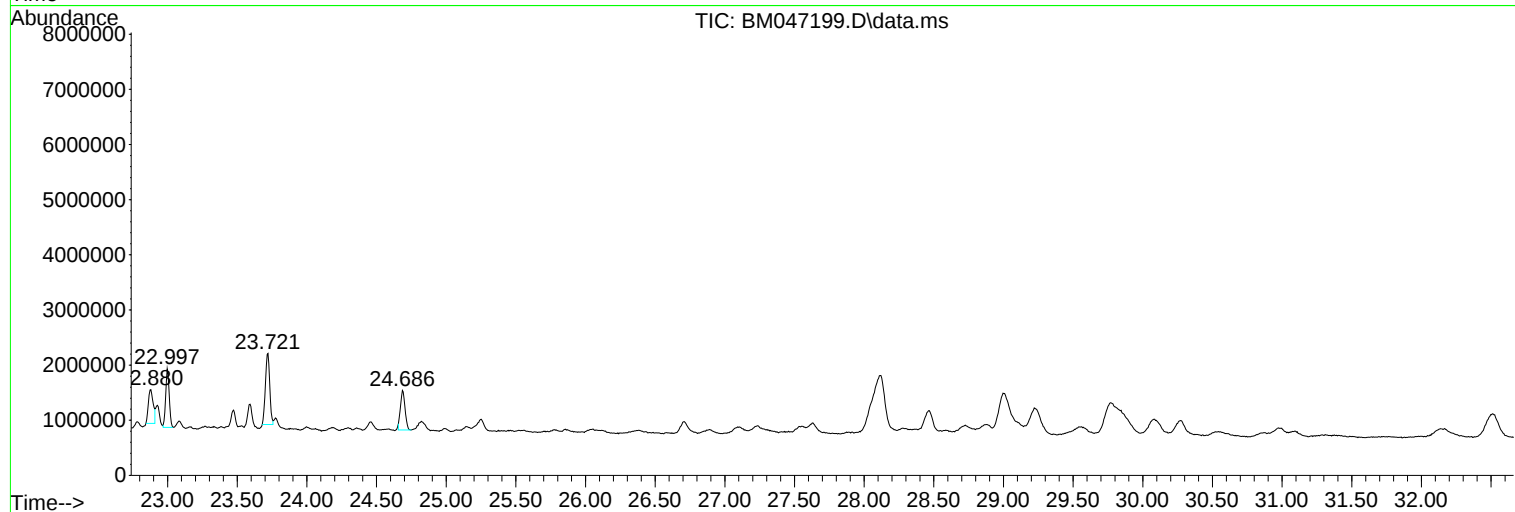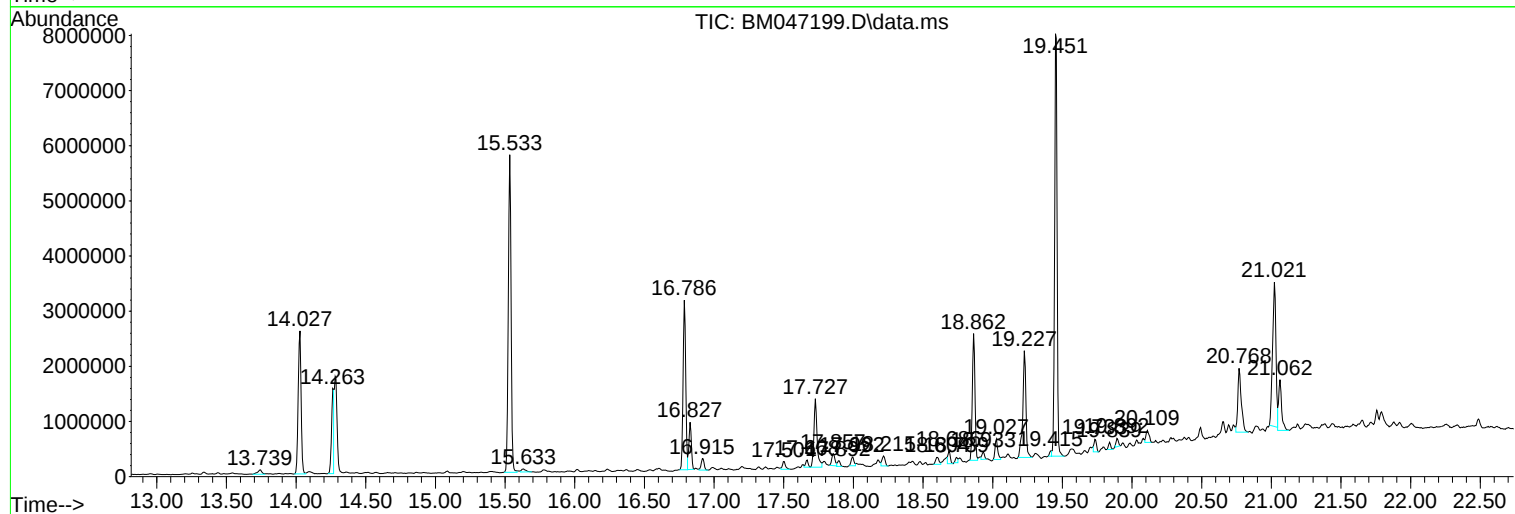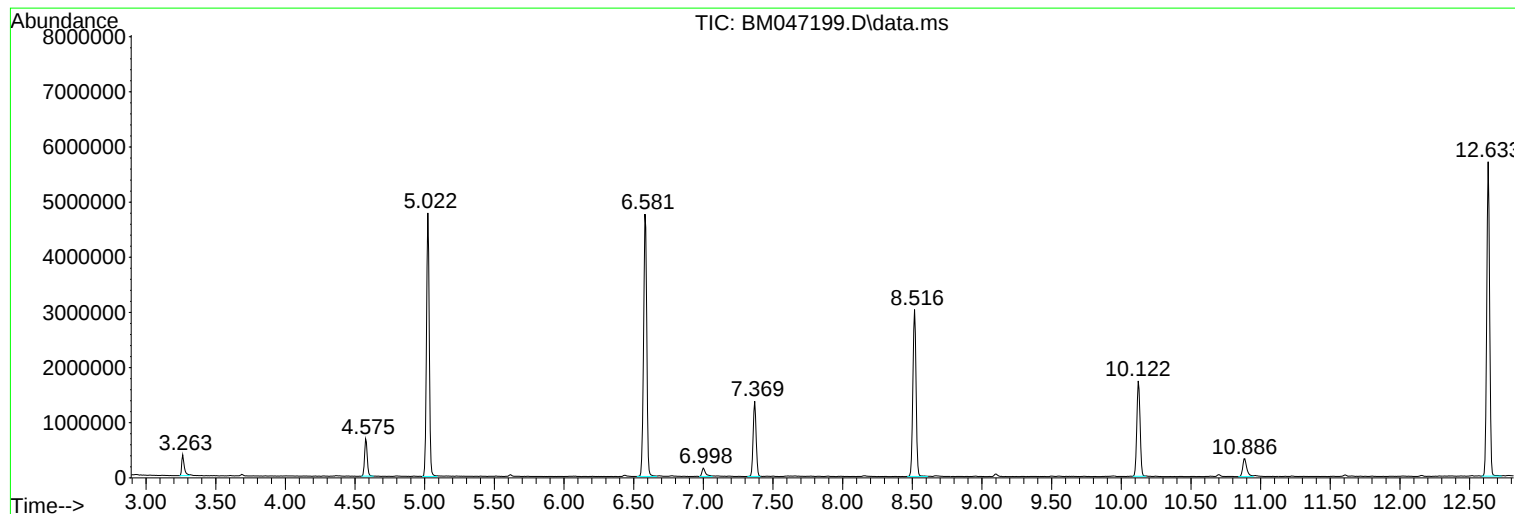

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047199.D
Acq On : 14 Aug 2024 20:11
Operator : RC/JU
Sample : P3519-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-21-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047199.D
Acq On : 14 Aug 2024 20:11
Operator : RC/JU
Sample : P3519-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-21-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------