

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047200.D
 Acq On : 14 Aug 2024 20:51
 Operator : RC/JU
 Sample : P3519-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-22-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	61	64	77	rBV	143966	209153	3.53%	0.383%
2	4.575	282	287	297	rBV	398908	539373	9.11%	0.989%
3	5.022	357	363	379	rBV	2863520	4043856	68.26%	7.413%
4	6.581	621	628	643	rBV	2843162	4332058	73.13%	7.941%
5	7.004	696	700	710	rBV	49559	91704	1.55%	0.168%
6	7.369	753	762	772	rBV	1286434	1911600	32.27%	3.504%
7	8.516	949	957	969	rBV	1827459	2916923	49.24%	5.347%
8	9.098	1052	1056	1069	rVB2	38626	78487	1.32%	0.144%
9	10.122	1223	1230	1241	rBV	1626962	2634638	44.48%	4.830%
10	10.886	1353	1360	1369	rBV	156836	317636	5.36%	0.582%
11	12.633	1650	1657	1666	rBV	3517383	5166587	87.22%	9.471%
12	13.739	1836	1845	1850	rBV4	39850	95059	1.60%	0.174%
13	14.027	1887	1894	1900	rBV	2456195	3533068	59.64%	6.477%
14	14.286	1929	1938	1946	rVB2	110942	269242	4.55%	0.494%
15	15.533	2142	2150	2162	rBV	3486054	4949897	83.56%	9.074%
16	15.780	2187	2192	2201	rBV7	26277	72079	1.22%	0.132%
17	16.016	2228	2232	2238	rBV4	36564	61094	1.03%	0.112%
18	16.786	2358	2363	2368	rBV	2899468	3935191	66.43%	7.214%
19	16.827	2368	2370	2375	rVB	254135	287120	4.85%	0.526%
20	16.916	2382	2385	2392	rVB2	91642	127948	2.16%	0.235%
21	17.498	2481	2484	2491	rVB	57822	78375	1.32%	0.144%
22	17.727	2517	2523	2532	rBV2	618898	1007288	17.00%	1.847%
23	17.857	2542	2545	2549	rVB2	50406	63923	1.08%	0.117%
24	17.992	2565	2568	2575	rBV6	87510	122530	2.07%	0.225%
25	18.327	2621	2625	2630	rVB5	66877	90827	1.53%	0.167%
26	18.862	2711	2716	2720	rBV	646144	833462	14.07%	1.528%
27	19.027	2740	2744	2750	rBV2	213042	325572	5.50%	0.597%
28	19.227	2771	2778	2787	rBV	482340	718573	12.13%	1.317%
29	19.457	2811	2817	2824	rVB	4679608	5923816	100.00%	10.859%
30	20.109	2924	2928	2934	rBV4	187623	297932	5.03%	0.546%
31	20.768	3037	3040	3048	rVB2	468410	715785	12.08%	1.312%
32	21.021	3078	3083	3088	rBV2	2384520	3371978	56.92%	6.181%
33	22.997	3414	3419	3427	rVB	796430	1426597	24.08%	2.615%
34	23.715	3535	3541	3549	rBV	1257993	2753998	46.49%	5.049%
35	24.686	3701	3706	3716	rVB	509217	1246669	21.05%	2.285%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047200.D
Acq On : 14 Aug 2024 20:51
Operator : RC/JU
Sample : P3519-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-22-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 54550038

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047200.D
Acq On : 14 Aug 2024 20:51
Operator : RC/JU
Sample : P3519-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-22-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

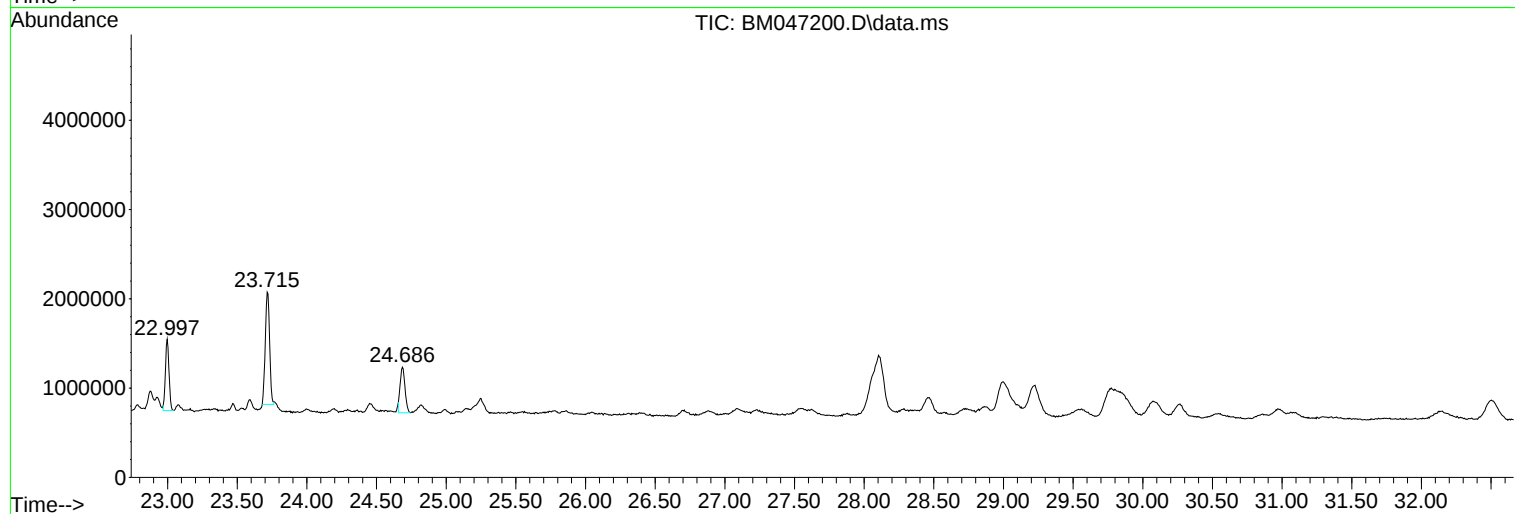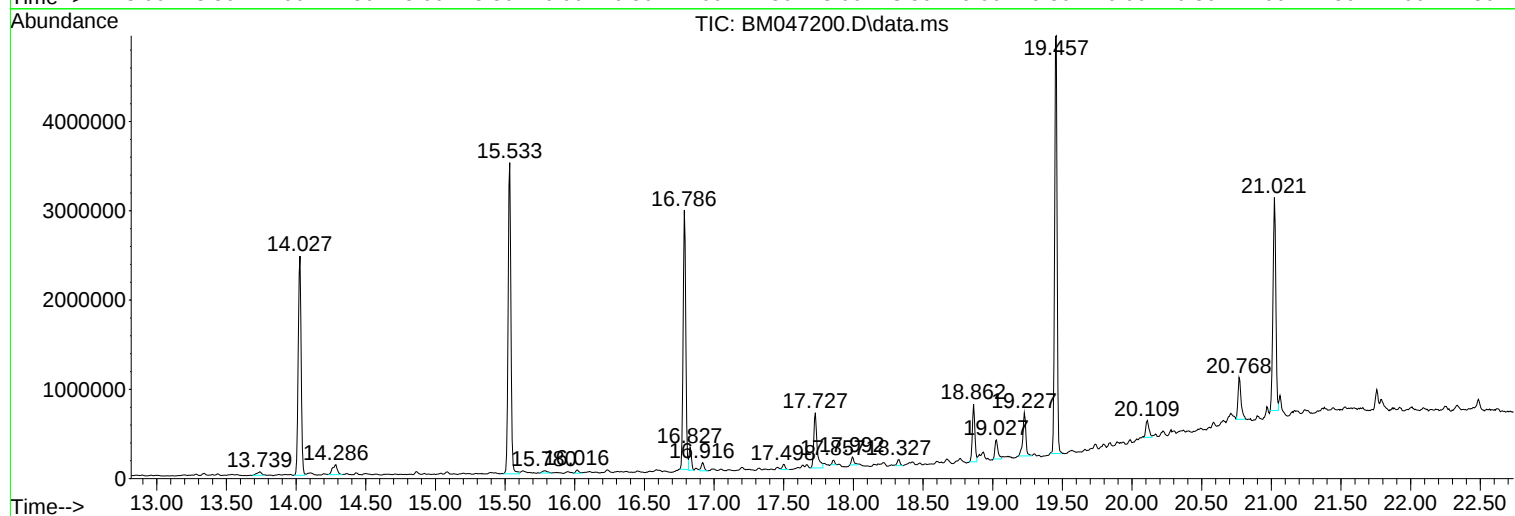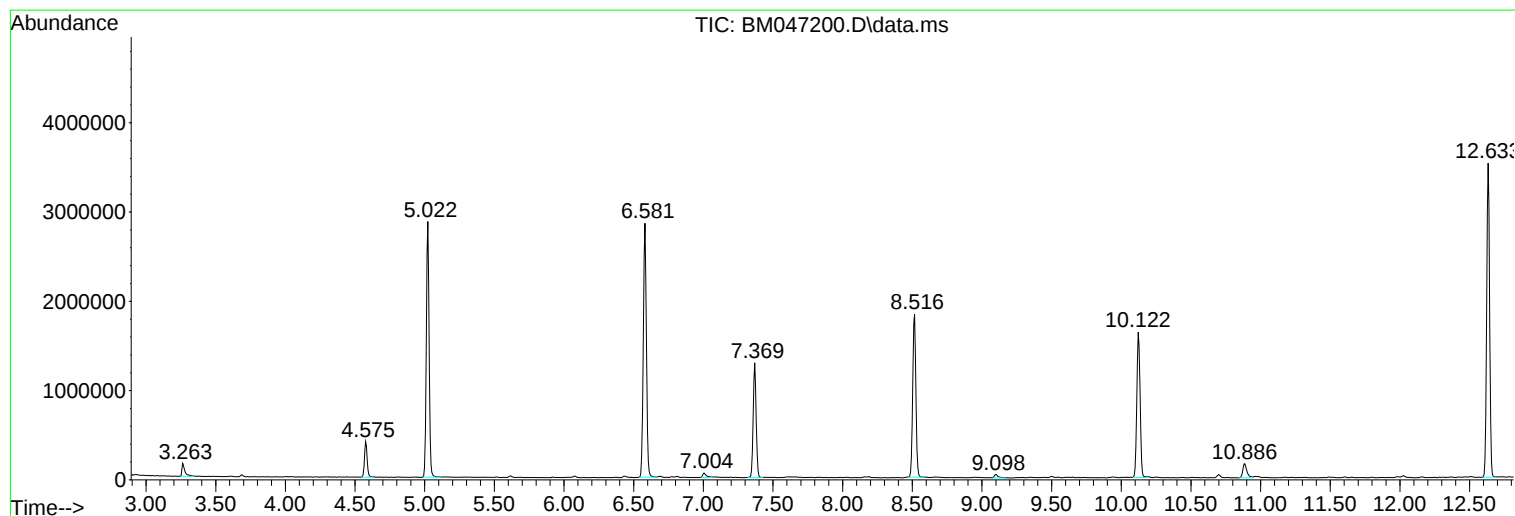

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047200.D
Acq On : 14 Aug 2024 20:51
Operator : RC/JU
Sample : P3519-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-22-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047200.D
Acq On : 14 Aug 2024 20:51
Operator : RC/JU
Sample : P3519-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-22-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------