

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047201.D
 Acq On : 14 Aug 2024 21:31
 Operator : RC/JU
 Sample : P3519-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-23-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	72	rBV	407812	521534	5.28%	0.509%
2	4.575	281	287	296	rBV	687032	925918	9.38%	0.903%
3	5.022	357	363	373	rBV	4834026	6788111	68.77%	6.623%
4	6.581	616	628	641	rBV	4675289	7434505	75.32%	7.254%
5	6.998	695	699	713	rBV	190796	339916	3.44%	0.332%
6	7.369	752	762	770	rBV	1359671	2045050	20.72%	1.995%
7	8.516	949	957	969	rBV	3101962	4960198	50.25%	4.839%
8	10.122	1223	1230	1237	rBV	1694694	2750182	27.86%	2.683%
9	10.886	1353	1360	1370	rBV	384611	772295	7.82%	0.754%
10	12.633	1650	1657	1666	rBV	6012367	8704774	88.19%	8.493%
11	14.027	1887	1894	1901	rBV	2528745	3672457	37.20%	3.583%
12	14.092	1901	1905	1914	rVB4	53505	110084	1.12%	0.107%
13	14.269	1928	1935	1937	rBV	5859121	9165134	92.85%	8.942%
14	14.292	1937	1939	1949	rVB	7738805	8288284	83.97%	8.087%
15	15.533	2143	2150	2159	rBV	5931304	8435587	85.46%	8.230%
16	15.627	2163	2166	2178	rVB6	60434	129548	1.31%	0.126%
17	16.786	2358	2363	2367	rBV	3020795	4186923	42.42%	4.085%
18	16.827	2367	2370	2375	rVB	662531	884783	8.96%	0.863%
19	16.921	2381	2386	2391	rVB2	190357	277017	2.81%	0.270%
20	17.204	2430	2434	2446	rVB	74232	189219	1.92%	0.185%
21	17.498	2481	2484	2490	rVB	125572	168879	1.71%	0.165%
22	17.668	2510	2513	2517	rVB	87278	109895	1.11%	0.107%
23	17.727	2517	2523	2532	rBV2	1318148	2018770	20.45%	1.970%
24	17.857	2541	2545	2549	rBV2	128179	174787	1.77%	0.171%
25	17.992	2564	2568	2572	rBV	169014	241177	2.44%	0.235%
26	18.215	2604	2606	2613	rVB	102956	136080	1.38%	0.133%
27	18.609	2668	2673	2678	rBV5	126632	248170	2.51%	0.242%
28	18.686	2683	2686	2691	rVB3	295280	360012	3.65%	0.351%
29	18.827	2707	2710	2712	rBV	97200	114693	1.16%	0.112%
30	18.862	2712	2716	2721	rVV	1379070	1851389	18.76%	1.806%
31	18.927	2724	2727	2732	rVB4	215464	314914	3.19%	0.307%
32	19.027	2740	2744	2751	rBV2	372484	538660	5.46%	0.526%
33	19.227	2770	2778	2788	rBV	1129217	1765253	17.88%	1.722%
34	19.456	2811	2817	2827	rVB	8171364	9870883	100.00%	9.631%
35	19.739	2862	2865	2869	rVB2	130629	153732	1.56%	0.150%
36	20.109	2925	2928	2933	rVB2	245316	359453	3.64%	0.351%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047201.D
Acq On : 14 Aug 2024 21:31
Operator : RC/JU
Sample : P3519-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-23-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.768	3036	3040	3050	rVB2	931947	1466388	14.86%	1.431%
38	21.021	3077	3083	3087	rBV2	2515832	3874635	39.25%	3.780%
39	21.062	3088	3090	3100	rVB	487273	633922	6.42%	0.618%
40	21.756	3205	3208	3211	rBV	340008	388970	3.94%	0.380%
41	22.997	3414	3419	3427	rVB	1231285	2229676	22.59%	2.175%
42	23.721	3535	3542	3549	rBV	1249966	2807593	28.44%	2.739%
43	24.686	3700	3706	3717	rVB	819879	2084729	21.12%	2.034%




Sum of corrected areas: 102494179

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047201.D
Acq On : 14 Aug 2024 21:31
Operator : RC/JU
Sample : P3519-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-23-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

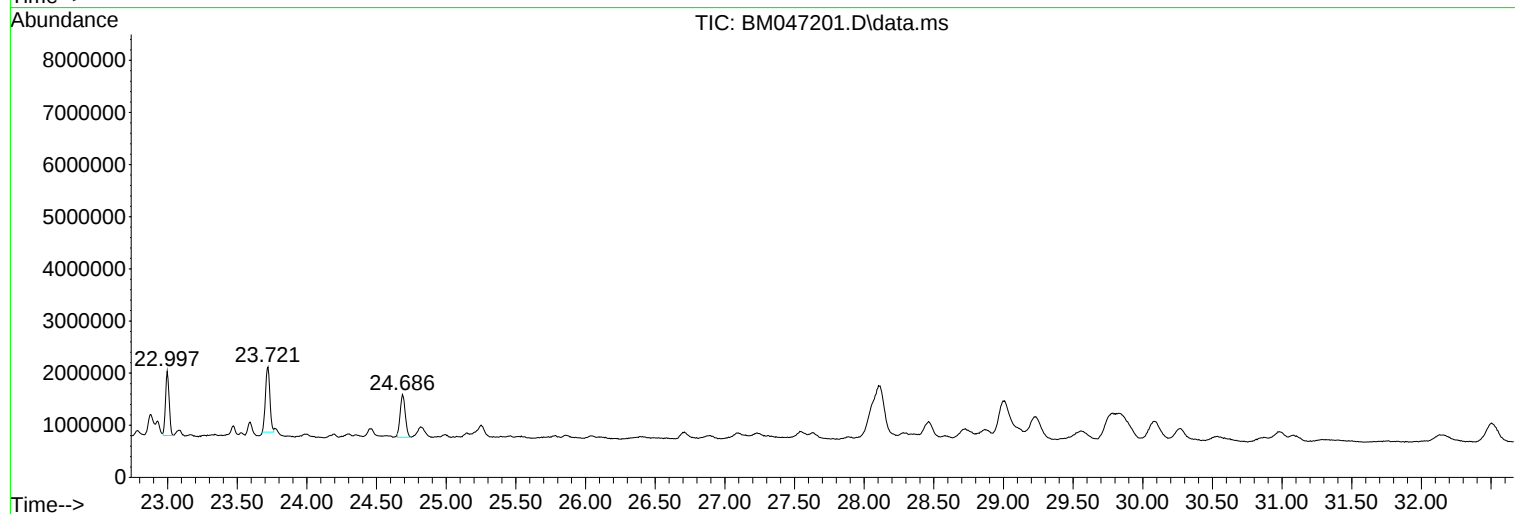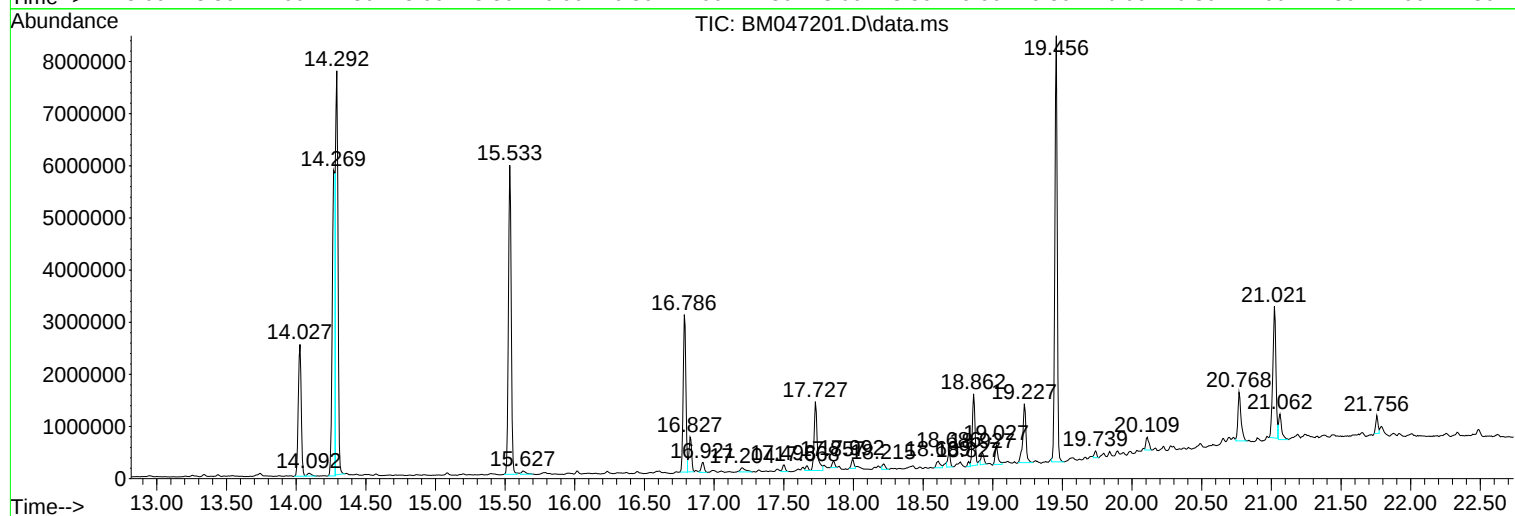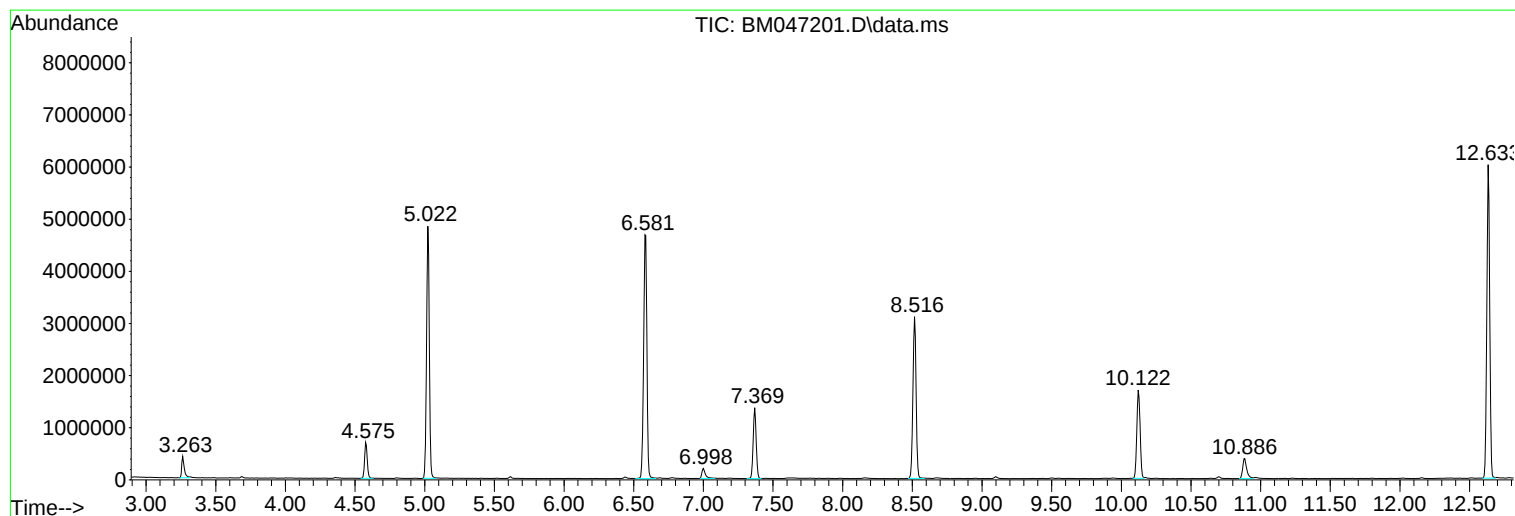

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047201.D
Acq On : 14 Aug 2024 21:31
Operator : RC/JU
Sample : P3519-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-23-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047201.D
Acq On : 14 Aug 2024 21:31
Operator : RC/JU
Sample : P3519-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-23-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------