

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047202.D
 Acq On : 14 Aug 2024 22:11
 Operator : RC/JU
 Sample : P3519-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-02-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	61	64	77	rBV	118842	171175	2.42%	0.345%
2	4.575	281	287	298	rBV	322790	441820	6.24%	0.892%
3	5.022	356	363	374	rBV	2301746	3353319	47.36%	6.767%
4	6.581	620	628	643	rBV	2371392	3713760	52.45%	7.495%
5	7.004	695	700	709	rBV2	51500	101702	1.44%	0.205%
6	7.369	755	762	770	rBV	1339821	2033234	28.72%	4.103%
7	8.516	949	957	968	rBV	1543278	2503705	35.36%	5.053%
8	10.122	1220	1230	1242	rBV	1719177	2849292	40.24%	5.750%
9	10.887	1353	1360	1370	rBV	156172	326492	4.61%	0.659%
10	12.633	1650	1657	1667	rBV	4058516	5841680	82.51%	11.789%
11	14.027	1887	1894	1902	rBV	2632928	3832542	54.13%	7.734%
12	14.263	1928	1934	1935	rBV	234538	283526	4.00%	0.572%
13	14.280	1935	1937	1947	rVB	270483	346303	4.89%	0.699%
14	15.533	2144	2150	2161	rBV	3155173	4375791	61.80%	8.831%
15	16.786	2358	2363	2373	rVB	3126056	4272499	60.35%	8.622%
16	17.498	2481	2484	2490	rVB	69509	85071	1.20%	0.172%
17	17.727	2518	2523	2530	rBV	349946	556218	7.86%	1.122%
18	18.686	2683	2686	2690	rVB4	61936	72989	1.03%	0.147%
19	19.027	2740	2744	2751	rBV2	143942	243658	3.44%	0.492%
20	19.451	2811	2816	2822	rBV	5669711	7080003	100.00%	14.288%
21	20.768	3037	3040	3048	rVB2	242297	370870	5.24%	0.748%
22	21.021	3078	3083	3089	rBV	2562653	3333088	47.08%	6.726%
23	23.721	3535	3542	3559	rVB	1360499	3363807	47.51%	6.788%




Sum of corrected areas: 49552544

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047202.D
Acq On : 14 Aug 2024 22:11
Operator : RC/JU
Sample : P3519-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-02-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

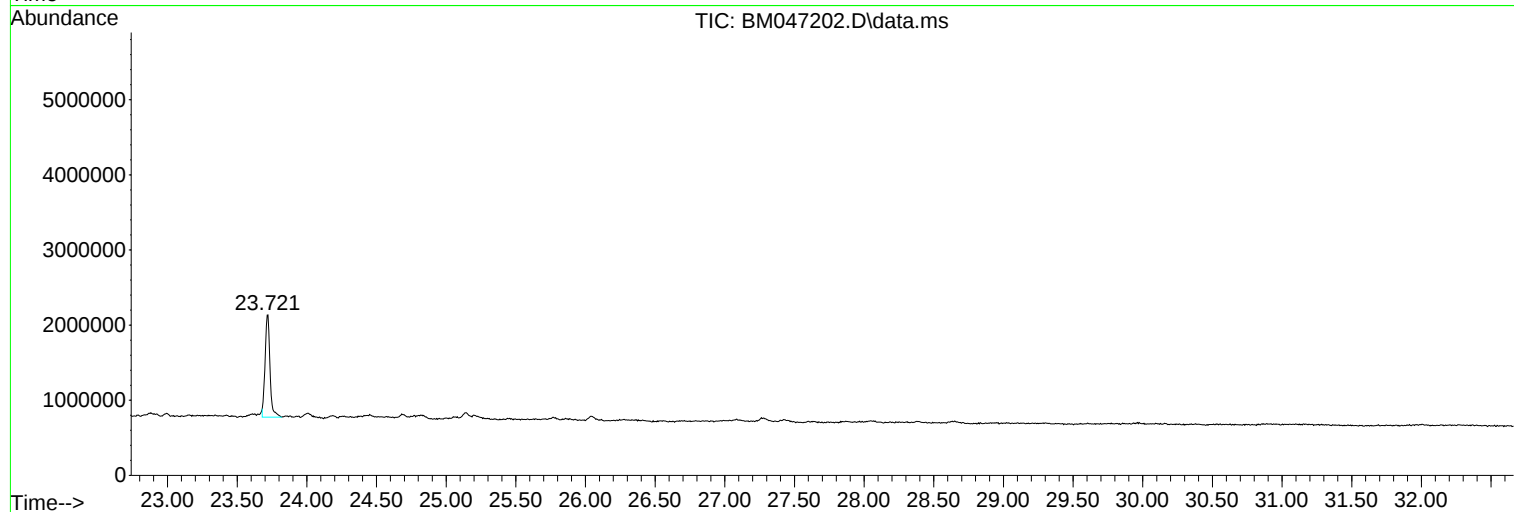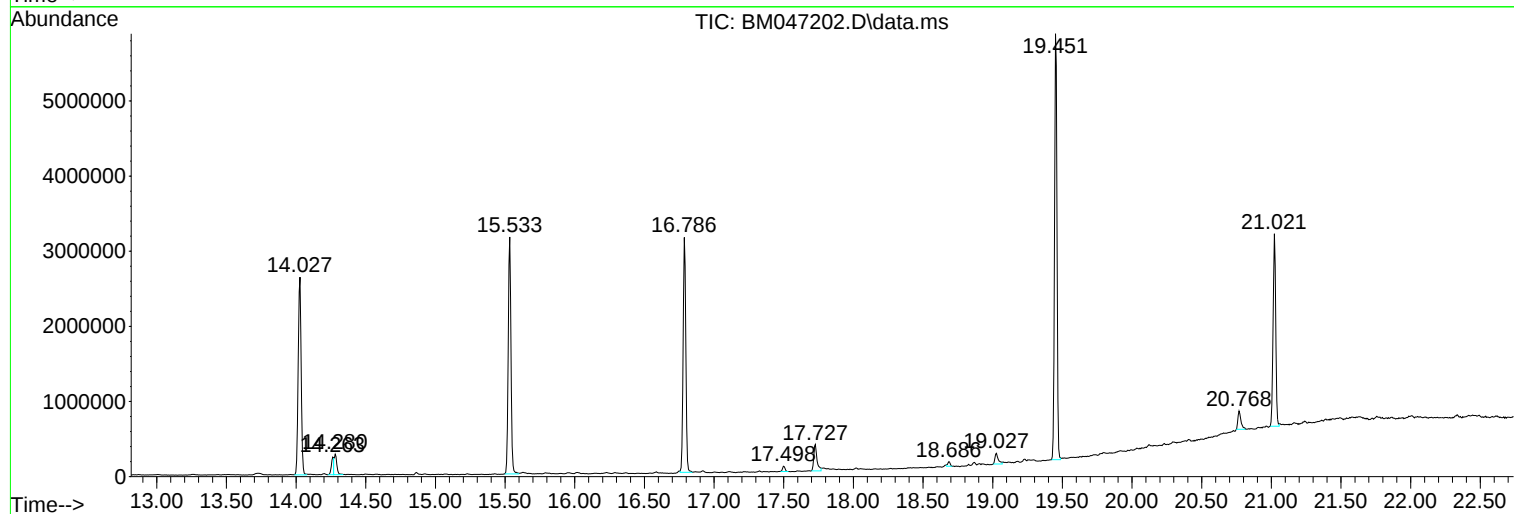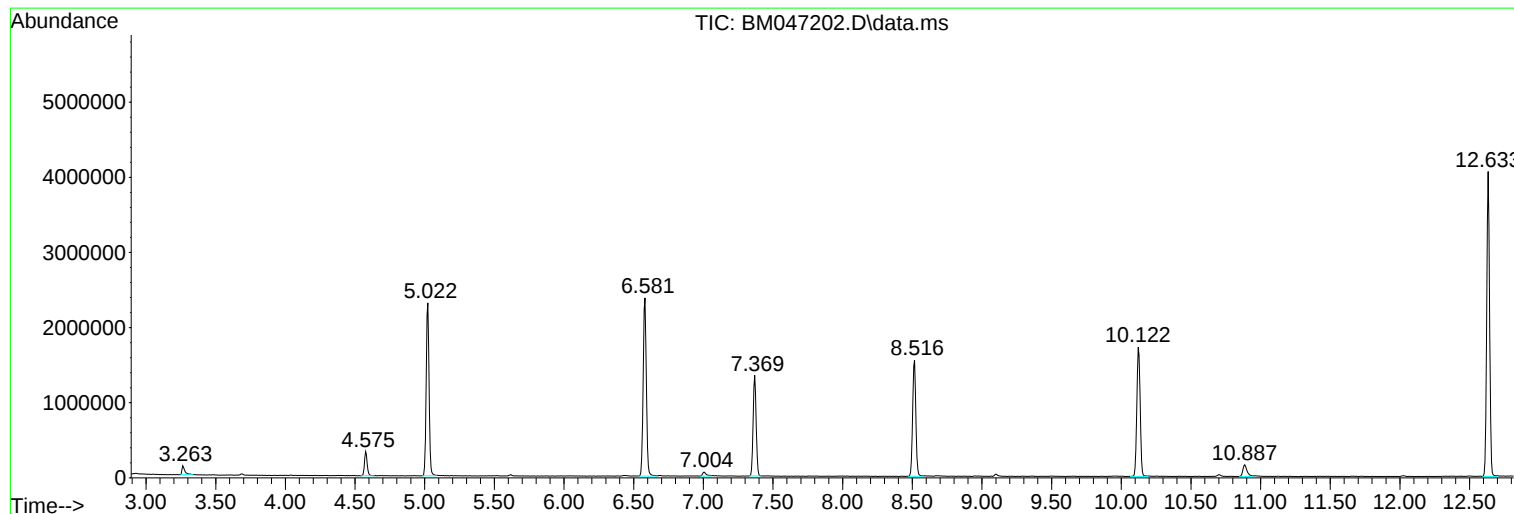

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047202.D
Acq On : 14 Aug 2024 22:11
Operator : RC/JU
Sample : P3519-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-02-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047202.D
Acq On : 14 Aug 2024 22:11
Operator : RC/JU
Sample : P3519-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-02-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------