

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047204.D
 Acq On : 14 Aug 2024 23:30
 Operator : RC/JU
 Sample : P3519-23
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-04-080624

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.575	280	287	295	rBV	546209	735067	7.09%	1.074%
2	5.022	356	363	376	rBV	3770826	5260836	50.71%	7.685%
3	6.581	619	628	641	rBV	3681128	5671400	54.67%	8.285%
4	7.004	695	700	709	rBV	60873	137634	1.33%	0.201%
5	7.369	753	762	771	rBV	1337100	2019911	19.47%	2.951%
6	8.516	949	957	970	rBV	2401224	3850693	37.12%	5.625%
7	10.122	1222	1230	1240	rBV	1665158	2755152	26.56%	4.025%
8	10.886	1352	1360	1371	rBV	275307	576800	5.56%	0.843%
9	12.633	1650	1657	1667	rBV	5756520	8763569	84.47%	12.802%
10	14.027	1887	1894	1903	rBV	2628660	3700207	35.67%	5.405%
11	14.263	1927	1934	1936	rBV	1453521	2140687	20.63%	3.127%
12	14.286	1936	1938	1952	rVB	1702125	1839418	17.73%	2.687%
13	15.533	2137	2150	2163	rBV	4543206	6706694	64.65%	9.797%
14	15.898	2208	2212	2217	rBV	124869	166775	1.61%	0.244%
15	15.962	2217	2223	2228	rVB3	109050	196138	1.89%	0.287%
16	16.015	2228	2232	2237	rBV2	107203	171223	1.65%	0.250%
17	16.215	2261	2266	2274	rVB3	120222	246405	2.38%	0.360%
18	16.286	2274	2278	2283	rVV	161836	239258	2.31%	0.350%
19	16.357	2287	2290	2296	rVB	93451	134851	1.30%	0.197%
20	16.786	2358	2363	2373	rVB	3035039	4127930	39.79%	6.030%
21	17.498	2480	2484	2492	rVB	88798	118970	1.15%	0.174%
22	17.727	2517	2523	2530	rBV	486436	771115	7.43%	1.126%
23	18.686	2680	2686	2690	rVB2	105941	144237	1.39%	0.211%
24	19.027	2739	2744	2749	rBV3	184294	303708	2.93%	0.444%
25	19.274	2783	2786	2795	rVB	170180	325695	3.14%	0.476%
26	19.456	2811	2817	2822	rBV	8173309	10374596	100.00%	15.155%
27	20.768	3036	3040	3050	rBV	600324	993923	9.58%	1.452%
28	21.021	3078	3083	3089	rBV2	2389173	3186680	30.72%	4.655%
29	23.715	3535	3541	3549	rVB	1304582	2796588	26.96%	4.085%




Sum of corrected areas: 68456160

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047204.D
Acq On : 14 Aug 2024 23:30
Operator : RC/JU
Sample : P3519-23
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-04-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

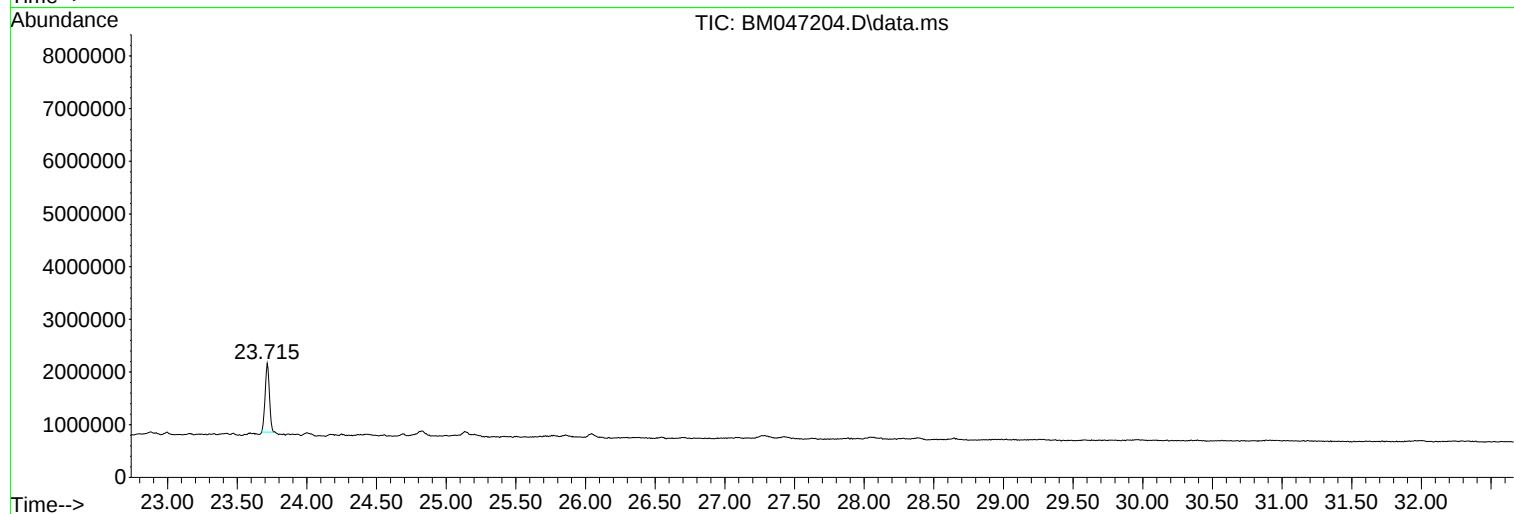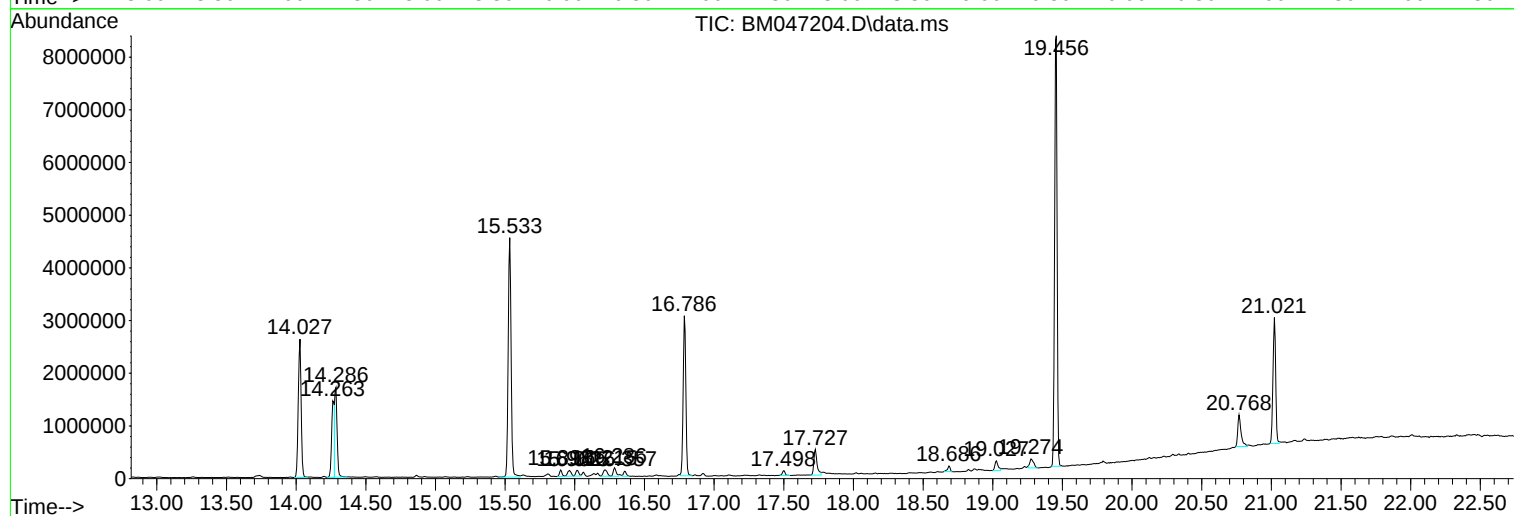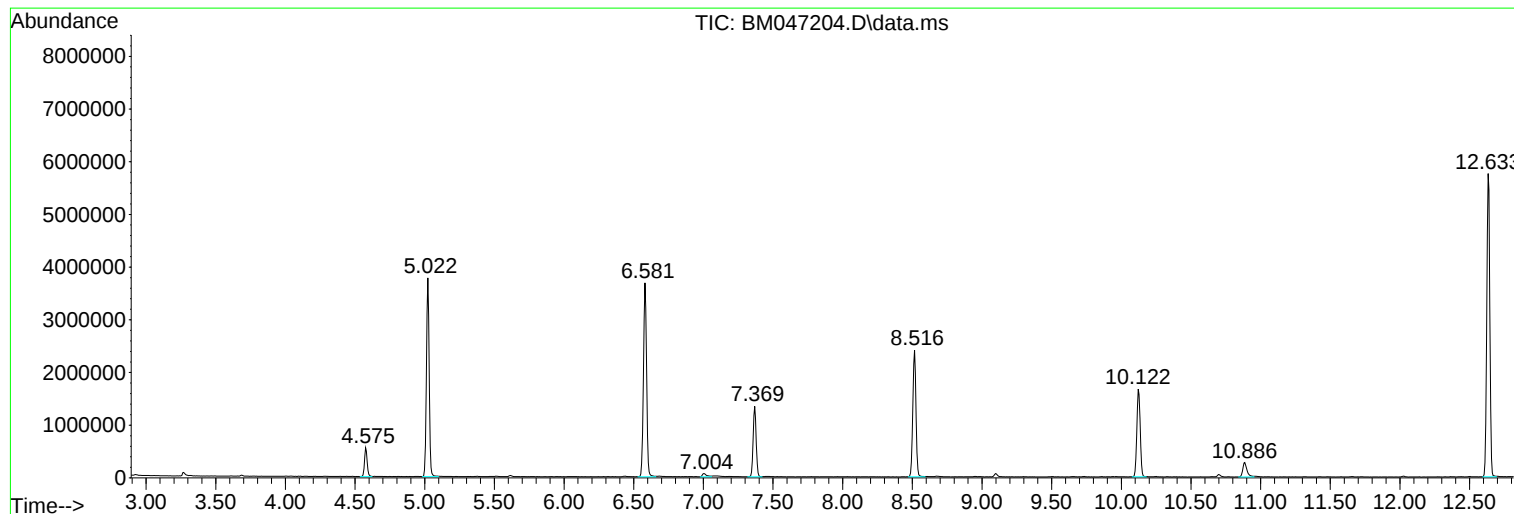

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047204.D
Acq On : 14 Aug 2024 23:30
Operator : RC/JU
Sample : P3519-23
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-04-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047204.D
Acq On : 14 Aug 2024 23:30
Operator : RC/JU
Sample : P3519-23
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-04-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------