

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047205.D
 Acq On : 15 Aug 2024 00:10
 Operator : RC/JU
 Sample : P3519-25
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-05-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	62	65	71	rBV	75467	109441	1.64%	0.211%
2	4.575	281	287	297	rVB	404540	544676	8.17%	1.048%
3	5.022	357	363	377	rBV	2971944	4173269	62.60%	8.031%
4	6.581	619	628	641	rBV	3038205	4697634	70.47%	9.040%
5	7.004	696	700	710	rBV2	42251	81664	1.23%	0.157%
6	7.369	755	762	770	rBV	1419482	2103211	31.55%	4.047%
7	8.516	949	957	968	rBV	1832112	2956818	44.35%	5.690%
8	10.122	1223	1230	1241	rBV	1728165	2915565	43.74%	5.610%
9	10.886	1353	1360	1371	rBV	173778	362708	5.44%	0.698%
10	12.633	1650	1657	1668	rBV	3956704	5897499	88.47%	11.349%
11	13.739	1835	1845	1855	rVB4	40519	106161	1.59%	0.204%
12	14.027	1887	1894	1901	rBV	2667782	3949522	59.24%	7.600%
13	14.263	1927	1934	1935	rBV	101480	126298	1.89%	0.243%
14	14.280	1935	1937	1948	rVB3	118959	160149	2.40%	0.308%
15	15.533	2143	2150	2163	rBV	3676484	5119029	76.79%	9.851%
16	16.786	2358	2363	2369	rBV	3100227	4231783	63.48%	8.143%
17	17.498	2480	2484	2490	rVB	64108	84897	1.27%	0.163%
18	17.727	2518	2523	2532	rBV2	306455	519917	7.80%	1.000%
19	18.862	2712	2716	2721	rBV	174184	231688	3.48%	0.446%
20	19.027	2740	2744	2750	rBV3	124487	202199	3.03%	0.389%
21	19.227	2775	2778	2782	rVB	132294	153429	2.30%	0.295%
22	19.450	2811	2816	2826	rBV	5322362	6666431	100.00%	12.828%
23	20.768	3037	3040	3050	rVB3	303481	485983	7.29%	0.935%
24	21.021	3078	3083	3088	rBV	2452388	3209924	48.15%	6.177%
25	23.715	3535	3541	3551	rVB	1302490	2876865	43.15%	5.536%




Sum of corrected areas: 51966760

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047205.D
Acq On : 15 Aug 2024 00:10
Operator : RC/JU
Sample : P3519-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-05-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

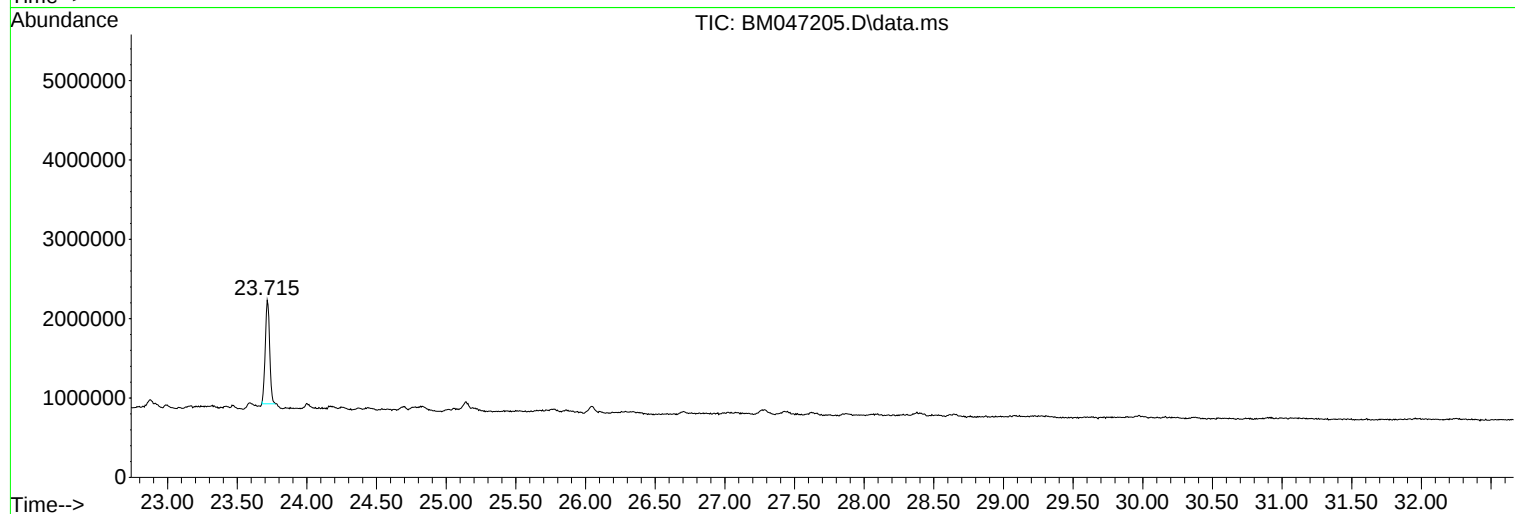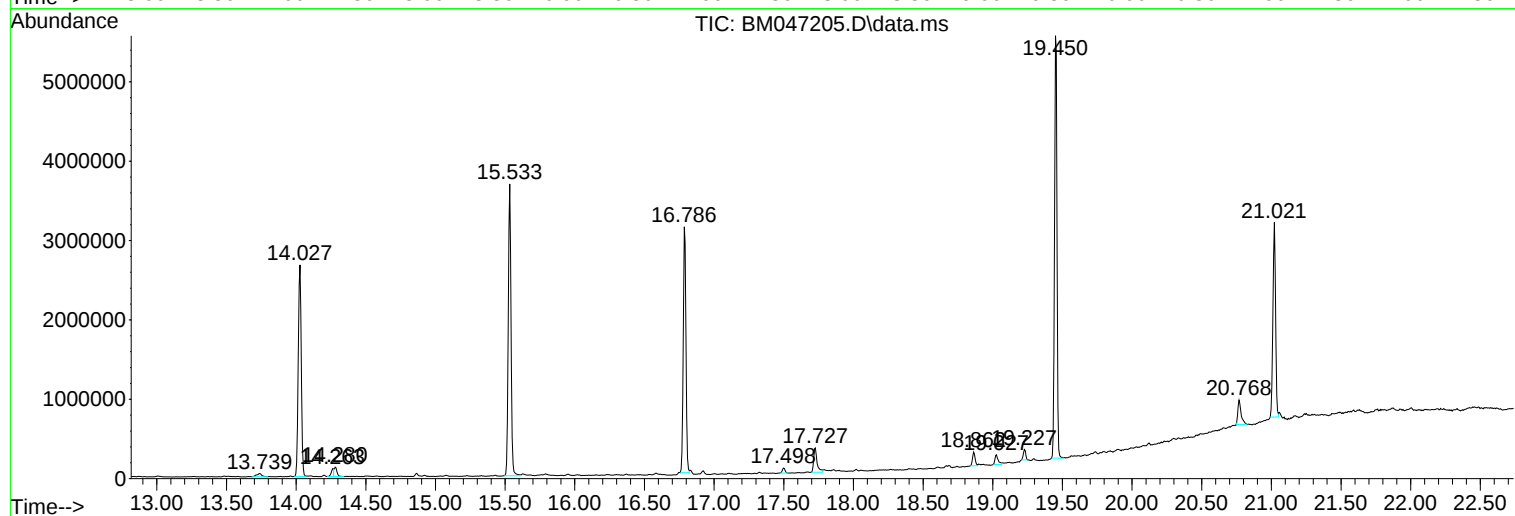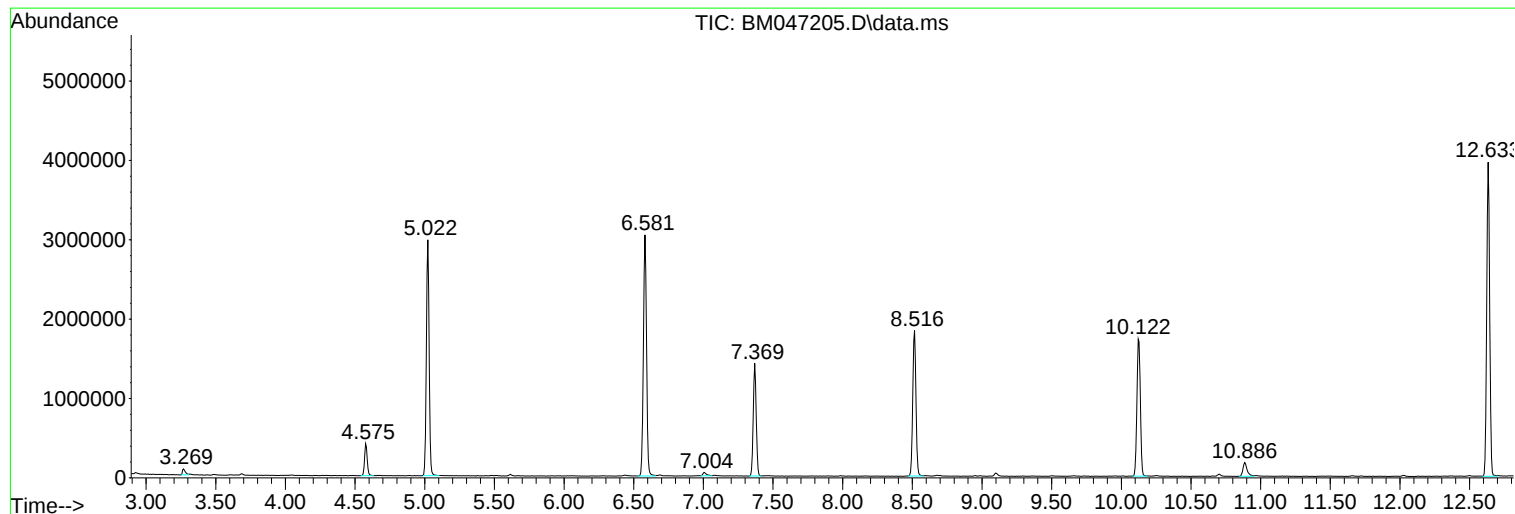

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047205.D
Acq On : 15 Aug 2024 00:10
Operator : RC/JU
Sample : P3519-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-05-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047205.D
Acq On : 15 Aug 2024 00:10
Operator : RC/JU
Sample : P3519-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-05-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------