

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047206.D
 Acq On : 15 Aug 2024 00:50
 Operator : RC/JU
 Sample : P3519-27
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-06-080624

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	62	65	72	rBV	120328	175341	2.51%	0.304%
2	4.575	281	287	295	rBV	517355	708961	10.14%	1.227%
3	5.022	357	363	376	rBV	3805933	5327177	76.19%	9.222%
4	6.581	620	628	641	rBV	3752513	5810354	83.10%	10.059%
5	7.004	695	700	712	rBV	67668	135682	1.94%	0.235%
6	7.369	753	762	771	rBV	1535717	2292469	32.79%	3.969%
7	8.516	949	957	969	rBV	2365651	3727134	53.30%	6.452%
8	9.098	1052	1056	1064	rBV2	52096	83248	1.19%	0.144%
9	10.122	1222	1230	1239	rBV	1861446	3102562	44.37%	5.371%
10	10.887	1351	1360	1371	rBV	221362	464474	6.64%	0.804%
11	12.633	1649	1657	1668	rBV	4742077	6926945	99.07%	11.992%
12	13.733	1835	1844	1854	rBV7	35769	100460	1.44%	0.174%
13	14.028	1887	1894	1904	rBV	2810692	4053071	57.97%	7.017%
14	14.263	1928	1934	1935	rBV	137603	168638	2.41%	0.292%
15	14.280	1935	1937	1942	rVB2	147321	197340	2.82%	0.342%
16	15.533	2143	2150	2163	rBV	4264200	6042172	86.41%	10.460%
17	16.786	2358	2363	2374	rVB	3046100	4212007	60.24%	7.292%
18	17.498	2480	2484	2493	rVB	80697	113551	1.62%	0.197%
19	17.727	2518	2523	2531	rBV	326905	529558	7.57%	0.917%
20	19.021	2740	2743	2753	rBV2	114163	173124	2.48%	0.300%
21	19.451	2811	2816	2827	rBV	5445361	6992251	100.00%	12.105%
22	20.768	3037	3040	3049	rVB2	284790	471828	6.75%	0.817%
23	21.021	3079	3083	3089	rVB	2284012	2889027	41.32%	5.001%
24	23.721	3535	3542	3555	rVB	1301912	3067178	43.87%	5.310%




Sum of corrected areas: 57764552

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047206.D
Acq On : 15 Aug 2024 00:50
Operator : RC/JU
Sample : P3519-27
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-06-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

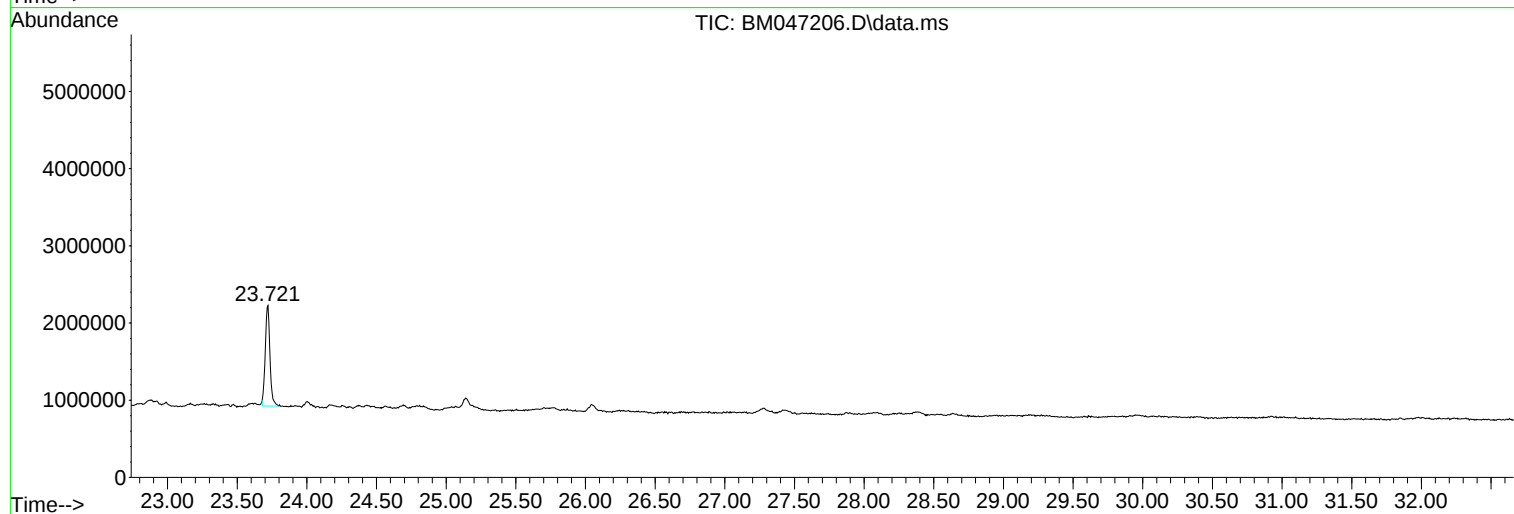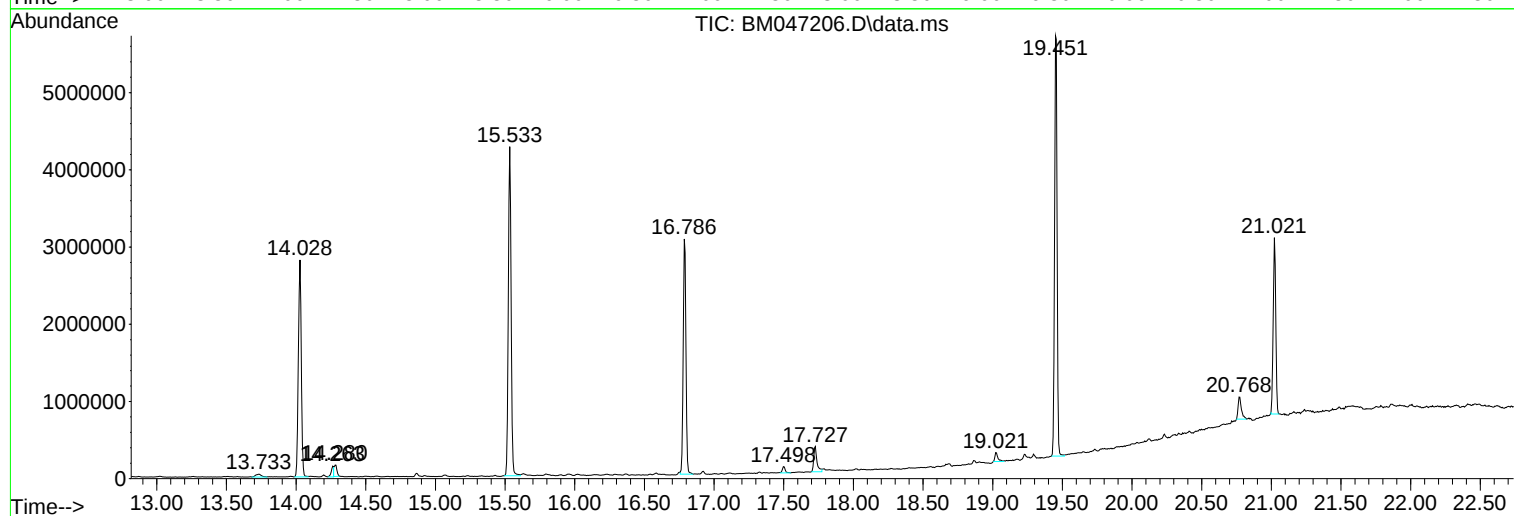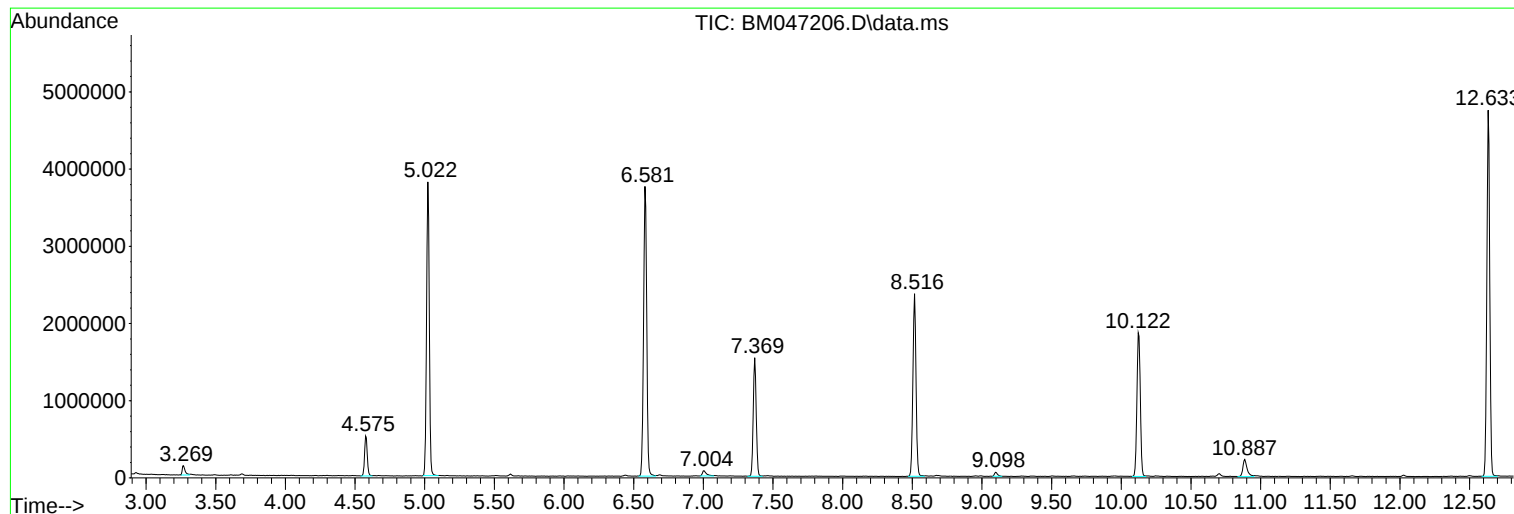

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047206.D
Acq On : 15 Aug 2024 00:50
Operator : RC/JU
Sample : P3519-27
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-06-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047206.D
Acq On : 15 Aug 2024 00:50
Operator : RC/JU
Sample : P3519-27
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-06-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------