

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047212.D
 Acq On : 15 Aug 2024 12:51
 Operator : RC/JU
 Sample : P3520-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-10-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	62	65	73	rBV	75970	108771	1.51%	0.247%
2	4.575	279	287	294	rBV	180245	251098	3.48%	0.571%
3	5.022	356	363	380	rBV	2792131	3949649	54.67%	8.982%
4	6.575	617	627	643	rBV	2590404	4076904	56.43%	9.271%
5	7.363	755	761	770	rBV	921325	1408467	19.49%	3.203%
6	8.510	947	956	968	rBV	1691167	2742733	37.96%	6.237%
7	10.122	1222	1230	1243	rVB	1068224	1795751	24.85%	4.084%
8	10.880	1350	1359	1370	rBV	84376	198330	2.74%	0.451%
9	12.633	1648	1657	1672	rBV	4000934	5896819	81.61%	13.410%
10	14.021	1887	1893	1903	rBV	1536989	2276176	31.50%	5.176%
11	14.263	1927	1934	1935	rBV3	65382	92212	1.28%	0.210%
12	14.280	1935	1937	1946	rVB2	77959	96867	1.34%	0.220%
13	15.527	2143	2149	2166	rBV	2839605	4346234	60.15%	9.884%
14	16.786	2350	2363	2373	rBV	1841142	2588361	35.82%	5.886%
15	16.921	2381	2386	2393	rVB3	51111	79460	1.10%	0.181%
16	17.721	2517	2522	2531	rBV	372953	639940	8.86%	1.455%
17	19.027	2739	2744	2753	rBV	178568	328206	4.54%	0.746%
18	19.280	2783	2787	2795	rBV	116299	210022	2.91%	0.478%
19	19.451	2811	2816	2825	rBV	5823914	7225170	100.00%	16.430%
20	20.774	3037	3041	3053	rBV2	232280	418263	5.79%	0.951%
21	21.021	3078	3083	3091	rBV2	1921232	2551598	35.32%	5.802%
22	23.715	3534	3541	3557	rVB	1177740	2693107	37.27%	6.124%




Sum of corrected areas: 43974138

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047212.D
Acq On : 15 Aug 2024 12:51
Operator : RC/JU
Sample : P3520-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-10-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

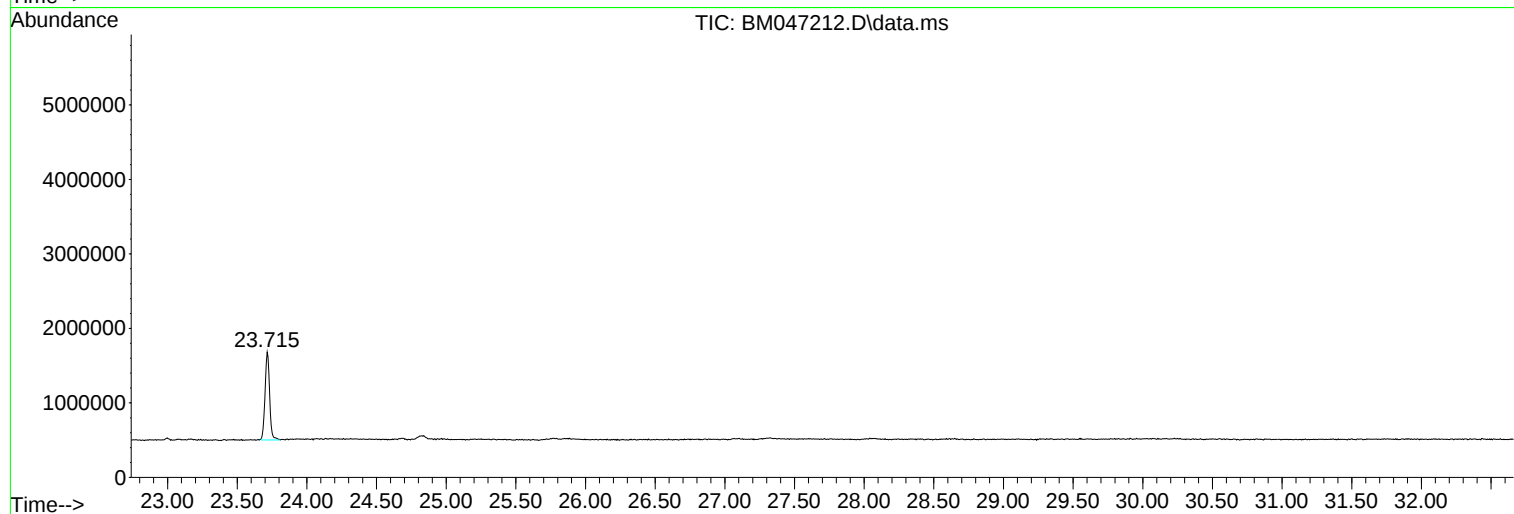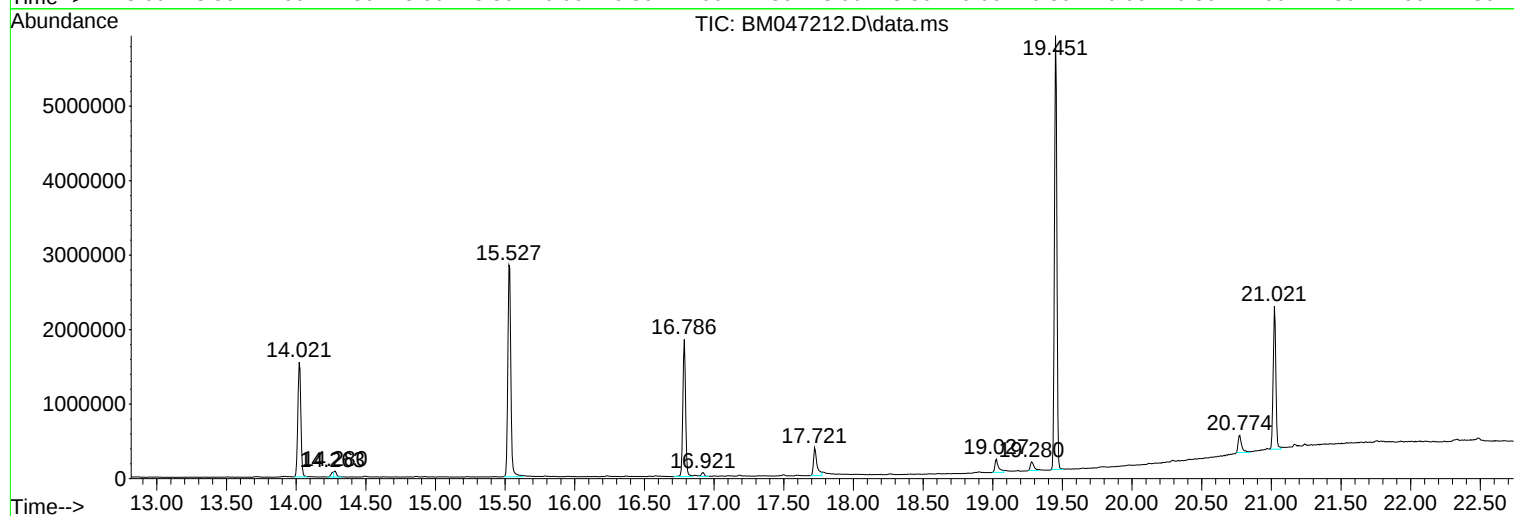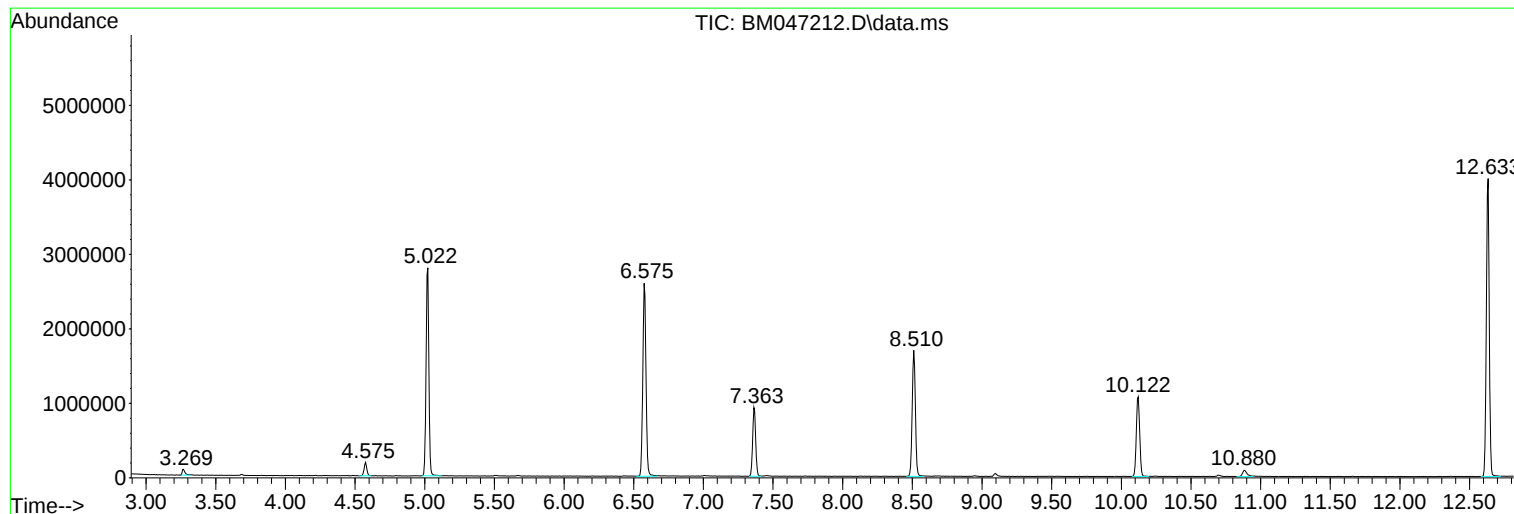

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047212.D
Acq On : 15 Aug 2024 12:51
Operator : RC/JU
Sample : P3520-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-10-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047212.D
Acq On : 15 Aug 2024 12:51
Operator : RC/JU
Sample : P3520-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-10-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------