

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081524\  
 Data File : BM047215.D  
 Acq On : 15 Aug 2024 14:51  
 Operator : RC/JU  
 Sample : P3520-11  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 OU4-CF-13-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047215.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.263       | 62            | 64          | 72           | rBV      | 76266          | 107134        | 1.48%           | 0.228%        |
| 2         | 4.575       | 282           | 287         | 295          | rVB      | 175171         | 230833        | 3.20%           | 0.491%        |
| 3         | 5.016       | 356           | 362         | 373          | rBV      | 2580000        | 3720344       | 51.55%          | 7.919%        |
| 4         | 6.575       | 620           | 627         | 644          | rBV      | 2514214        | 3941963       | 54.62%          | 8.391%        |
| 5         | 7.363       | 752           | 761         | 770          | rBV      | 1145259        | 1778268       | 24.64%          | 3.785%        |
| 6         | 8.510       | 947           | 956         | 968          | rBV      | 1639991        | 2601535       | 36.05%          | 5.538%        |
| 7         | 9.092       | 1050          | 1055        | 1063         | rVB2     | 60665          | 97341         | 1.35%           | 0.207%        |
| 8         | 10.122      | 1222          | 1230        | 1240         | rBV      | 1372640        | 2270399       | 31.46%          | 4.833%        |
| 9         | 10.880      | 1353          | 1359        | 1369         | rBV      | 106798         | 234891        | 3.25%           | 0.500%        |
| 10        | 12.633      | 1648          | 1657        | 1665         | rBV      | 3775910        | 5569310       | 77.17%          | 11.855%       |
| 11        | 14.021      | 1886          | 1893        | 1905         | rBV      | 1915449        | 2807562       | 38.90%          | 5.976%        |
| 12        | 15.533      | 2143          | 2150        | 2161         | rBV      | 2899954        | 4161631       | 57.66%          | 8.858%        |
| 13        | 15.757      | 2183          | 2188        | 2197         | rBV      | 114191         | 187690        | 2.60%           | 0.400%        |
| 14        | 16.786      | 2357          | 2363        | 2375         | rBV      | 2352217        | 3145681       | 43.59%          | 6.696%        |
| 15        | 17.727      | 2518          | 2523        | 2538         | rBV      | 545283         | 1000995       | 13.87%          | 2.131%        |
| 16        | 19.021      | 2739          | 2743        | 2753         | rBV      | 306026         | 545364        | 7.56%           | 1.161%        |
| 17        | 19.450      | 2811          | 2816        | 2825         | rBV      | 5750884        | 7216912       | 100.00%         | 15.362%       |
| 18        | 20.768      | 3036          | 3040        | 3050         | rBV      | 348291         | 699122        | 9.69%           | 1.488%        |
| 19        | 21.021      | 3078          | 3083        | 3089         | rBV2     | 2351939        | 3137948       | 43.48%          | 6.679%        |
| 20        | 23.721      | 3535          | 3542        | 3559         | rVB      | 1487684        | 3524281       | 48.83%          | 7.502%        |




Sum of corrected areas: 46979204

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081524\  
Data File : BM047215.D  
Acq On : 15 Aug 2024 14:51  
Operator : RC/JU  
Sample : P3520-11  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
OU4-CF-13-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

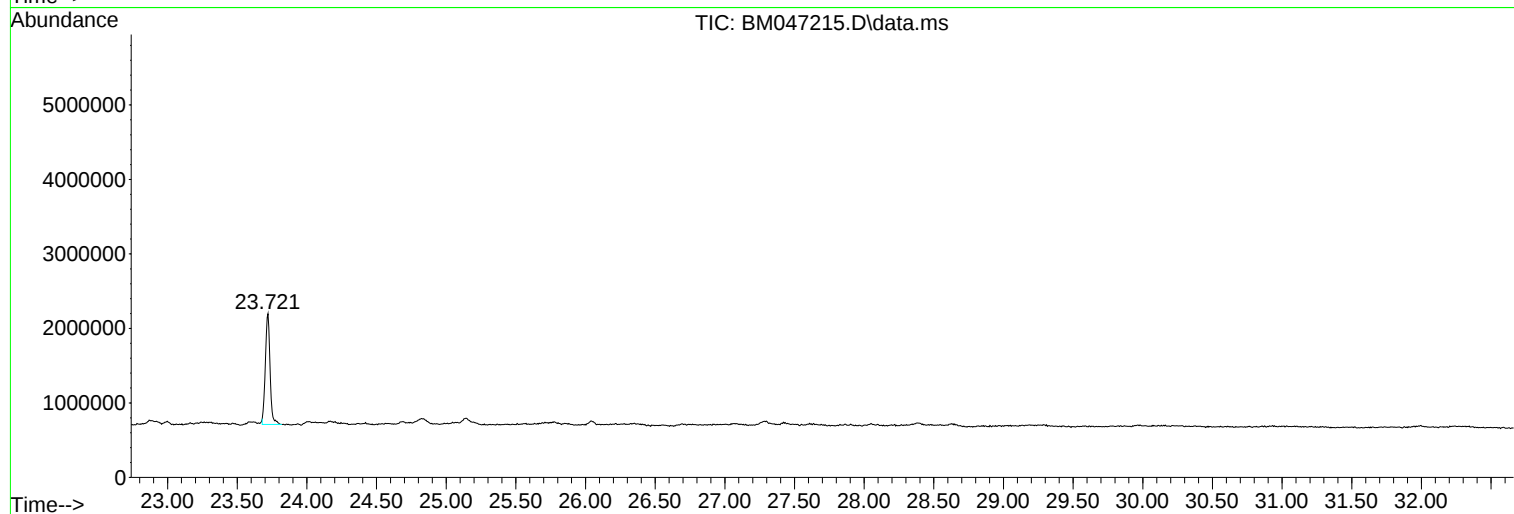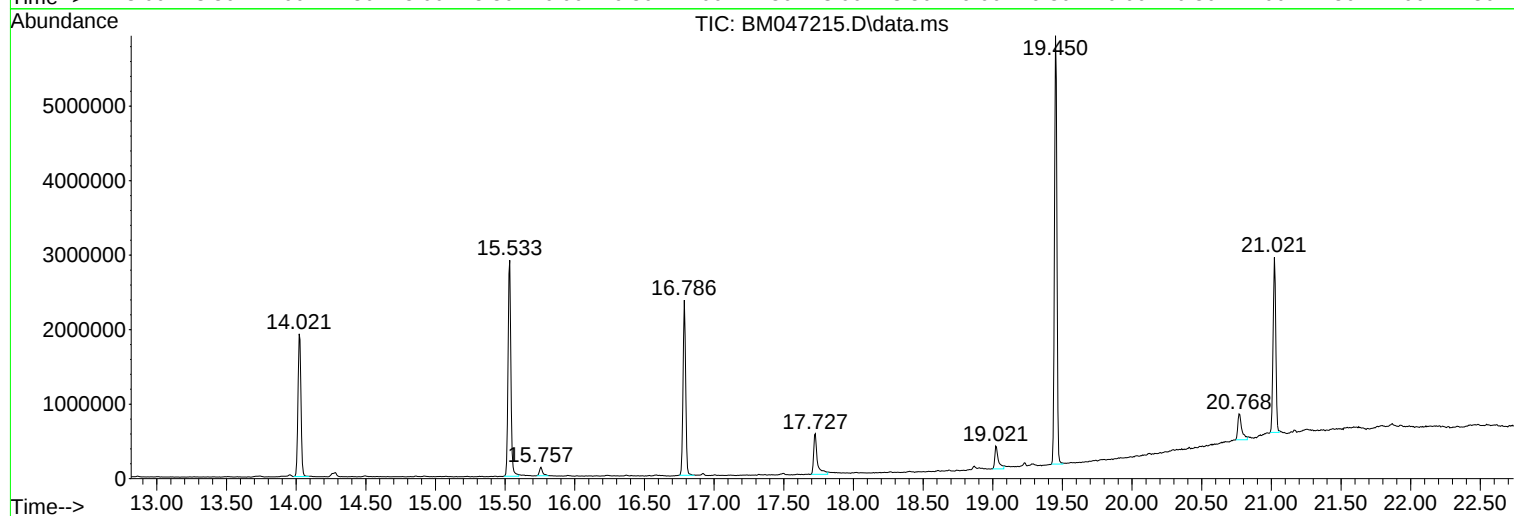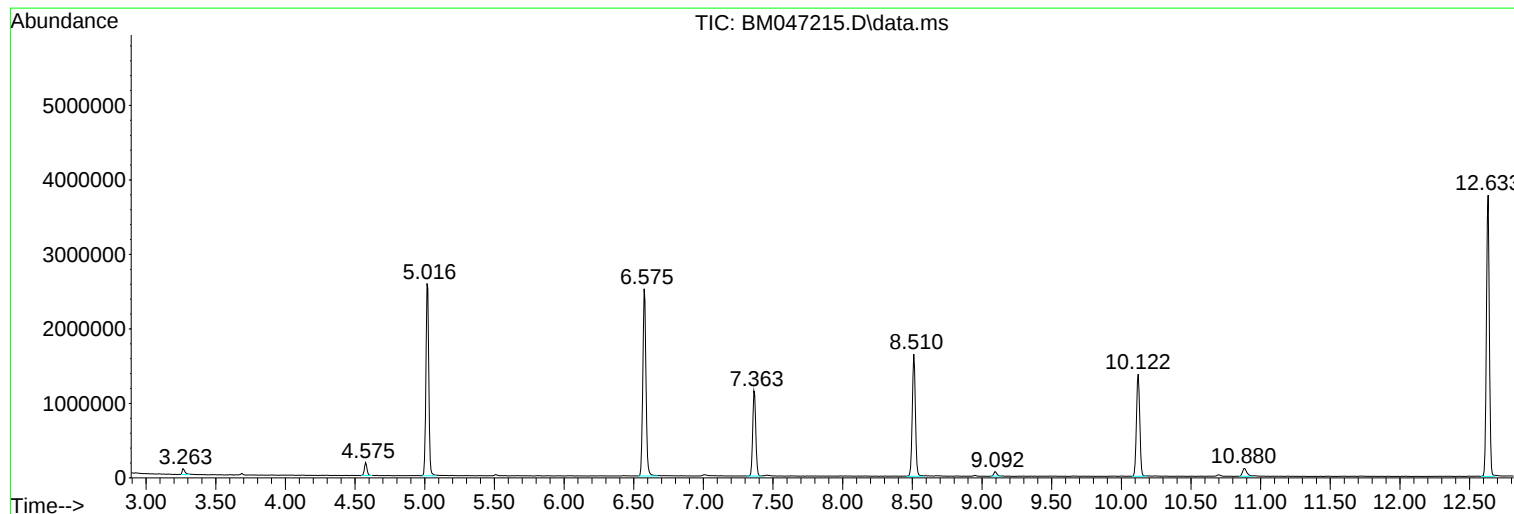

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081524\  
Data File : BM047215.D  
Acq On : 15 Aug 2024 14:51  
Operator : RC/JU  
Sample : P3520-11  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
OU4-CF-13-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM081524\  
Data File : BM047215.D  
Acq On : 15 Aug 2024 14:51  
Operator : RC/JU  
Sample : P3520-11  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
OU4-CF-13-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM081024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|