

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047216.D
 Acq On : 15 Aug 2024 15:31
 Operator : RC/JU
 Sample : P3519-29
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-07-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	61	64	72	rBV	78039	114055	1.97%	0.258%
2	4.575	281	287	294	rBV	382771	496186	8.58%	1.122%
3	5.016	356	362	377	rBV	2604092	3770684	65.22%	8.527%
4	6.575	618	627	641	rBV	2517778	3938767	68.13%	8.907%
5	6.998	695	699	708	rBV	41851	81482	1.41%	0.184%
6	7.363	754	761	769	rBV	1146423	1808182	31.28%	4.089%
7	8.510	948	956	968	rBV	1579237	2532411	43.80%	5.727%
8	10.122	1221	1230	1239	rBV	1444718	2343362	40.53%	5.299%
9	10.881	1352	1359	1370	rBV2	128177	284570	4.92%	0.644%
10	12.633	1650	1657	1667	rBV	3154209	4736874	81.94%	10.712%
11	13.739	1835	1845	1850	rBV3	33426	84520	1.46%	0.191%
12	14.022	1887	1893	1904	rBV	1952792	2862268	49.51%	6.473%
13	14.263	1927	1934	1935	rBV2	113714	159157	2.75%	0.360%
14	14.280	1935	1937	1946	rVB	126181	156074	2.70%	0.353%
15	15.533	2143	2150	2161	rBV	2500687	3755159	64.96%	8.492%
16	16.786	2358	2363	2369	rBV	2174554	3034104	52.48%	6.862%
17	16.916	2382	2385	2394	rVB	41189	58852	1.02%	0.133%
18	17.498	2481	2484	2488	rVB	51839	59275	1.03%	0.134%
19	17.721	2517	2522	2531	rBV	353687	601903	10.41%	1.361%
20	18.862	2712	2716	2721	rBV	173485	228656	3.96%	0.517%
21	19.021	2739	2743	2750	rBV3	187011	315910	5.46%	0.714%
22	19.227	2775	2778	2785	rVB	142102	169119	2.93%	0.382%
23	19.451	2811	2816	2822	rBV	4630928	5781155	100.00%	13.074%
24	20.774	3038	3041	3050	rVB3	191035	325760	5.63%	0.737%
25	21.021	3078	3083	3089	rBV	2229055	3168492	54.81%	7.166%
26	23.721	3535	3542	3559	rVB	1387243	3351608	57.97%	7.580%




Sum of corrected areas: 44218585

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047216.D
Acq On : 15 Aug 2024 15:31
Operator : RC/JU
Sample : P3519-29
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-07-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

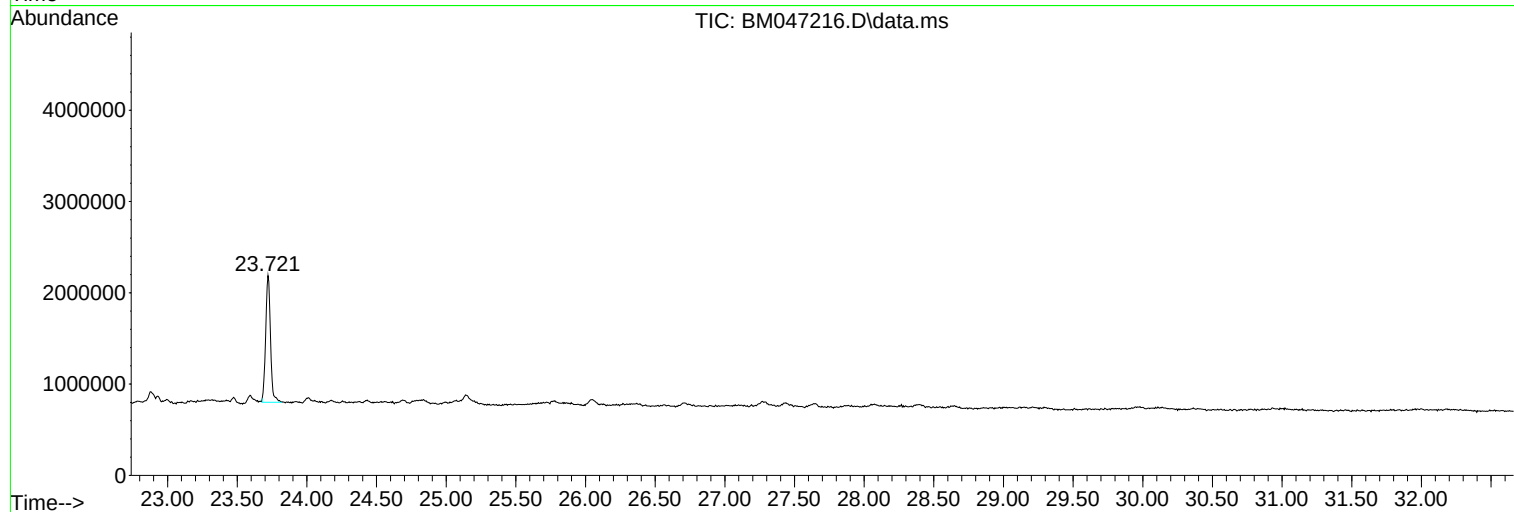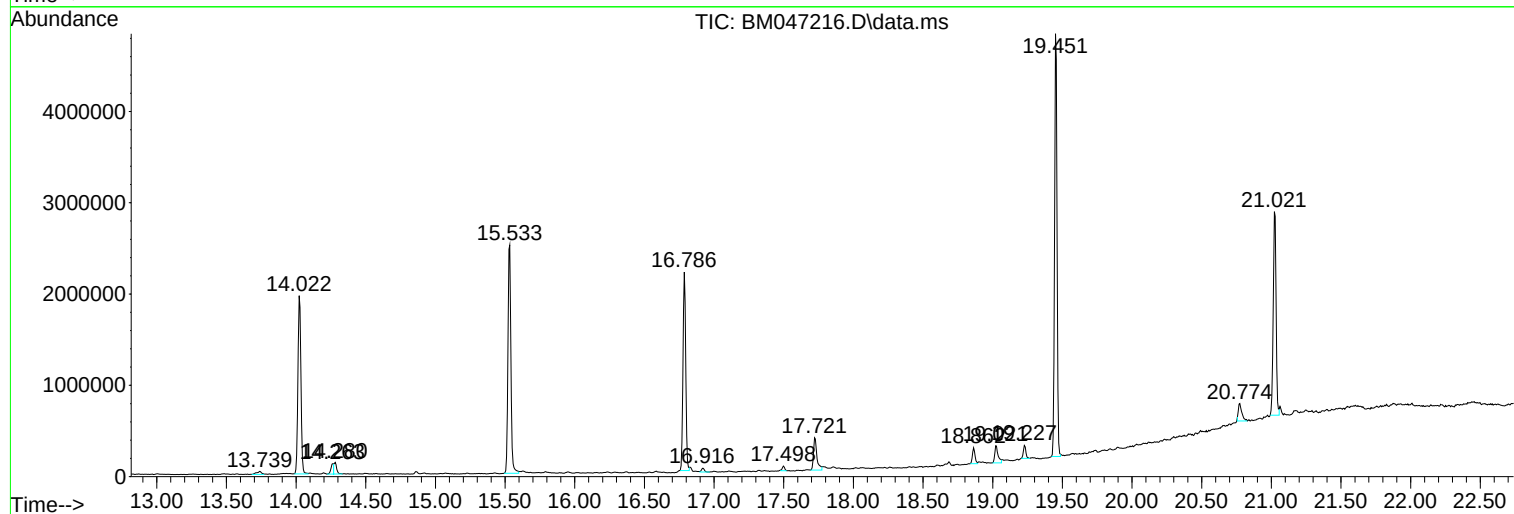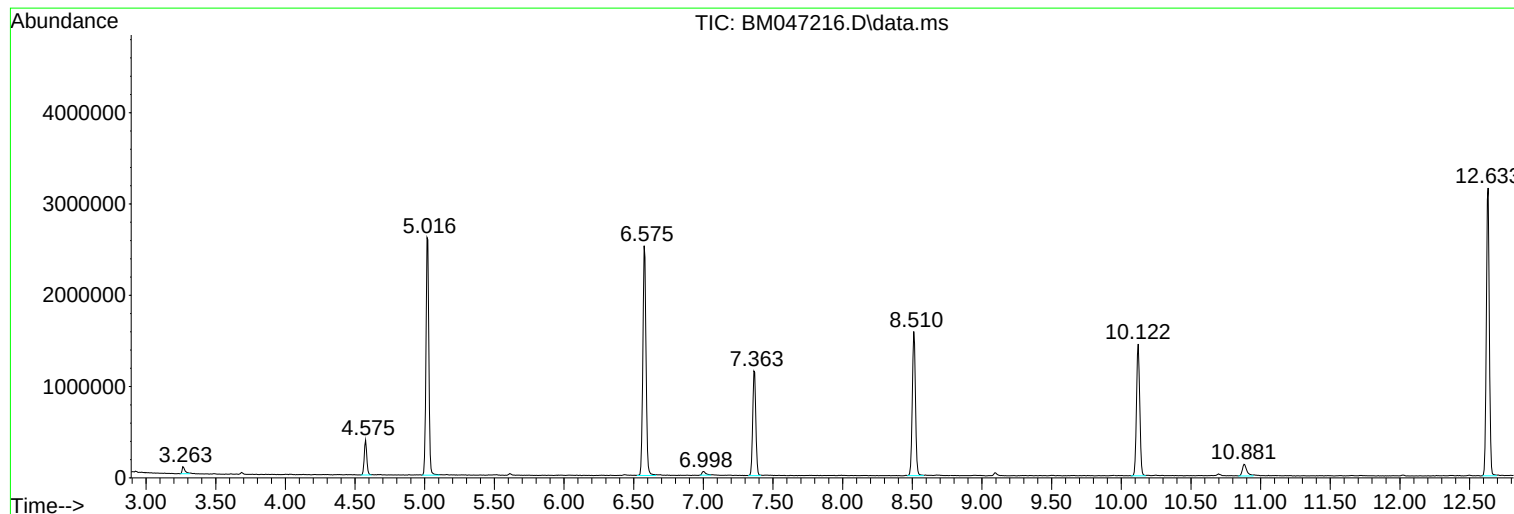

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047216.D
Acq On : 15 Aug 2024 15:31
Operator : RC/JU
Sample : P3519-29
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-07-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047216.D
Acq On : 15 Aug 2024 15:31
Operator : RC/JU
Sample : P3519-29
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-07-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------