

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047217.D
 Acq On : 15 Aug 2024 16:11
 Operator : RC/JU
 Sample : P3518-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-01-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	61	64	73	rBV	81802	110770	2.60%	0.240%
2	4.575	280	287	292	rBV	194041	253711	5.95%	0.550%
3	5.022	356	363	378	rBV	2569583	3669926	86.11%	7.954%
4	6.575	620	627	642	rBV	2347221	3730858	87.53%	8.086%
5	6.998	695	699	710	rBV	53868	99892	2.34%	0.216%
6	7.369	752	762	768	rBV	1257222	1968275	46.18%	4.266%
7	8.510	949	956	966	rBV	1632314	2625383	61.60%	5.690%
8	10.122	1222	1230	1242	rBV	1540935	2510404	58.90%	5.441%
9	10.880	1353	1359	1369	rBV	175299	362207	8.50%	0.785%
10	12.633	1650	1657	1677	rBV	2821632	4262135	100.00%	9.237%
11	14.027	1887	1894	1902	rBV	1959619	2984515	70.02%	6.468%
12	14.263	1927	1934	1935	rBV	772027	987670	23.17%	2.141%
13	14.280	1935	1937	1947	rVB	959181	1169601	27.44%	2.535%
14	15.533	2143	2150	2163	rBV	2255048	3332930	78.20%	7.223%
15	15.627	2163	2166	2177	rVB	25297	66096	1.55%	0.143%
16	16.233	2264	2269	2276	rBV3	38529	64053	1.50%	0.139%
17	16.786	2357	2363	2368	rBV	2291812	3099563	72.72%	6.718%
18	16.827	2368	2370	2374	rVB	196981	231300	5.43%	0.501%
19	16.915	2382	2385	2391	rVB2	58463	80193	1.88%	0.174%
20	16.998	2394	2399	2405	rBV7	26231	46852	1.10%	0.102%
21	17.498	2481	2484	2491	rVB2	57795	81420	1.91%	0.176%
22	17.592	2496	2500	2504	rBV5	53116	80833	1.90%	0.175%
23	17.727	2517	2523	2531	rBV2	552243	930394	21.83%	2.016%
24	17.856	2541	2545	2549	rBV2	41265	60186	1.41%	0.130%
25	17.992	2565	2568	2572	rBV4	42222	54047	1.27%	0.117%
26	18.603	2668	2672	2677	rBV2	40491	78681	1.85%	0.171%
27	18.686	2683	2686	2690	rVB3	104009	121729	2.86%	0.264%
28	18.862	2712	2716	2720	rBV	338509	438576	10.29%	0.951%
29	19.027	2739	2744	2751	rBV2	227676	379020	8.89%	0.821%
30	19.227	2774	2778	2785	rVB	294653	376151	8.83%	0.815%
31	19.450	2811	2816	2826	rVB	3180546	3878809	91.01%	8.406%
32	20.768	3037	3040	3050	rVB4	244592	435180	10.21%	0.943%
33	21.021	3078	3083	3088	rBV	2148545	3075076	72.15%	6.664%
34	22.486	3328	3332	3338	rVB	450824	702747	16.49%	1.523%
35	22.997	3416	3419	3425	rVB	327298	537380	12.61%	1.165%
36	23.721	3535	3542	3559	rVB	1418307	3254949	76.37%	7.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047217.D
Acq On : 15 Aug 2024 16:11
Operator : RC/JU
Sample : P3518-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-01-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 46141512

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047217.D
Acq On : 15 Aug 2024 16:11
Operator : RC/JU
Sample : P3518-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-01-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

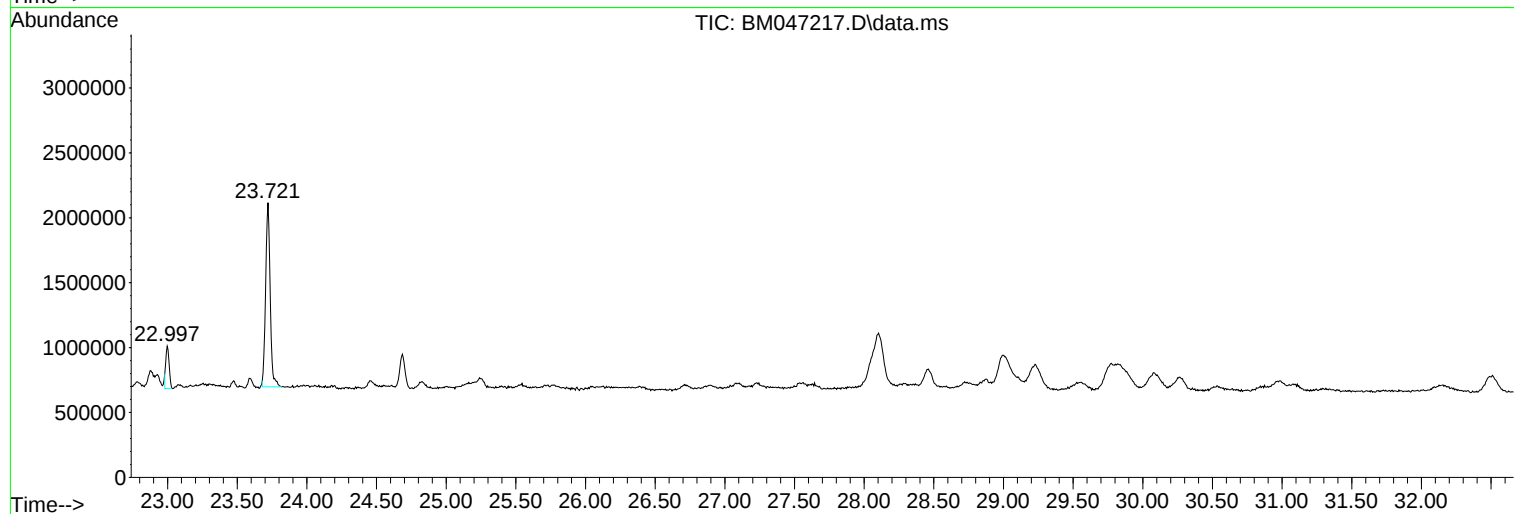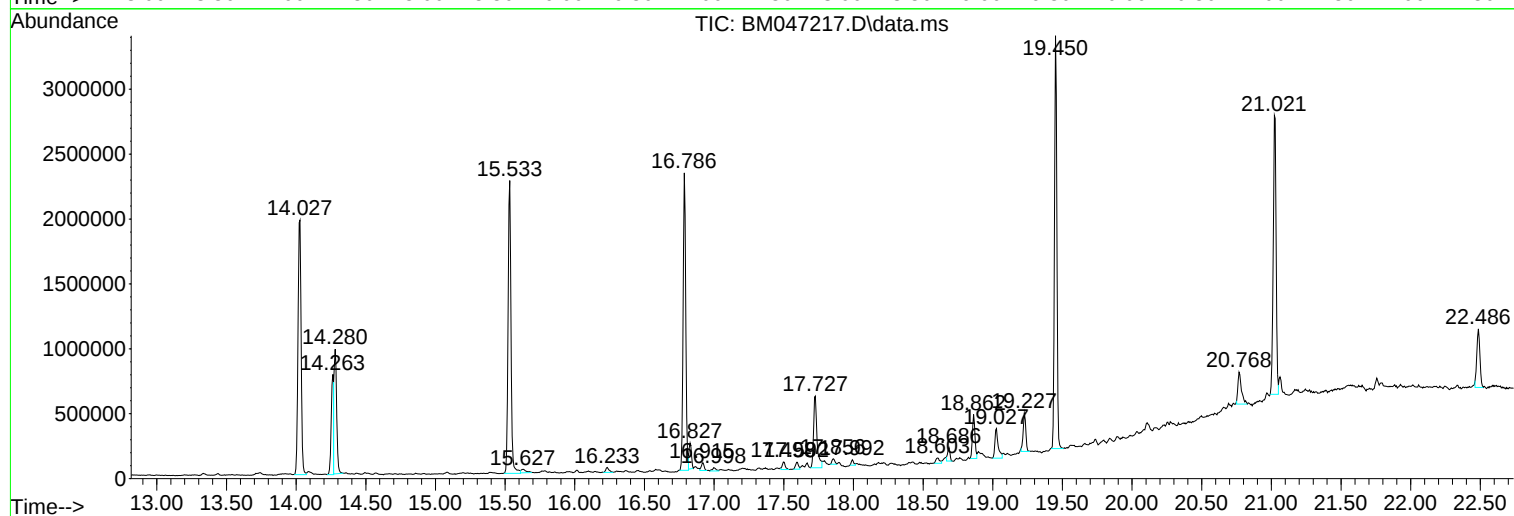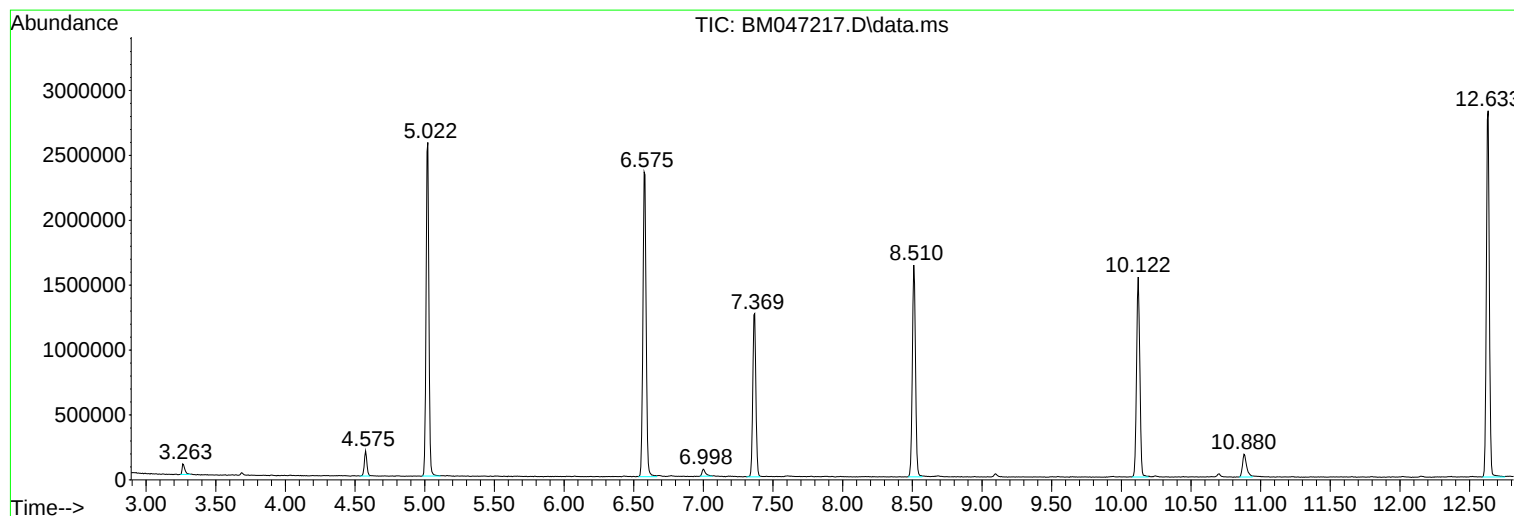

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047217.D
Acq On : 15 Aug 2024 16:11
Operator : RC/JU
Sample : P3518-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-01-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047217.D
Acq On : 15 Aug 2024 16:11
Operator : RC/JU
Sample : P3518-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-01-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------