

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047219.D
 Acq On : 15 Aug 2024 17:32
 Operator : RC/JU
 Sample : P3520-09RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-CF-12-080624RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	62	65	72	rBV	53893	75993	1.26%	0.181%
2	4.575	280	287	296	rBV	152128	206111	3.41%	0.491%
3	5.016	355	362	374	rBV	2489065	3617382	59.86%	8.611%
4	6.575	620	627	643	rBV	2404997	3758526	62.19%	8.947%
5	7.363	754	761	770	rBV	1085186	1688202	27.93%	4.019%
6	8.510	949	956	968	rBV	1543285	2482515	41.08%	5.910%
7	9.098	1048	1056	1066	rBV2	35023	62847	1.04%	0.150%
8	10.122	1222	1230	1240	rBV	1279879	2118115	35.05%	5.042%
9	10.886	1352	1360	1371	rBV	64936	150952	2.50%	0.359%
10	12.633	1650	1657	1671	rBV	3404831	5184100	85.78%	12.341%
11	14.021	1886	1893	1903	rBV	1705573	2531008	41.88%	6.025%
12	14.280	1928	1937	1946	rBV	339750	768835	12.72%	1.830%
13	15.533	2143	2150	2164	rBV	2483197	3640620	60.24%	8.666%
14	16.786	2357	2363	2373	rBV	1941301	2678110	44.31%	6.375%
15	17.721	2517	2522	2534	rBV	341215	606973	10.04%	1.445%
16	19.027	2739	2744	2753	rBV	174588	323650	5.36%	0.770%
17	19.174	2766	2769	2773	rVB2	67930	67837	1.12%	0.161%
18	19.450	2811	2816	2828	rBV	4919974	6043423	100.00%	14.386%
19	20.768	3037	3040	3050	rVB2	226181	362961	6.01%	0.864%
20	21.021	3078	3083	3090	rBV	1961311	2693422	44.57%	6.412%
21	23.721	3535	3542	3559	rVB	1277581	2946732	48.76%	7.015%




Sum of corrected areas: 42008314

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047219.D
Acq On : 15 Aug 2024 17:32
Operator : RC/JU
Sample : P3520-09RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-12-080624RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

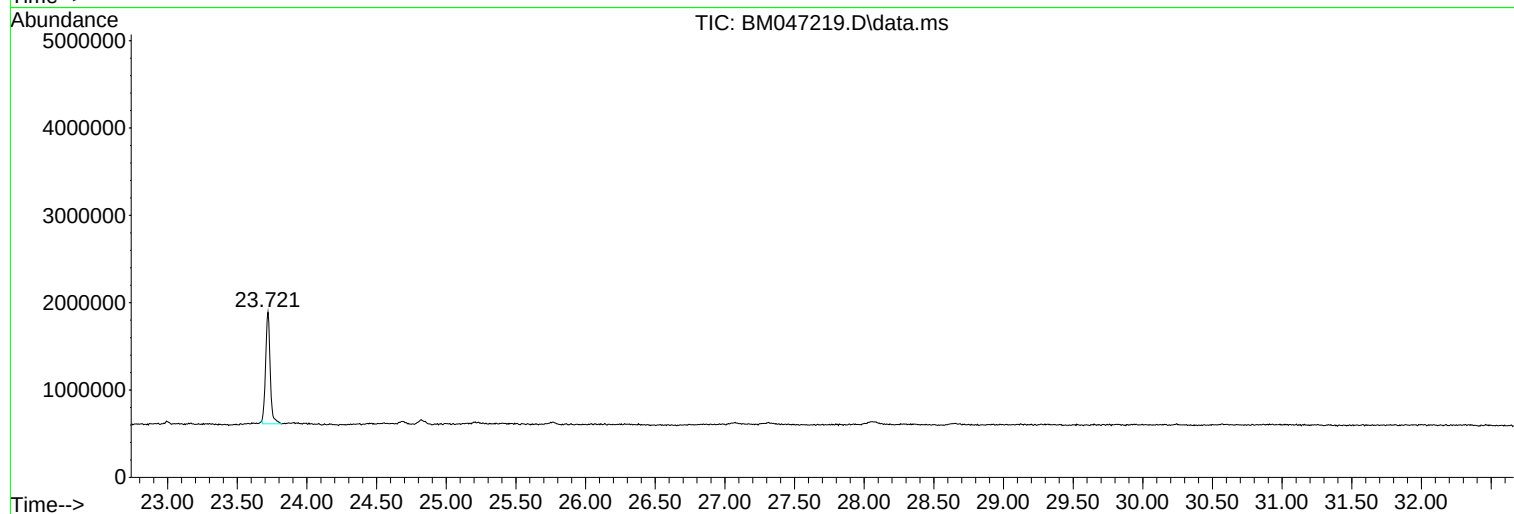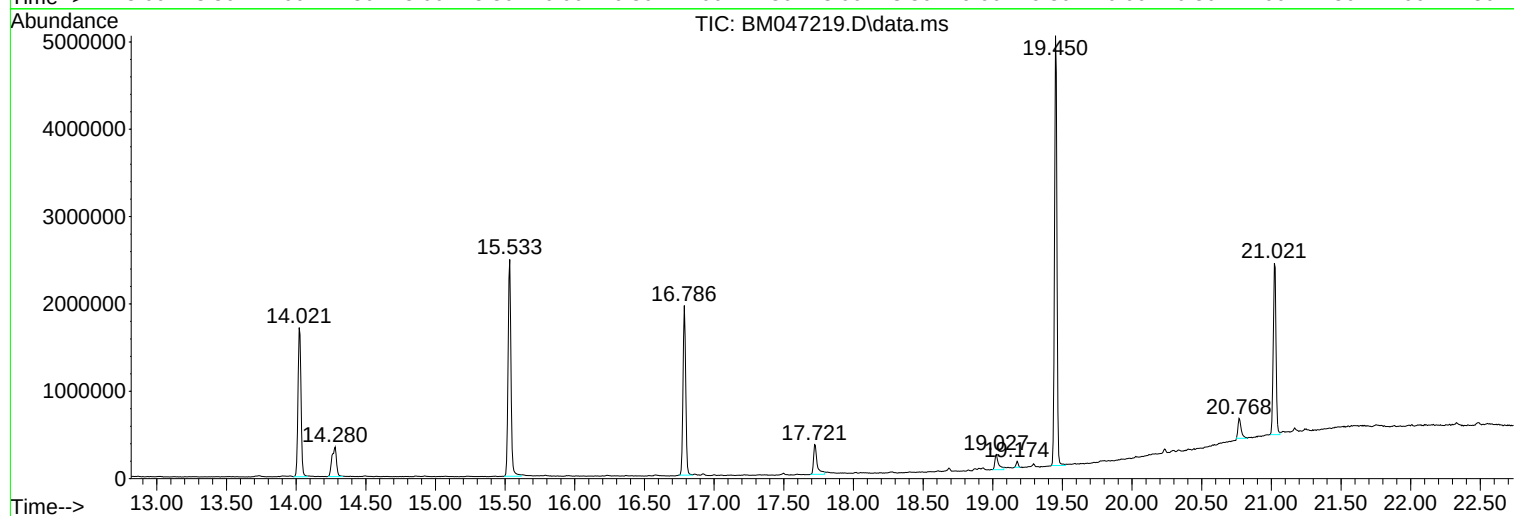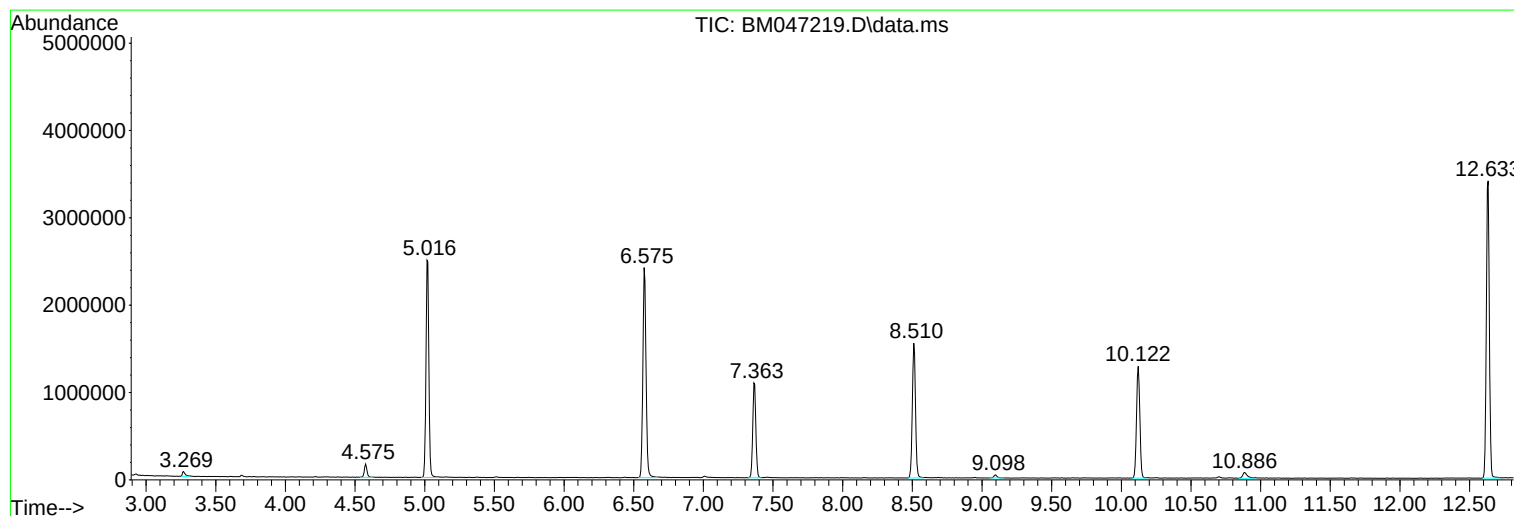

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047219.D
Acq On : 15 Aug 2024 17:32
Operator : RC/JU
Sample : P3520-09RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-12-080624RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047219.D
Acq On : 15 Aug 2024 17:32
Operator : RC/JU
Sample : P3520-09RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-CF-12-080624RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------