

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047220.D
 Acq On : 15 Aug 2024 18:12
 Operator : RC/JU
 Sample : P3518-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-03-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	74	rBV	278268	368837	7.71%	0.736%
2	4.575	281	287	295	rBV	213678	294718	6.16%	0.588%
3	5.022	355	363	381	rBV	3019042	4318534	90.32%	8.619%
4	6.581	620	628	642	rBV	2712972	4350983	91.00%	8.683%
5	6.998	694	699	713	rBV	103875	213973	4.48%	0.427%
6	7.363	752	761	773	rBV	1124249	1715772	35.88%	3.424%
7	8.510	949	956	966	rBV	1823342	2898875	60.63%	5.785%
8	10.122	1223	1230	1238	rBV	1292750	2102449	43.97%	4.196%
9	10.880	1354	1359	1370	rBV	138050	293435	6.14%	0.586%
10	12.633	1650	1657	1670	rBV	3010169	4528539	94.71%	9.038%
11	13.739	1835	1845	1851	rBV5	32961	97585	2.04%	0.195%
12	14.021	1887	1893	1901	rBV	1655520	2457972	51.41%	4.905%
13	14.092	1901	1905	1914	rVB9	28031	66495	1.39%	0.133%
14	14.263	1928	1934	1935	rBV	459959	580409	12.14%	1.158%
15	14.280	1935	1937	1946	rVB	531091	649915	13.59%	1.297%
16	15.410	2122	2129	2140	rBV	16686	47836	1.00%	0.095%
17	15.533	2143	2150	2162	rVV	2566013	3818515	79.86%	7.621%
18	15.627	2162	2166	2177	rVB	41020	104632	2.19%	0.209%
19	15.786	2187	2193	2198	rBV7	21902	50581	1.06%	0.101%
20	16.015	2228	2232	2237	rBV3	43694	56773	1.19%	0.113%
21	16.786	2357	2363	2368	rBV	1875257	2611230	54.61%	5.211%
22	16.827	2368	2370	2374	rVV	171633	202109	4.23%	0.403%
23	16.868	2374	2377	2380	rVV2	53081	67064	1.40%	0.134%
24	16.915	2381	2385	2393	rVB3	95821	144963	3.03%	0.289%
25	17.498	2481	2484	2493	rVB	66130	91061	1.90%	0.182%
26	17.727	2517	2523	2532	rBV	768455	1221191	25.54%	2.437%
27	17.857	2542	2545	2550	rVB2	39289	49843	1.04%	0.099%
28	17.992	2564	2568	2572	rBV2	107957	138650	2.90%	0.277%
29	18.604	2668	2672	2675	rBV4	41275	65078	1.36%	0.130%
30	18.686	2683	2686	2690	rVB3	87160	110925	2.32%	0.221%
31	18.762	2697	2699	2706	rVB5	60187	80103	1.68%	0.160%
32	18.862	2712	2716	2721	rBV	389164	512610	10.72%	1.023%
33	19.027	2739	2744	2751	rBV2	321775	530849	11.10%	1.059%
34	19.227	2774	2778	2784	rVB	319993	419554	8.77%	0.837%
35	19.451	2811	2816	2821	rBV	3972946	4781343	100.00%	9.542%
36	20.109	2924	2928	2933	rVB3	158597	234130	4.90%	0.467%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047220.D
Acq On : 15 Aug 2024 18:12
Operator : RC/JU
Sample : P3518-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-03-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.768	3036	3040	3050	rVB2	400275	659700	13.80%	1.317%
38	21.021	3077	3083	3088	rBV	2012305	2999814	62.74%	5.987%
39	21.756	3205	3208	3211	rBV	186467	226084	4.73%	0.451%
40	22.997	3414	3419	3427	rVB	941822	1672528	34.98%	3.338%
41	23.721	3535	3542	3549	rBV	1173788	2639042	55.19%	5.267%
42	24.685	3700	3706	3715	rVB	670146	1632187	34.14%	3.257%




Sum of corrected areas: 50106886

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047220.D
Acq On : 15 Aug 2024 18:12
Operator : RC/JU
Sample : P3518-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-03-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

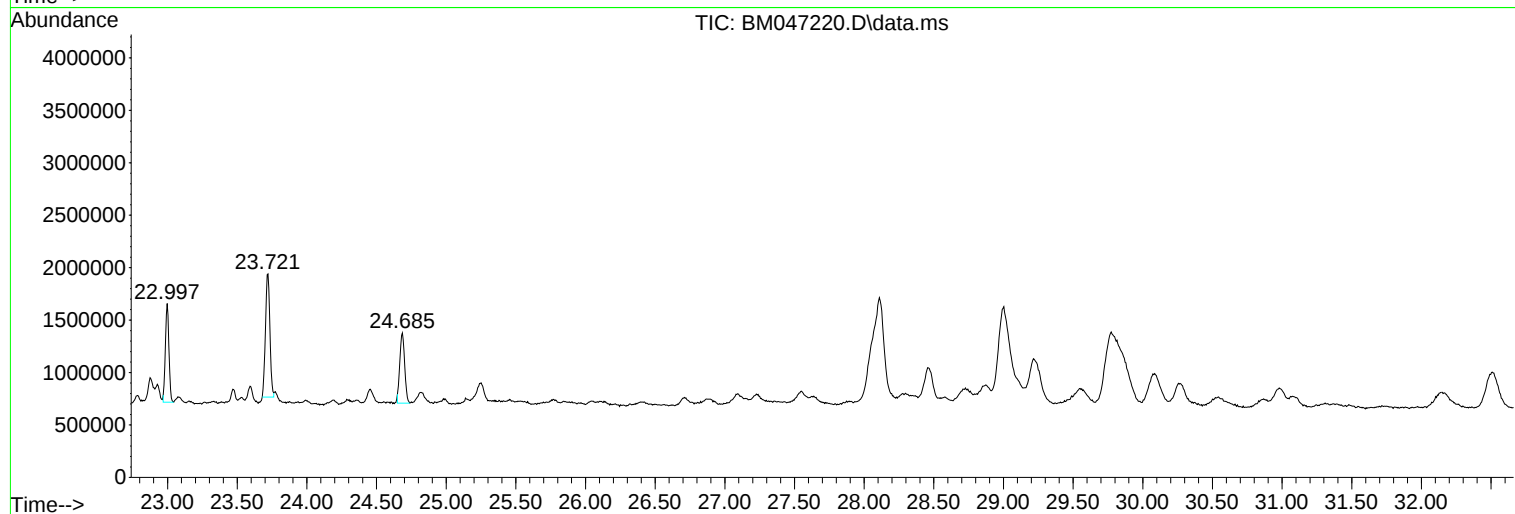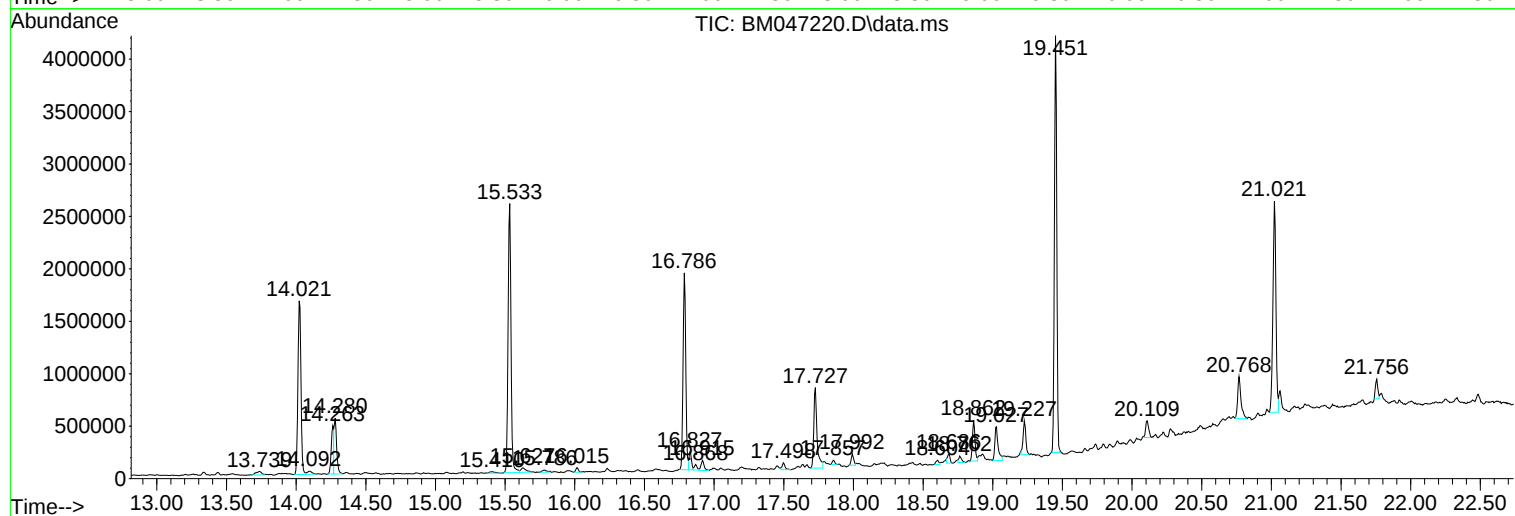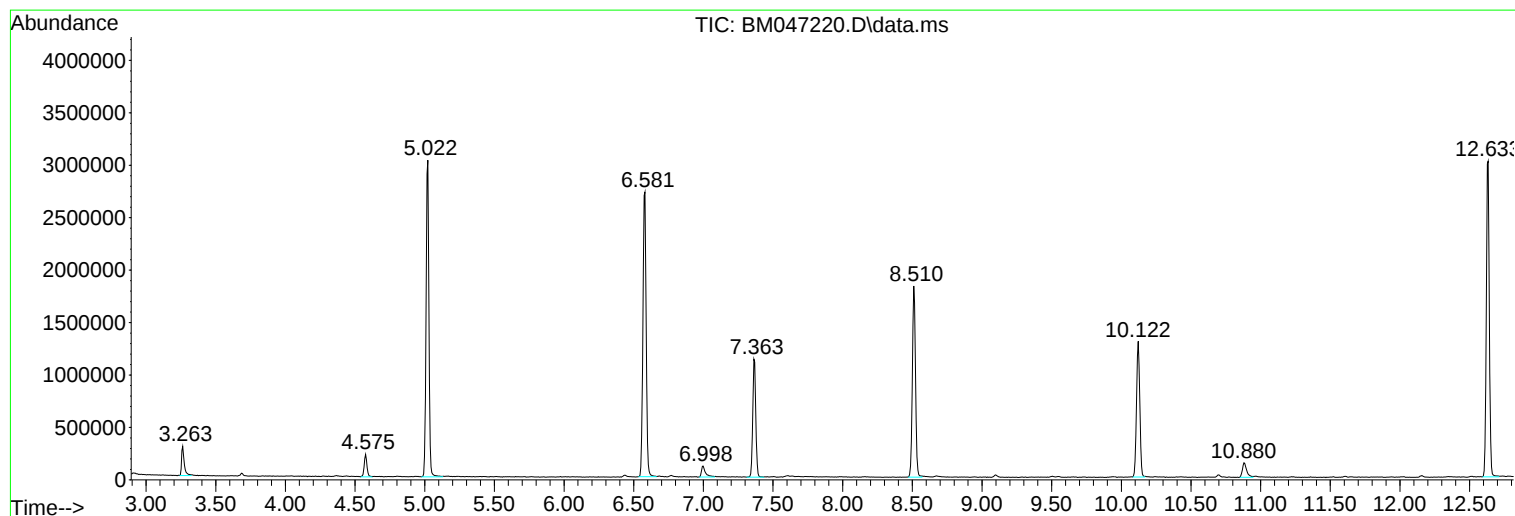

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047220.D
Acq On : 15 Aug 2024 18:12
Operator : RC/JU
Sample : P3518-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-03-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047220.D
Acq On : 15 Aug 2024 18:12
Operator : RC/JU
Sample : P3518-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-03-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------