

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047221.D
 Acq On : 15 Aug 2024 18:53
 Operator : RC/JU
 Sample : P3518-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-04-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	60	64	73	rBV	241868	305937	7.10%	0.601%
2	4.575	281	287	295	rVB	195633	261879	6.08%	0.514%
3	5.022	356	363	376	rBV	2717017	3940903	91.46%	7.741%
4	6.575	619	627	641	rBV	2641073	4136133	95.99%	8.125%
5	6.998	694	699	712	rBV	84458	168335	3.91%	0.331%
6	7.363	752	761	768	rBV	1195592	1848447	42.90%	3.631%
7	7.604	794	802	808	rBV8	15784	43856	1.02%	0.086%
8	8.510	948	956	968	rBV	1704343	2723229	63.20%	5.349%
9	10.122	1218	1230	1237	rBV	1457699	2401259	55.73%	4.717%
10	10.880	1352	1359	1371	rBV	191544	408531	9.48%	0.803%
11	12.633	1649	1657	1669	rBV	2786598	4308778	100.00%	8.464%
12	13.333	1771	1776	1782	rBV4	28095	50828	1.18%	0.100%
13	13.739	1836	1845	1851	rBV7	29382	73519	1.71%	0.144%
14	14.021	1886	1893	1901	rBV	1953213	2852054	66.19%	5.603%
15	14.098	1902	1906	1914	rVB9	26203	59034	1.37%	0.116%
16	14.263	1928	1934	1935	rBV	1614519	1945276	45.15%	3.821%
17	14.280	1935	1937	1947	rVB	1832761	2287395	53.09%	4.493%
18	15.404	2123	2128	2139	rVB	16933	50611	1.17%	0.099%
19	15.533	2143	2150	2162	rBV	2417772	3476360	80.68%	6.829%
20	15.757	2182	2188	2196	rBV3	52268	123598	2.87%	0.243%
21	16.015	2228	2232	2237	rBV4	51400	70547	1.64%	0.139%
22	16.233	2265	2269	2274	rVB8	30219	44376	1.03%	0.087%
23	16.786	2357	2363	2368	rBV	2080140	2792849	64.82%	5.486%
24	16.827	2368	2370	2374	rVV	121359	139721	3.24%	0.274%
25	16.868	2374	2377	2381	rVV4	38081	55605	1.29%	0.109%
26	16.915	2381	2385	2393	rVB2	77189	117538	2.73%	0.231%
27	17.192	2428	2432	2440	rBV7	19423	52978	1.23%	0.104%
28	17.451	2473	2476	2481	rBV4	29036	53460	1.24%	0.105%
29	17.498	2481	2484	2492	rVB	57943	82311	1.91%	0.162%
30	17.727	2517	2523	2531	rBV2	574035	932930	21.65%	1.833%
31	17.992	2564	2568	2573	rBV4	94620	130777	3.04%	0.257%
32	18.686	2683	2686	2691	rVB5	84210	104294	2.42%	0.205%
33	18.862	2712	2716	2721	rBV	272579	395470	9.18%	0.777%
34	19.027	2739	2744	2750	rBV2	240643	382766	8.88%	0.752%
35	19.227	2775	2778	2784	rVB	211294	266218	6.18%	0.523%
36	19.451	2811	2816	2828	rVB	3279563	4066240	94.37%	7.988%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047221.D
Acq On : 15 Aug 2024 18:53
Operator : RC/JU
Sample : P3518-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-04-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.109	2925	2928	2934	rBV4	141124	201640	4.68%	0.396%
38	20.768	3037	3040	3049	rVB2	314632	471798	10.95%	0.927%
39	21.021	3078	3083	3088	rBV	1920712	2761484	64.09%	5.425%
40	21.756	3205	3208	3212	rBV	192591	237184	5.50%	0.466%
41	22.997	3414	3419	3427	rVB	871693	1580943	36.69%	3.106%
42	23.721	3535	3542	3558	rVB	1205198	2989637	69.38%	5.873%
43	24.685	3700	3706	3716	rVB	610847	1510011	35.04%	2.966%




Sum of corrected areas: 50906739

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047221.D
Acq On : 15 Aug 2024 18:53
Operator : RC/JU
Sample : P3518-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-04-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

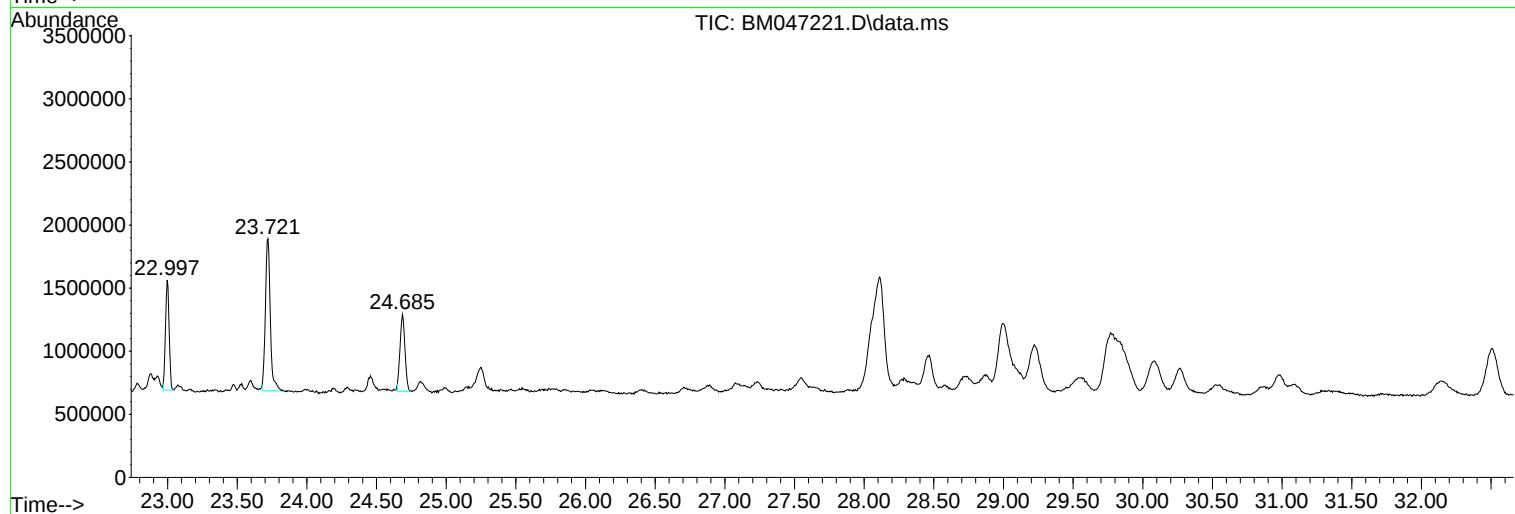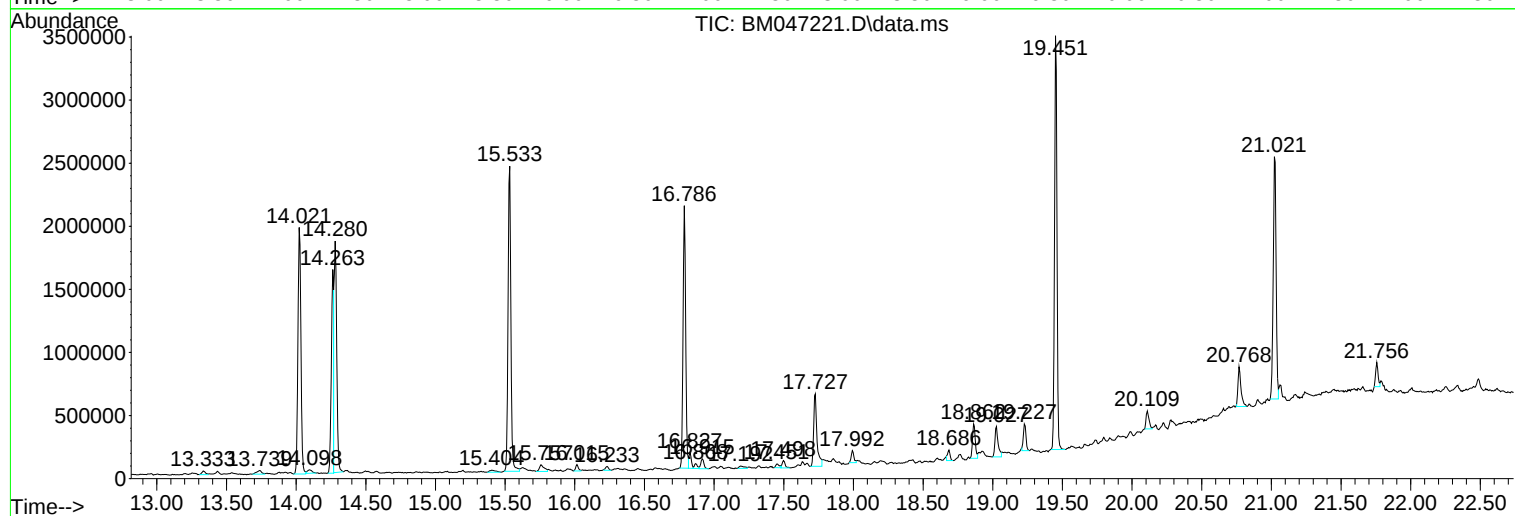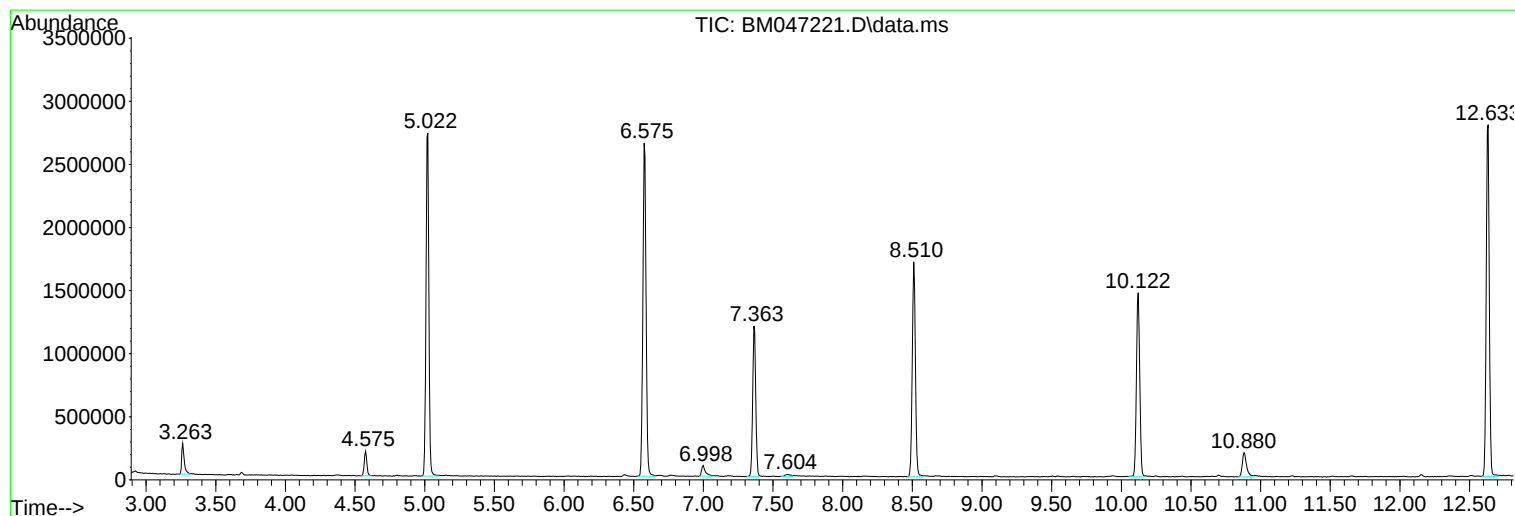

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047221.D
Acq On : 15 Aug 2024 18:53
Operator : RC/JU
Sample : P3518-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-04-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047221.D
Acq On : 15 Aug 2024 18:53
Operator : RC/JU
Sample : P3518-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-04-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------