

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047223.D
 Acq On : 15 Aug 2024 20:13
 Operator : RC/JU
 Sample : P3518-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-06-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	61	64	77	rVB	276608	344109	4.60%	0.468%
2	4.575	281	287	296	rVB	272626	364716	4.87%	0.496%
3	5.022	355	363	373	rBV	3740026	5263145	70.28%	7.165%
4	6.581	620	628	641	rBV	3562312	5380419	71.85%	7.324%
5	6.998	694	699	709	rBV	105544	201491	2.69%	0.274%
6	7.363	750	761	769	rBV	1130097	1783073	23.81%	2.427%
7	8.510	949	956	967	rBV	2150874	3563053	47.58%	4.850%
8	10.122	1223	1230	1237	rBV	1310048	2193670	29.29%	2.986%
9	10.881	1350	1359	1370	rBV2	319540	662016	8.84%	0.901%
10	12.633	1648	1657	1665	rBV	3682243	5610185	74.92%	7.637%
11	13.739	1835	1845	1855	rBV2	69207	160423	2.14%	0.218%
12	14.022	1887	1893	1901	rBV	1692925	2590218	34.59%	3.526%
13	14.269	1928	1935	1936	rBV	4638578	6804124	90.86%	9.263%
14	14.286	1936	1938	1947	rVB	6297554	7488714	100.00%	10.194%
15	15.533	2144	2150	2162	rBV	3363180	4864435	64.96%	6.622%
16	16.015	2228	2232	2237	rBV	68929	91696	1.22%	0.125%
17	16.233	2265	2269	2276	rVB3	51120	77338	1.03%	0.105%
18	16.786	2357	2363	2368	rBV	1976109	2768450	36.97%	3.769%
19	16.827	2368	2370	2374	rVV	233305	263682	3.52%	0.359%
20	16.868	2374	2377	2381	rVV3	64971	83867	1.12%	0.114%
21	16.915	2381	2385	2391	rVB2	141296	214476	2.86%	0.292%
22	17.498	2481	2484	2490	rVB2	77200	107577	1.44%	0.146%
23	17.727	2517	2523	2531	rBV2	1153248	1735144	23.17%	2.362%
24	17.857	2542	2545	2549	rVB2	57872	78522	1.05%	0.107%
25	17.992	2564	2568	2578	rBV6	122206	222397	2.97%	0.303%
26	18.604	2668	2672	2678	rBV2	166217	293348	3.92%	0.399%
27	18.686	2683	2686	2692	rVB3	207129	255822	3.42%	0.348%
28	18.821	2707	2709	2712	rBV	60289	76885	1.03%	0.105%
29	18.862	2712	2716	2720	rVV	601930	838855	11.20%	1.142%
30	18.921	2724	2726	2732	rVB4	195736	286691	3.83%	0.390%
31	19.027	2739	2744	2751	rBV2	483711	743870	9.93%	1.013%
32	19.227	2774	2778	2786	rVB	502113	686349	9.17%	0.934%
33	19.451	2811	2816	2826	rVB	4690219	6156013	82.20%	8.380%
34	20.109	2925	2928	2934	rVB2	210860	341604	4.56%	0.465%
35	20.768	3036	3040	3050	rVB2	672379	1037548	13.85%	1.412%
36	21.027	3078	3084	3088	rBV	2080670	3121386	41.68%	4.249%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047223.D
Acq On : 15 Aug 2024 20:13
Operator : RC/JU
Sample : P3518-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-06-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.756	3205	3208	3211	rBV	252747	337420	4.51%	0.459%
38	22.997	3414	3419	3427	rVB	1072030	1884741	25.17%	2.566%
39	23.721	3536	3542	3549	rBV	1243867	2574161	34.37%	3.504%
40	24.686	3700	3706	3717	rVB	753730	1906753	25.46%	2.596%




Sum of corrected areas: 73458386

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047223.D
Acq On : 15 Aug 2024 20:13
Operator : RC/JU
Sample : P3518-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-06-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

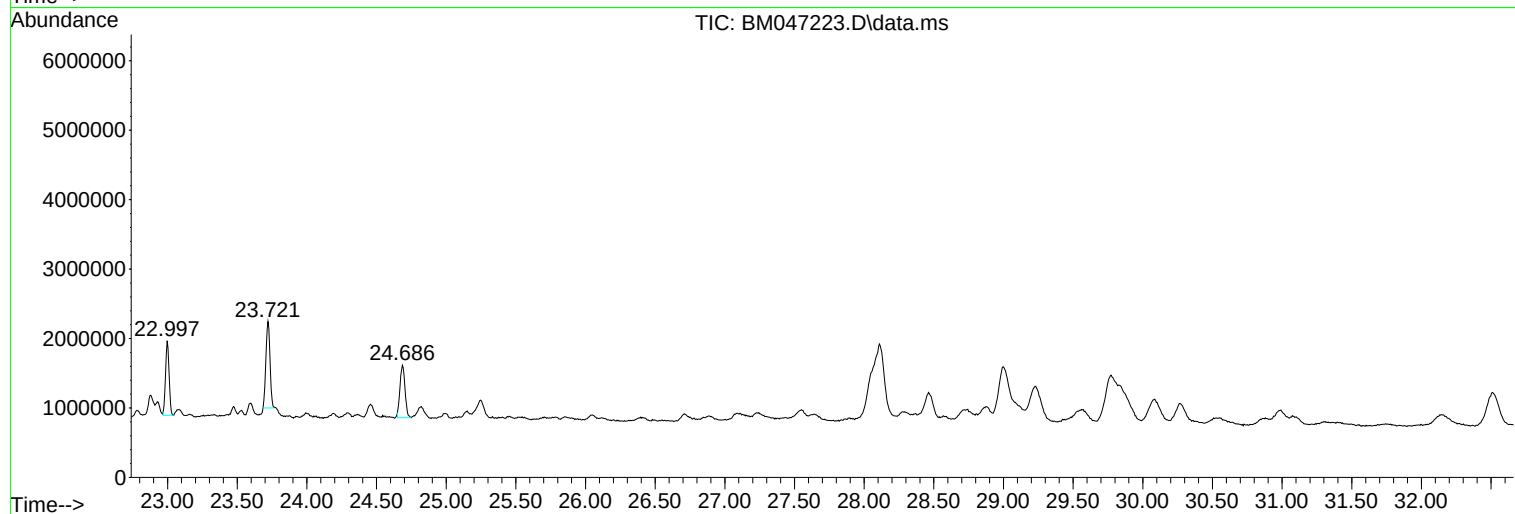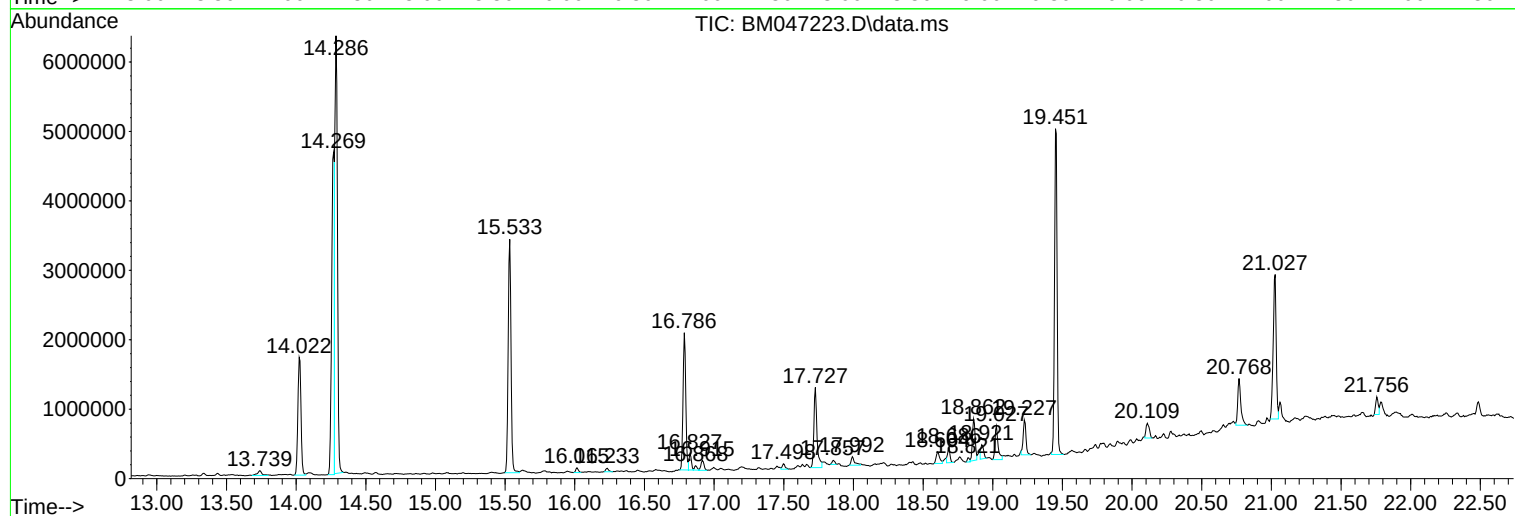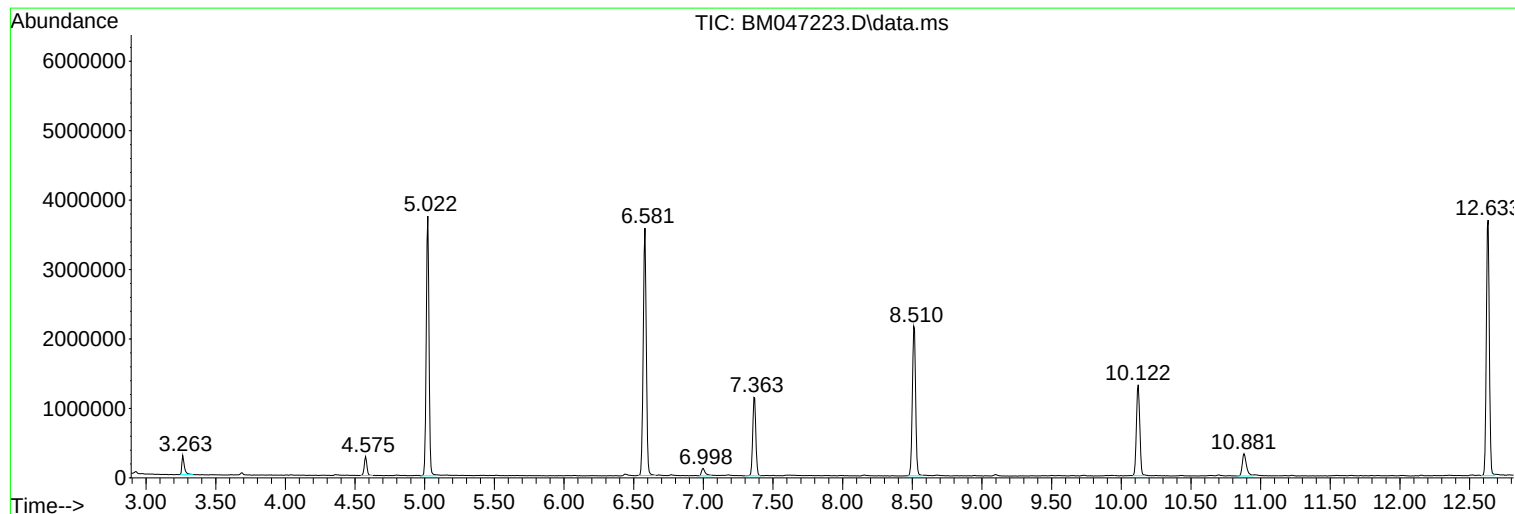

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047223.D
Acq On : 15 Aug 2024 20:13
Operator : RC/JU
Sample : P3518-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-06-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047223.D
Acq On : 15 Aug 2024 20:13
Operator : RC/JU
Sample : P3518-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-06-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------