

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
 Data File : BM047224.D
 Acq On : 15 Aug 2024 20:53
 Operator : RC/JU
 Sample : P3518-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-07-080724

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	60	64	80	rVB	246364	329140	7.50%	0.583%
2	4.575	281	287	293	rBV	180260	237612	5.41%	0.421%
3	5.022	356	363	371	rBV	2529247	3624139	82.57%	6.415%
4	6.581	617	628	642	rBV	2330485	3687181	84.00%	6.526%
5	6.999	694	699	710	rBV	81202	165006	3.76%	0.292%
6	7.363	753	761	769	rBV	1115620	1710112	38.96%	3.027%
7	8.510	948	956	965	rBV	1517155	2461660	56.08%	4.357%
8	10.122	1222	1230	1247	rVB	1284664	2144684	48.86%	3.796%
9	10.881	1352	1359	1370	rBV	242460	479226	10.92%	0.848%
10	12.628	1649	1656	1667	rBV	2523915	3769064	85.87%	6.671%
11	13.333	1770	1776	1781	rBV5	39811	63077	1.44%	0.112%
12	13.733	1837	1844	1851	rBV3	92781	167024	3.81%	0.296%
13	14.022	1886	1893	1901	rBV	1734247	2517953	57.37%	4.457%
14	14.086	1901	1904	1912	rVB5	24977	58223	1.33%	0.103%
15	14.263	1927	1934	1935	rBV	2482966	3019053	68.78%	5.344%
16	14.280	1935	1937	1947	rVB	2960621	3774797	86.00%	6.681%
17	15.533	2143	2150	2160	rBV	2287415	3297933	75.14%	5.837%
18	15.627	2163	2166	2172	rVB8	22526	45144	1.03%	0.080%
19	15.780	2187	2192	2197	rBV8	20368	45311	1.03%	0.080%
20	16.016	2228	2232	2238	rBV3	48006	63548	1.45%	0.112%
21	16.786	2357	2363	2367	rBV	1939455	2649493	60.36%	4.690%
22	16.827	2367	2370	2374	rVB	280994	357234	8.14%	0.632%
23	16.916	2381	2385	2393	rVB2	116089	176105	4.01%	0.312%
24	17.198	2430	2433	2439	rVB	35678	58044	1.32%	0.103%
25	17.498	2481	2484	2491	rVB2	65200	89963	2.05%	0.159%
26	17.668	2510	2513	2517	rVB	56207	66177	1.51%	0.117%
27	17.721	2517	2522	2531	rBV2	593359	967079	22.03%	1.712%
28	17.857	2541	2545	2549	rBV2	109179	155747	3.55%	0.276%
29	17.992	2565	2568	2572	rBV5	65611	78562	1.79%	0.139%
30	18.216	2603	2606	2611	rVB	127368	180508	4.11%	0.319%
31	18.598	2668	2671	2676	rBV5	50598	95510	2.18%	0.169%
32	18.686	2683	2686	2690	rVB4	125606	160600	3.66%	0.284%
33	18.739	2692	2695	2704	rVB3	73389	159709	3.64%	0.283%
34	18.863	2711	2716	2721	rBV	1831267	2419221	55.12%	4.282%
35	19.021	2739	2743	2750	rBV2	231750	383094	8.73%	0.678%
36	19.227	2770	2778	2784	rBV	1325222	2082500	47.45%	3.686%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047224.D
Acq On : 15 Aug 2024 20:53
Operator : RC/JU
Sample : P3518-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-07-080724

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.451	2811	2816	2827	rVB	3537205	4389265	100.00%	7.769%
38	19.733	2862	2864	2869	rVB3	160948	196044	4.47%	0.347%
39	19.839	2879	2882	2886	rBV	101504	128773	2.93%	0.228%
40	20.104	2925	2927	2934	rVB5	129336	185985	4.24%	0.329%
41	20.762	3036	3039	3049	rVB4	382044	719932	16.40%	1.274%
42	21.021	3077	3083	3087	rBV2	2086916	3296131	75.10%	5.834%
43	21.062	3087	3090	3099	rVB	436406	634339	14.45%	1.123%
44	22.998	3414	3419	3427	rVB	724371	1300748	29.63%	2.302%
45	23.721	3535	3542	3549	rBV	1204310	2696553	61.44%	4.773%
46	24.680	3701	3705	3716	rVB	511279	1211003	27.59%	2.143%




Sum of corrected areas: 56498206

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047224.D
Acq On : 15 Aug 2024 20:53
Operator : RC/JU
Sample : P3518-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-07-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

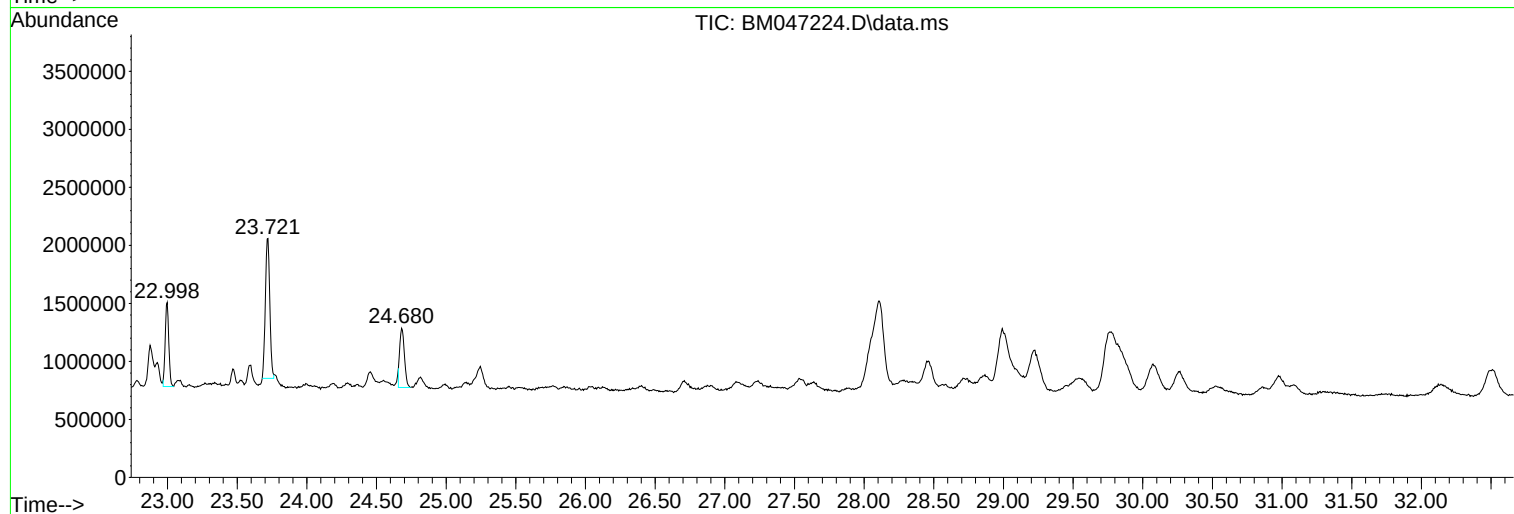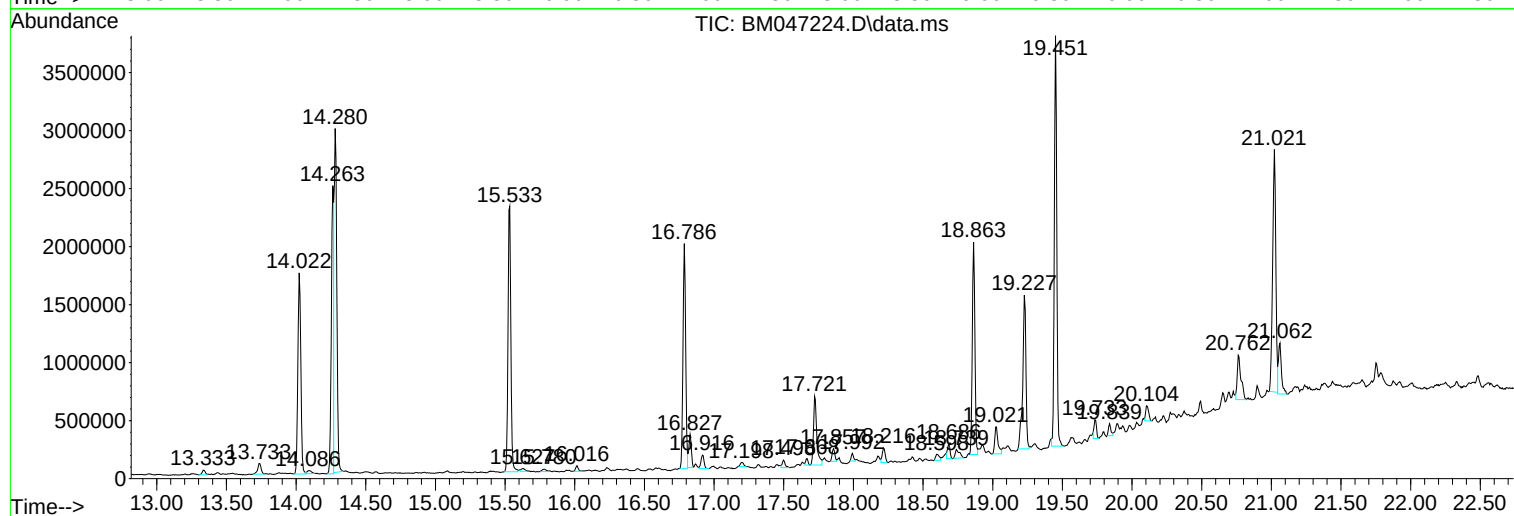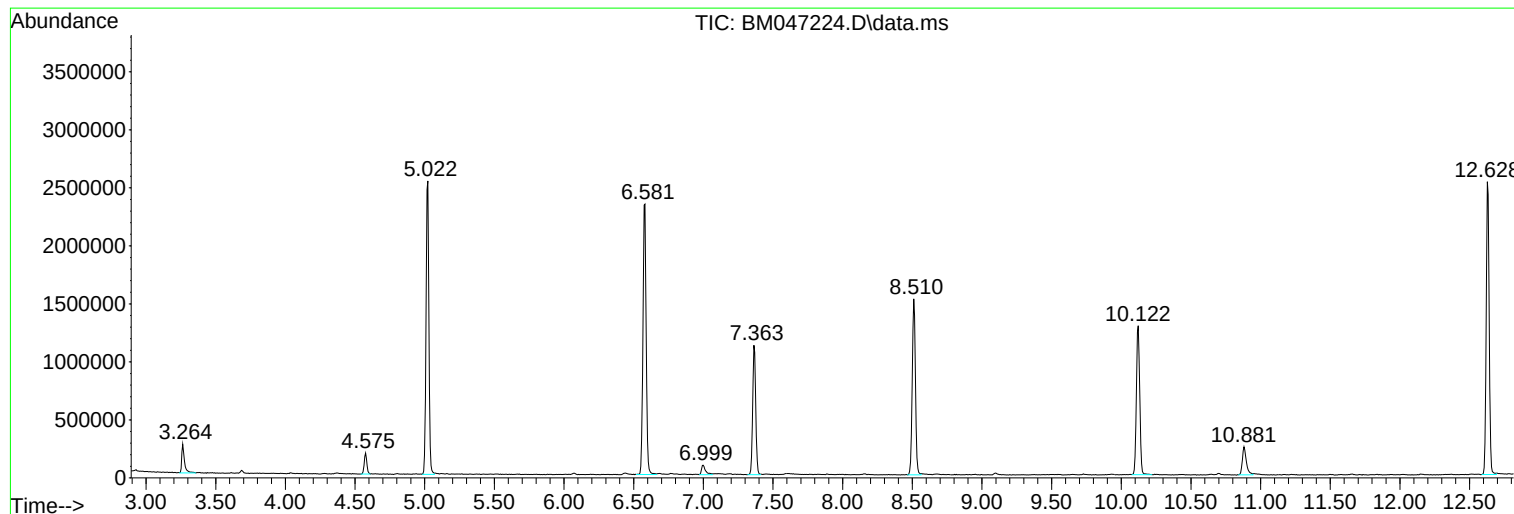

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047224.D
Acq On : 15 Aug 2024 20:53
Operator : RC/JU
Sample : P3518-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-07-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047224.D
Acq On : 15 Aug 2024 20:53
Operator : RC/JU
Sample : P3518-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-07-080724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------