
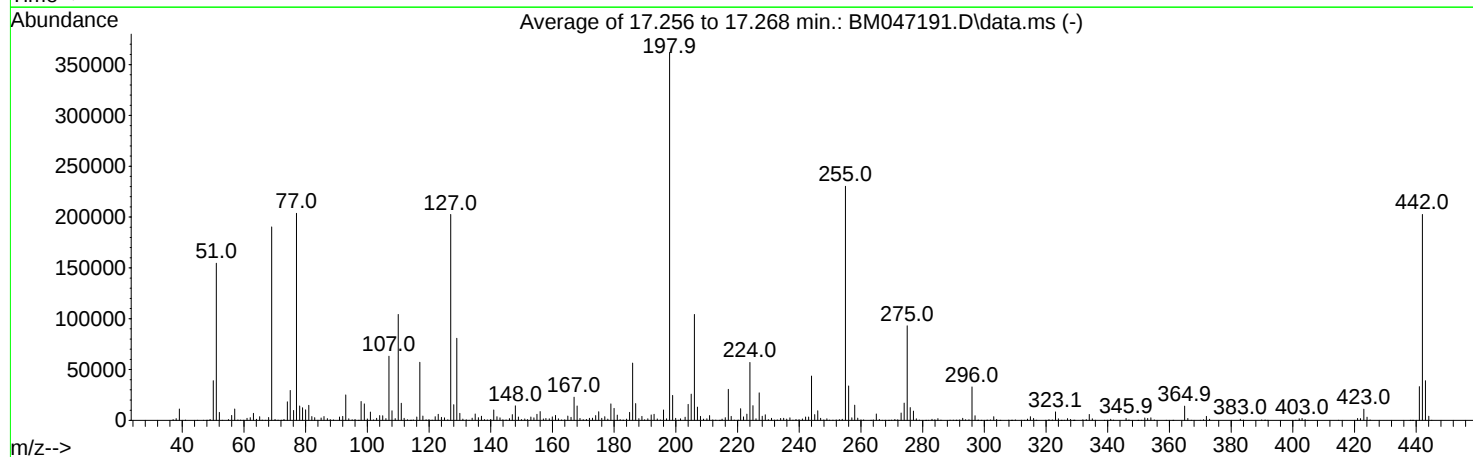


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047191.D
Acq On : 14 Aug 2024 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

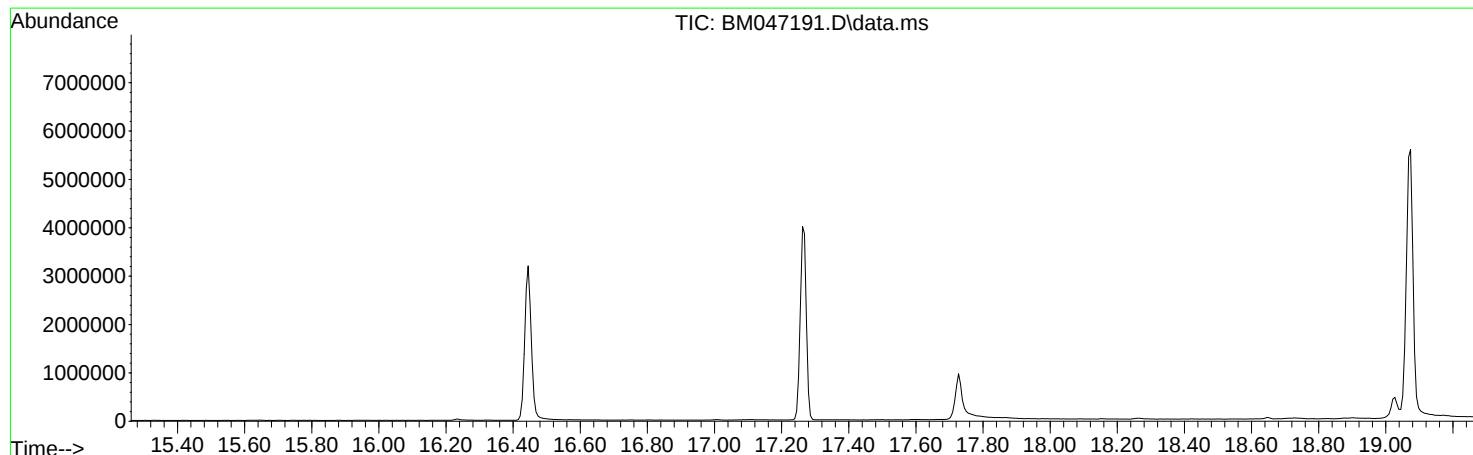

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	154517	PASS
68	69	0.00	2	1.5	2836	PASS
69	198	0.00	100	52.6	190256	PASS
70	69	0.00	2	0.5	925	PASS
127	198	10	80	56.0	202517	PASS
197	198	0.00	2	0.4	1591	PASS
198	198	100	100	100.0	361899	PASS
199	198	5	9	6.8	24605	PASS
275	198	10	60	25.7	93059	PASS
365	198	1	100	3.9	13951	PASS
441	198	0.01	100	9.2	33248	PASS
442	442	50	100	100.0	202635	PASS
443	442	15	24	19.2	38976	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/15/2024	BNA_M	<u>BM047191.D</u>
Compound Name	Response	Retention Time
DDT	1570572	20.315
DDD	18584	19.921
DDE	987	19.368
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19571	1590143	1.23

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047191.D
Acq On : 14 Aug 2024 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 14 17:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

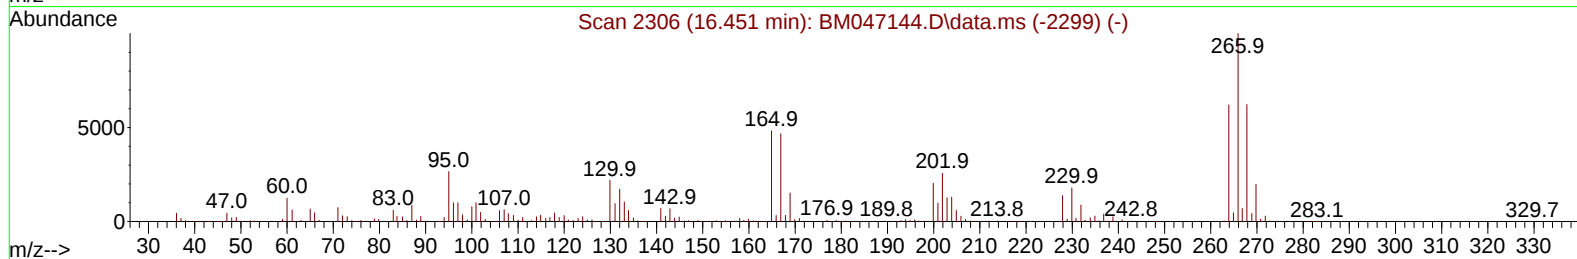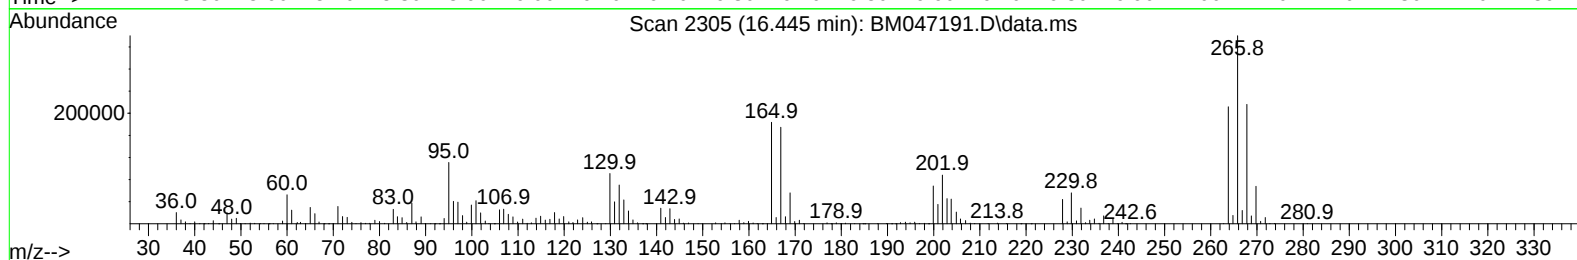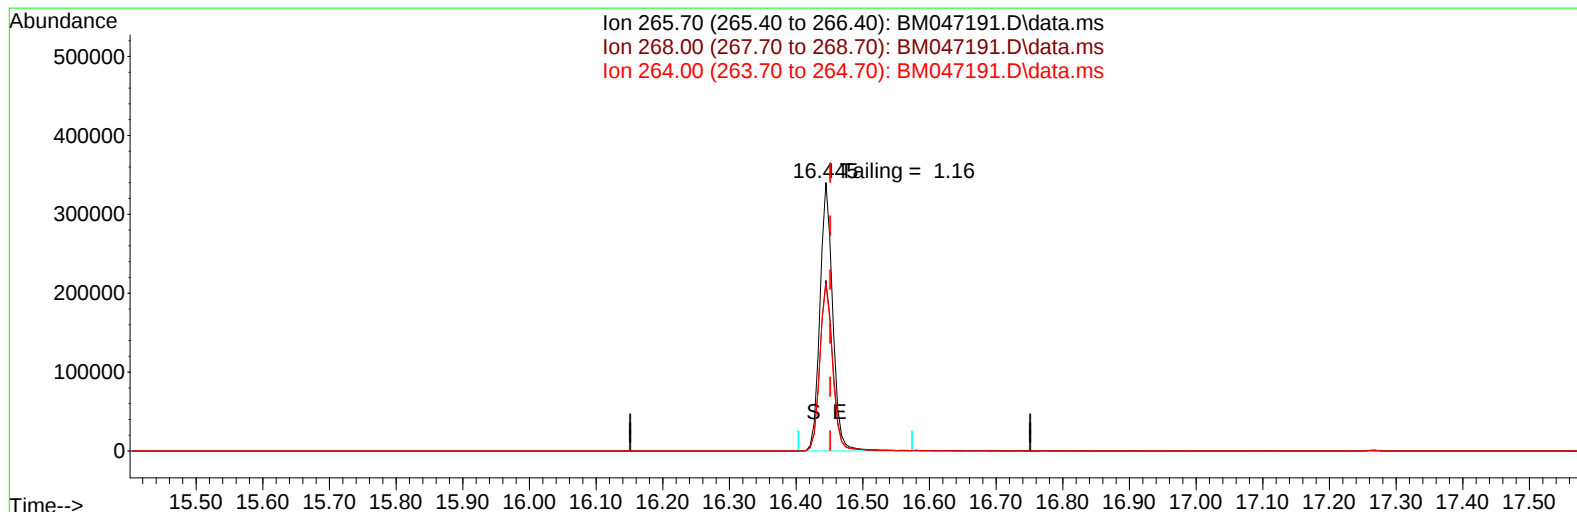

TIC: BM047191.D\data.ms

(70) Pentachlorophenol (C)

16.445min (-0.006) 414349.63 ng




response 455878

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.54
264.00	62.00	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047191.D
Acq On : 14 Aug 2024 14:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 14 17:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

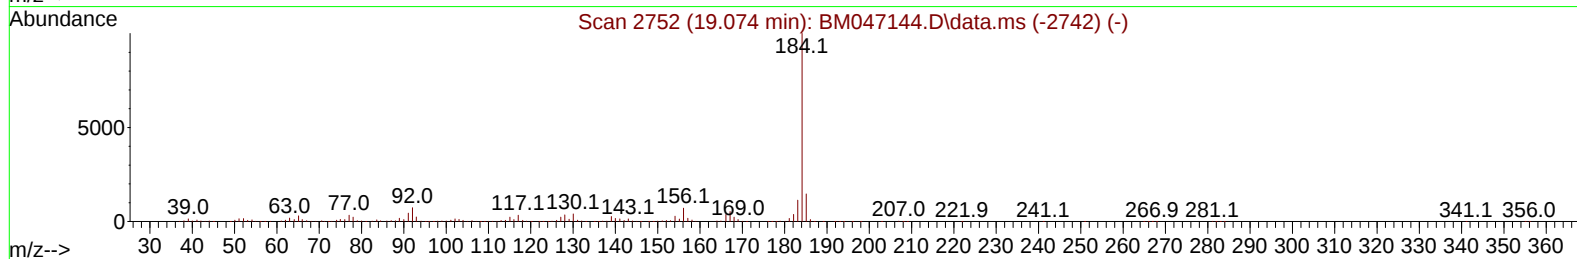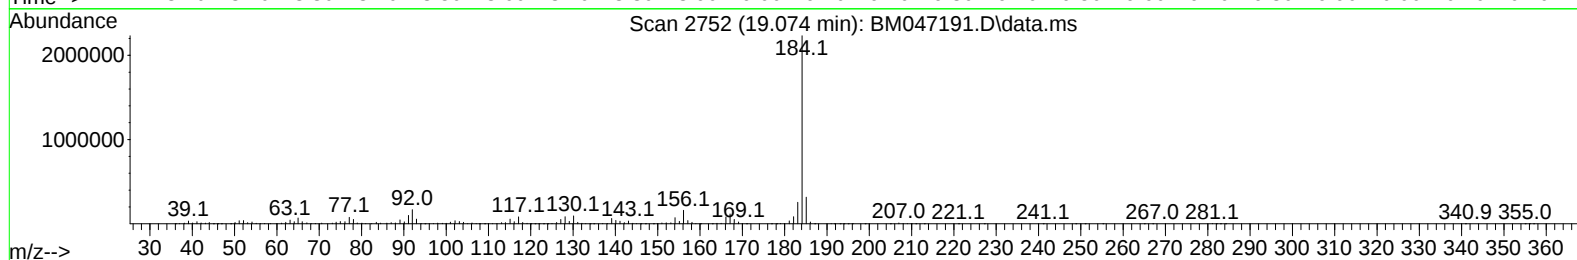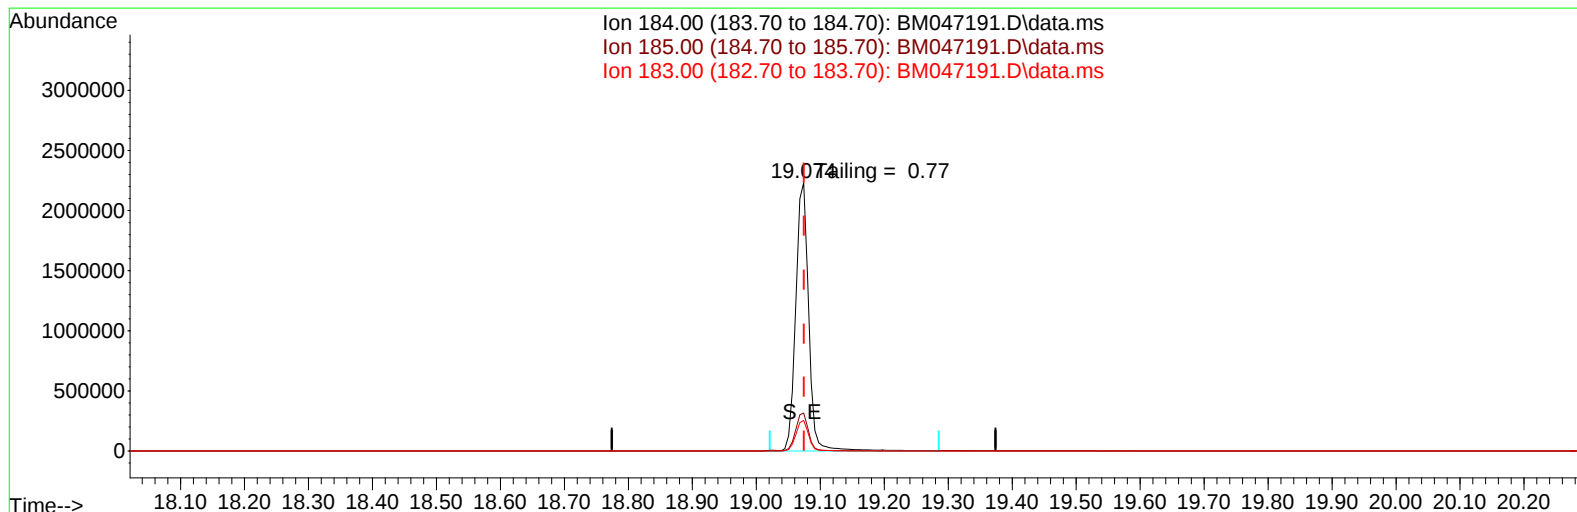

TIC: BM047191.D\data.ms

(77) Benzidine

19.074min (-0.000) 112139.60 ng

response 3139731

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.13
183.00	11.30	11.39
0.00	0.00	0.00