


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047208.D
Acq On : 15 Aug 2024 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

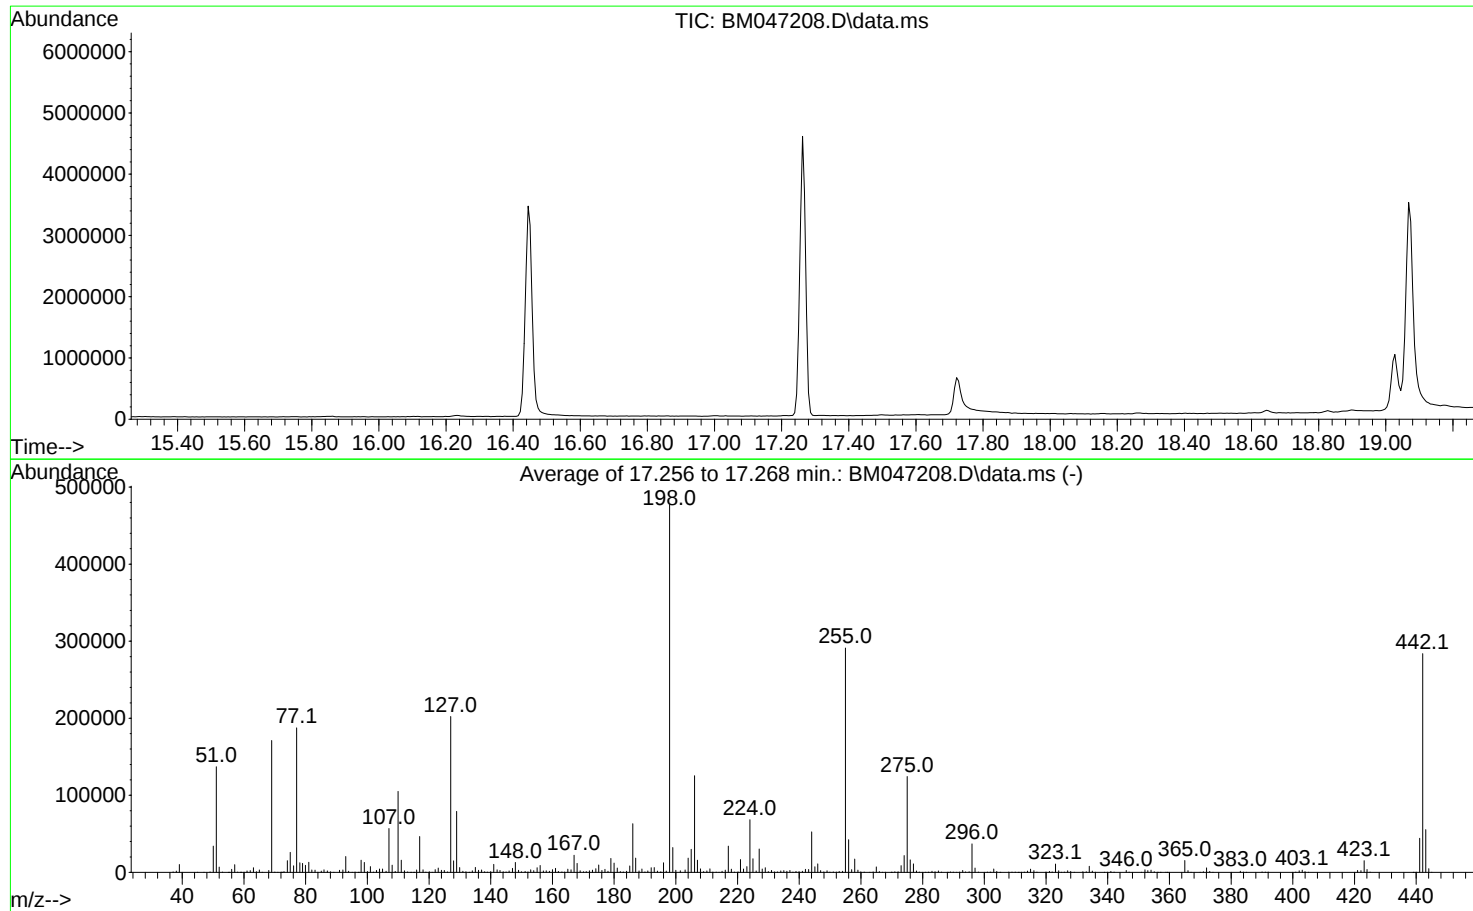




AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	137133	PASS
68	69	0.00	2	1.5	2550	PASS
69	198	0.00	100	35.8	171011	PASS
70	69	0.00	2	0.3	526	PASS
127	198	10	80	42.4	202197	PASS
197	198	0.00	2	0.4	1679	PASS
198	198	100	100	100.0	477397	PASS
199	198	5	9	6.7	32133	PASS
275	198	10	60	26.1	124379	PASS
365	198	1	100	3.2	15297	PASS
441	198	0.01	100	9.3	44296	PASS
442	442	50	100	100.0	283776	PASS
443	442	15	24	19.6	55493	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\  
Data File : BM047208.D  
Acq On    : 15 Aug 2024  10:11  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 15 12:02:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

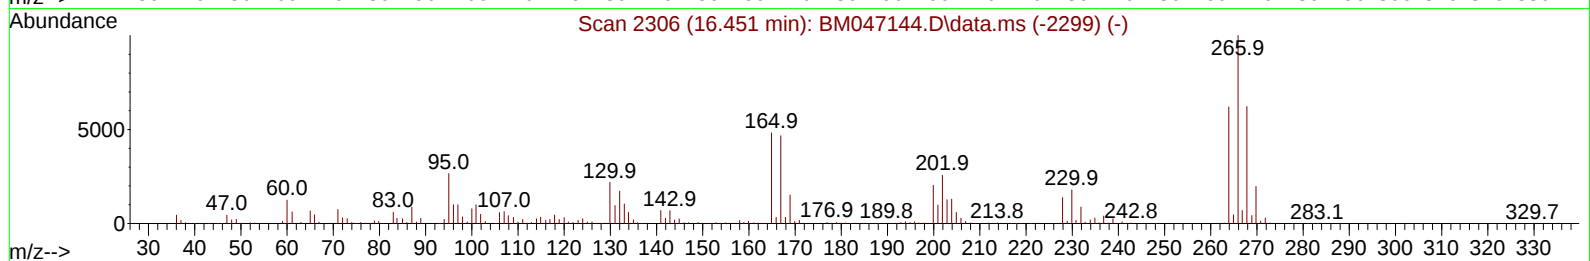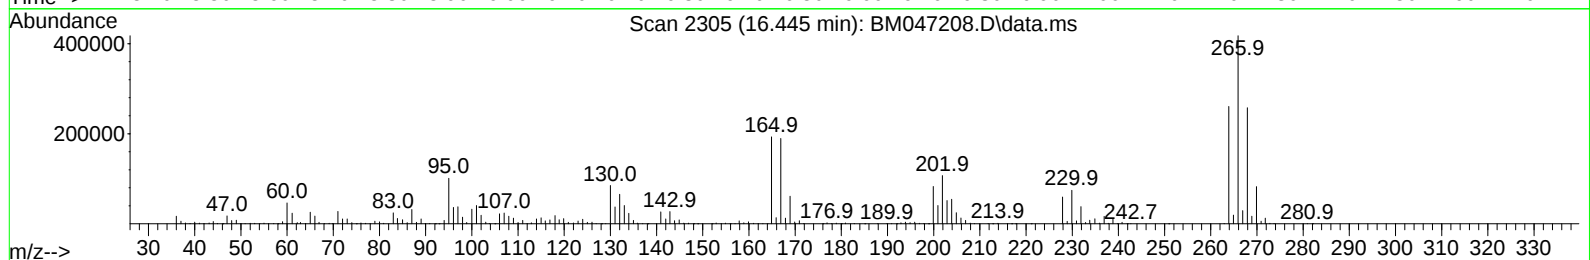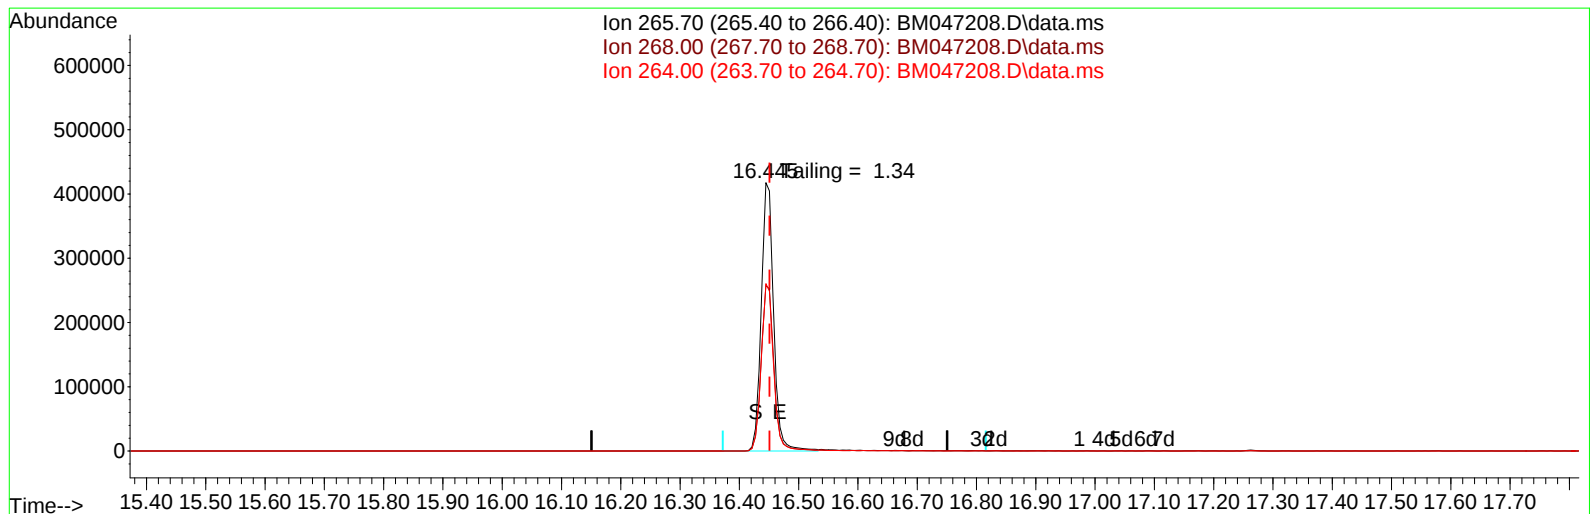

TIC: BM047208.D\data.ms

(70) Pentachlorophenol (C)

16.445min (-0.006) 27141.91 ng m




response **619202**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.71
264.00	62.00	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081524\
Data File : BM047208.D
Acq On : 15 Aug 2024 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 15 12:02:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

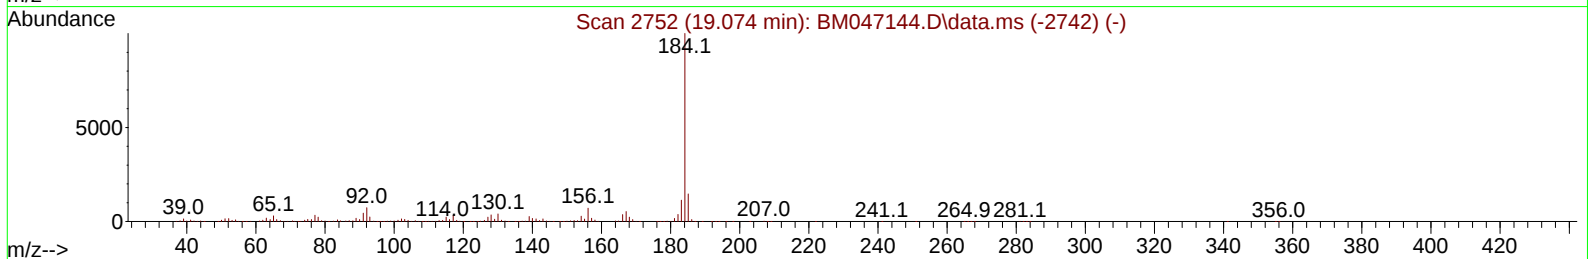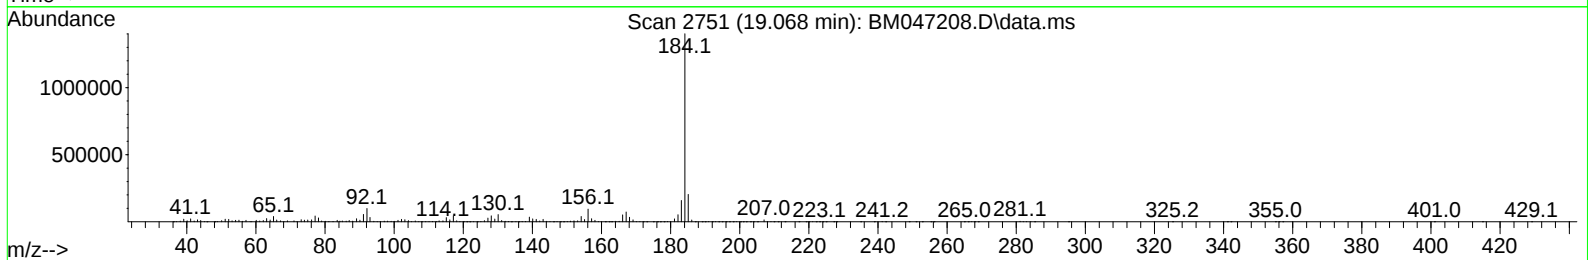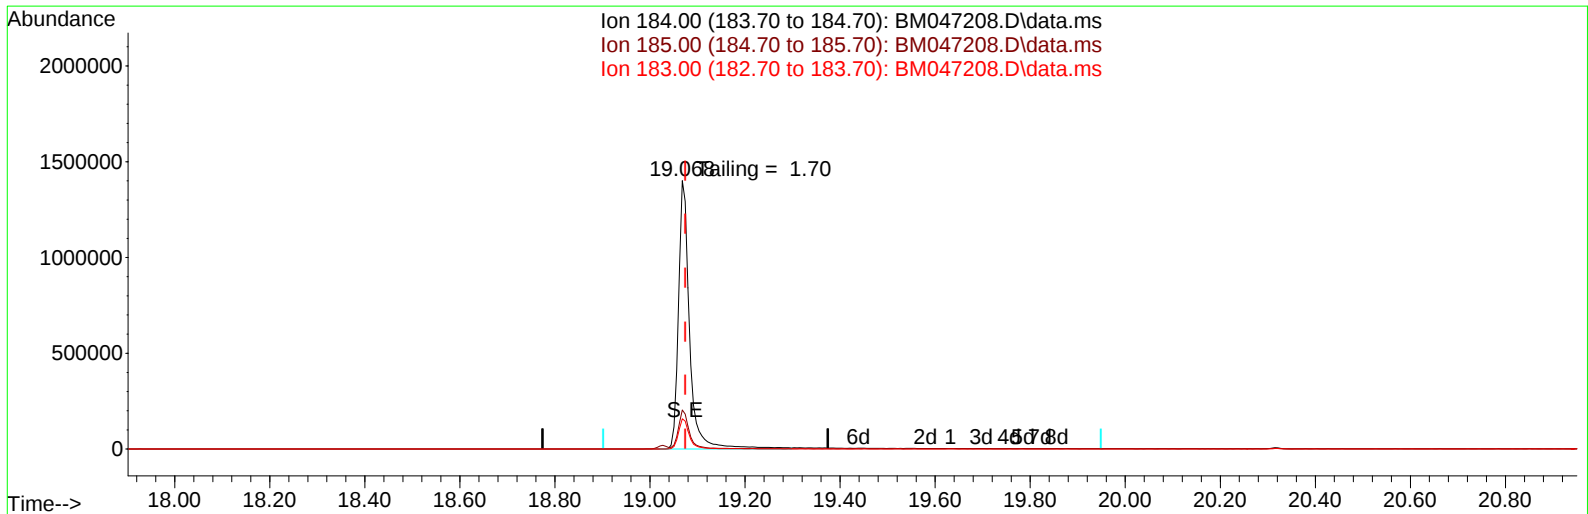

TIC: BM047208.D\data.ms

(77) Benzidine

19.068min (-0.006) 686262.64 ng m

response 2409057

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.56
183.00	11.30	11.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2024	BNA_M	<u>BM047208.D</u>
Compound Name	Response	Retention Time
DDT	1474682	20.321
DDD	79198	19.88
DDE	3581	19.362
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
82779	1557461	5.31

Instrument :
BNA_M
ClientSampleId :
DFTPP