
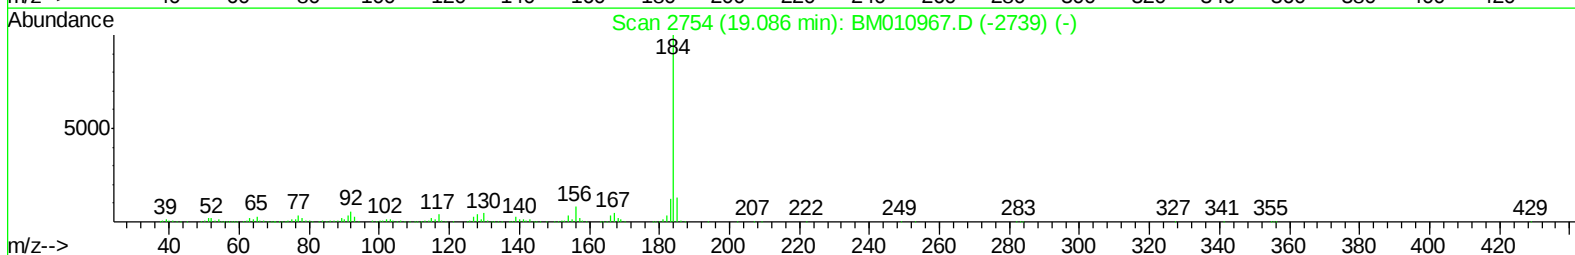
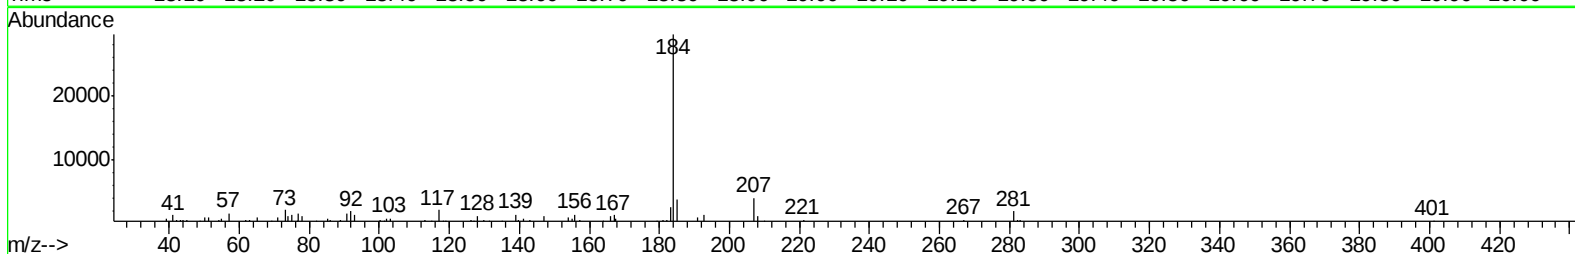


Data Path : Z:\HPCHEM1\BNA M\Data\BM081617\
 Data File : BM011250.D
 Acq On : 16 Aug 2017 10:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 05:18:36 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 02:25:04 2017
 Response via : Initial Calibration

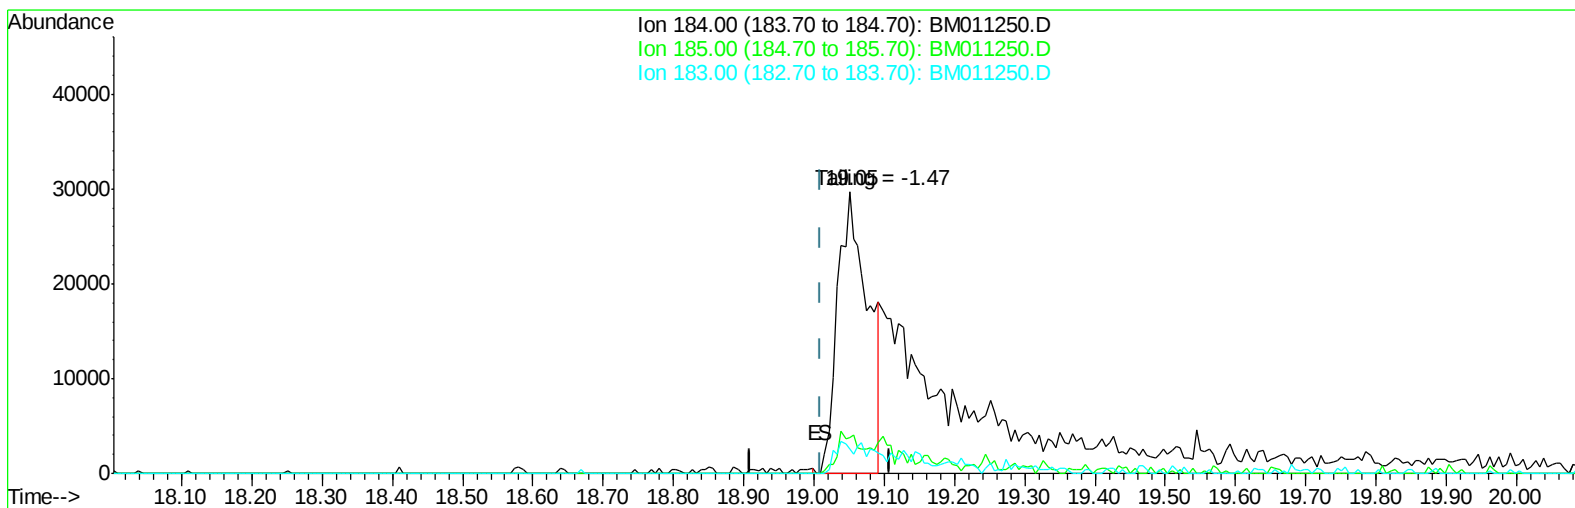

TIC: BM011250.D

(76) Benzidine




19.051min (+0.041) 0.00ng

response 83164

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	12.86
183.00	11.10	8.51#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM081617\
Data File : BM011250.D
Acq On : 16 Aug 2017 10:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 05:18:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

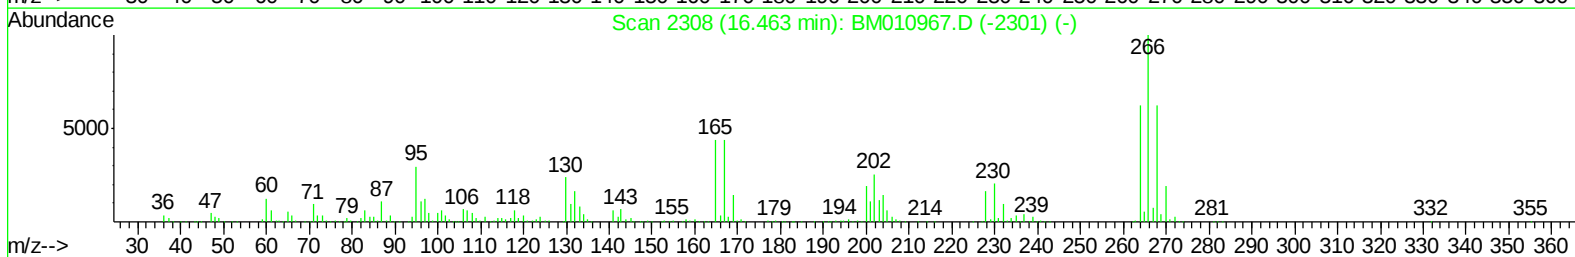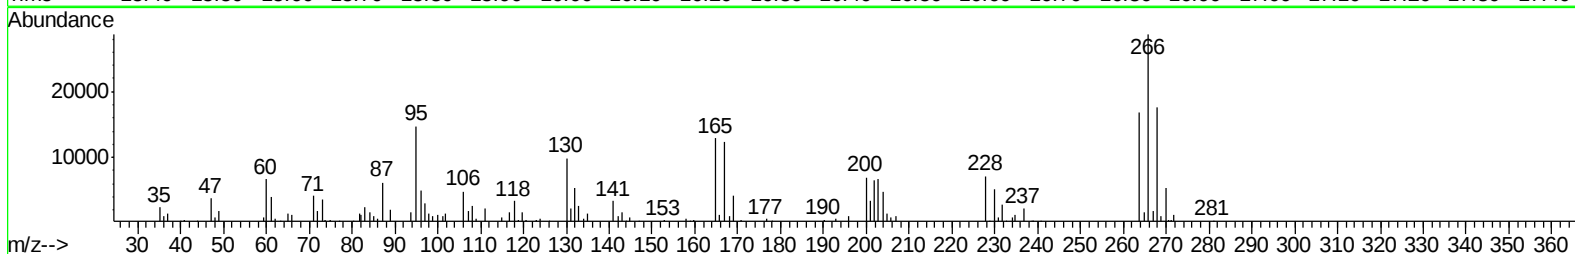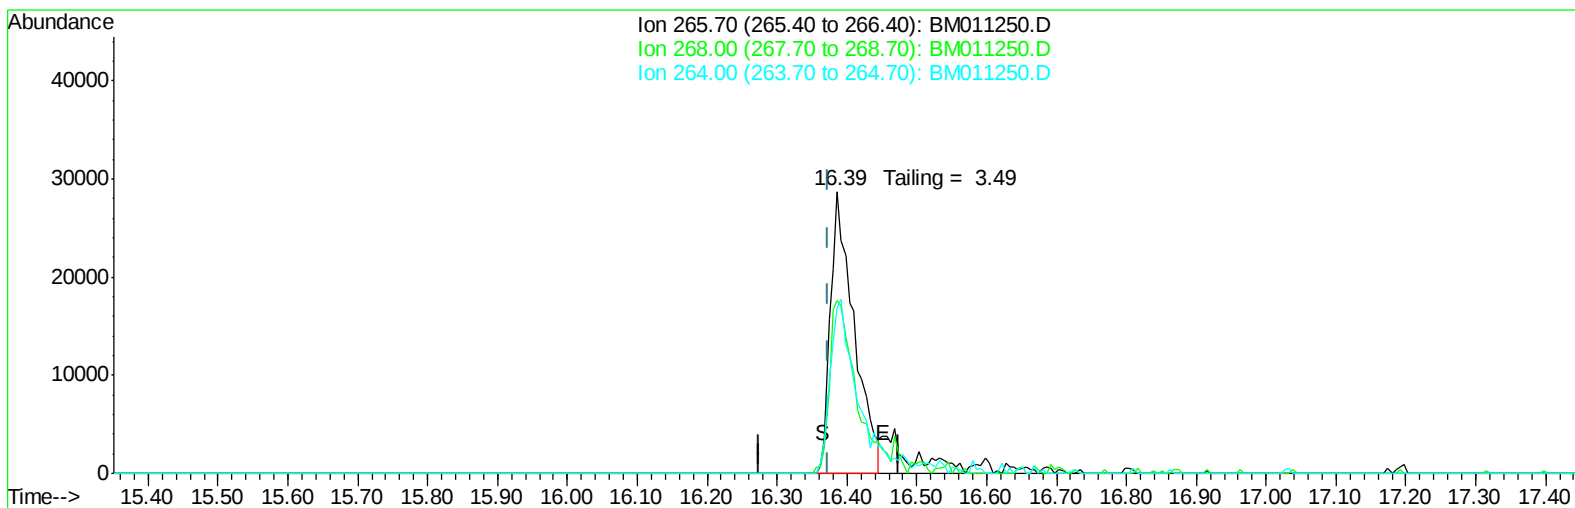

TIC: BM011250.D

(69) Pentachlorophenol (C)

16.386min (+0.012) 0.00ng

response 67058

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.32
264.00	61.20	58.73
0.00	0.00	0.00