


Data Path : Z:\HPCHEM1\BNA M\Data\BM081617\
 Data File : BM011250.D
 Acq On : 16 Aug 2017 10:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 16 02:25:04 2017

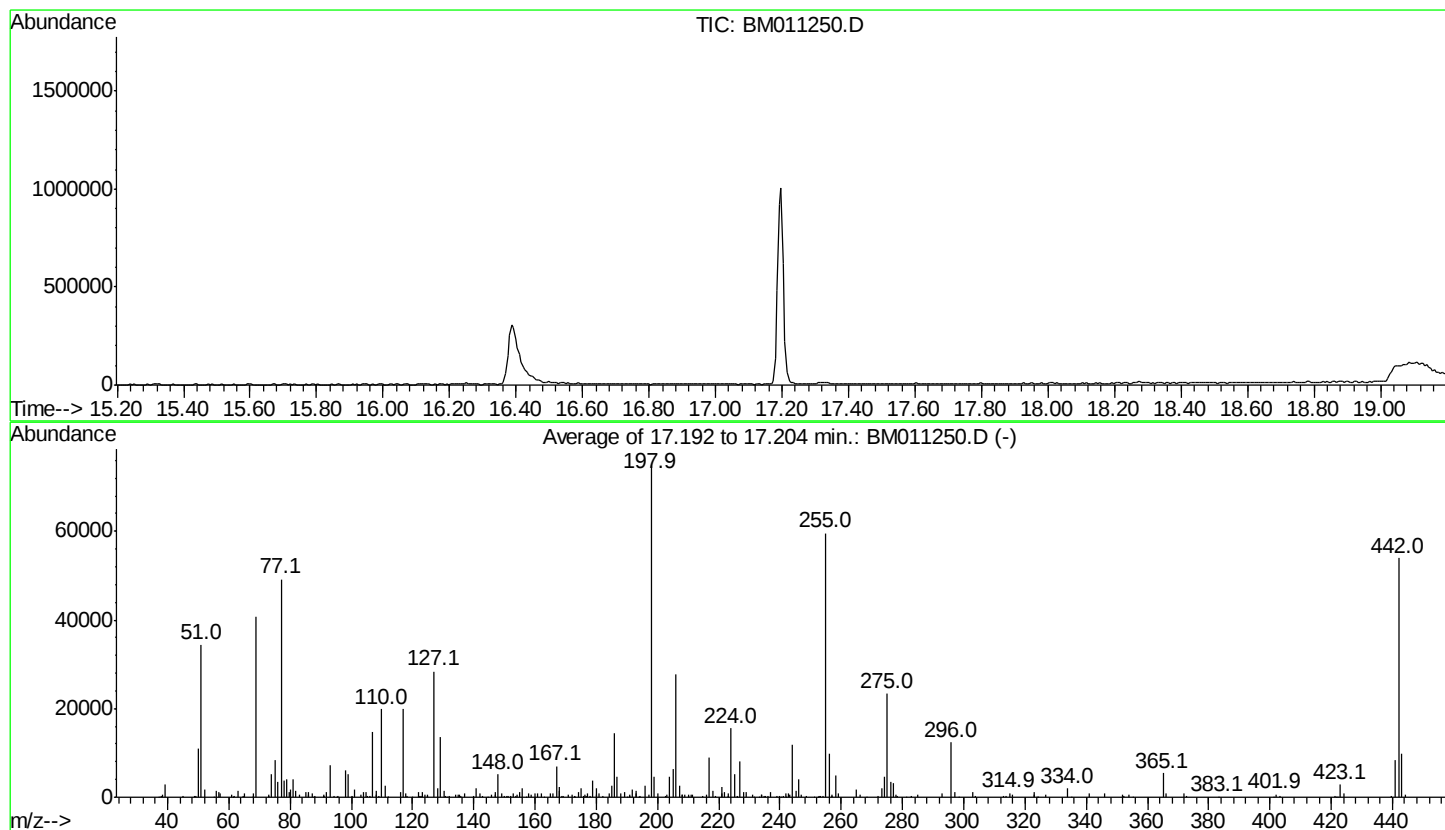

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	34509	PASS
68	69	0.00	2	2.0	831	PASS
69	198	0.00	100	54.4	40730	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.9	28328	PASS
197	198	0.00	2	0.7	534	PASS
198	198	100	100	100.0	74834	PASS
199	198	5	9	6.3	4742	PASS
275	198	10	60	31.3	23392	PASS
365	198	1	100	7.2	5396	PASS
441	442	0.01	24	15.5	8334	PASS
442	198	50	100	72.1	53933	PASS
443	442	15	24	18.2	9815	PASS