

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
 Data File : BM036302.D
 Acq On : 16 Aug 2022 16:12
 Operator : CG/JU
 Sample : PB147024BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	35	rVB	76303	101676	2.45%	0.204%
2	3.634	91	93	111	rBV	820830	1204181	29.06%	2.415%
3	3.957	144	148	153	rVB	18285	23634	0.57%	0.047%
4	6.986	656	663	680	rBV	889358	1468365	35.43%	2.944%
5	7.139	682	689	700	rBV	793542	1221551	29.48%	2.449%
6	7.333	715	722	736	rBV	961392	1509832	36.43%	3.027%
7	7.804	794	802	812	rBV	824579	1329276	32.08%	2.665%
8	8.528	918	925	939	rBV	1088599	1802432	43.49%	3.614%
9	8.969	993	1000	1012	rBV	866475	1451647	35.03%	2.911%
10	9.692	1115	1123	1136	rBV	695090	1167988	28.18%	2.342%
11	9.798	1139	1141	1146	rVB5	3252	4551	0.11%	0.009%
12	10.233	1208	1215	1239	rBV	952101	1731251	41.77%	3.471%
13	10.386	1239	1241	1245	rVB5	3237	4233	0.10%	0.008%
14	10.604	1270	1278	1291	rBV	1182496	1944037	46.91%	3.898%
15	10.751	1296	1303	1334	rBV	992599	1908720	46.06%	3.827%
16	12.216	1545	1552	1559	rBV2	11935	28644	0.69%	0.057%
17	13.868	1826	1833	1848	rBV	1724071	2469784	59.60%	4.952%
18	14.139	1873	1879	1894	rBV	2124867	3062774	73.90%	6.141%
19	14.445	1924	1931	1946	rVB	1591326	2326209	56.13%	4.664%
20	14.674	1964	1970	2000	rBV	458857	1105223	26.67%	2.216%
21	15.439	2090	2100	2114	rBV	2670990	3759568	90.72%	7.538%
22	15.568	2117	2122	2137	rVV	554041	906524	21.87%	1.818%
23	15.680	2137	2141	2158	rVB	33882	78297	1.89%	0.157%
24	16.221	2230	2233	2239	rVB5	7993	11504	0.28%	0.023%
25	16.662	2302	2308	2310	rVB6	4499	6585	0.16%	0.013%
26	16.868	2341	2343	2348	rVB5	5413	7218	0.17%	0.014%
27	16.980	2360	2362	2368	rVB5	4500	7577	0.18%	0.015%
28	17.192	2391	2398	2407	rBV	1658750	2349107	56.68%	4.710%
29	17.292	2408	2415	2429	rVV	2609485	3855683	93.04%	7.731%
30	17.721	2485	2488	2493	rBV7	3811	7407	0.18%	0.015%
31	17.786	2495	2499	2502	rBV5	3502	4519	0.11%	0.009%
32	19.150	2727	2731	2737	rVB3	29335	38137	0.92%	0.076%
33	19.221	2740	2743	2751	rVB2	24667	37445	0.90%	0.075%
34	19.586	2799	2805	2816	rBV	2999329	4050530	97.74%	8.122%
35	20.586	2972	2975	2980	rBV2	80434	89710	2.16%	0.180%
36	21.374	3104	3109	3120	rBV	1778456	2350678	56.72%	4.713%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036302.D
Acq On : 16 Aug 2022 16:12
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37	23.556	3473	3480	3493	rBV	2143653	4144238	100.00%	8.310%
38	23.703	3500	3505	3515	rVB2	1176400	2301575	55.54%	4.615%




Sum of corrected areas: 49872310

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036302.D
Acq On : 16 Aug 2022 16:12
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

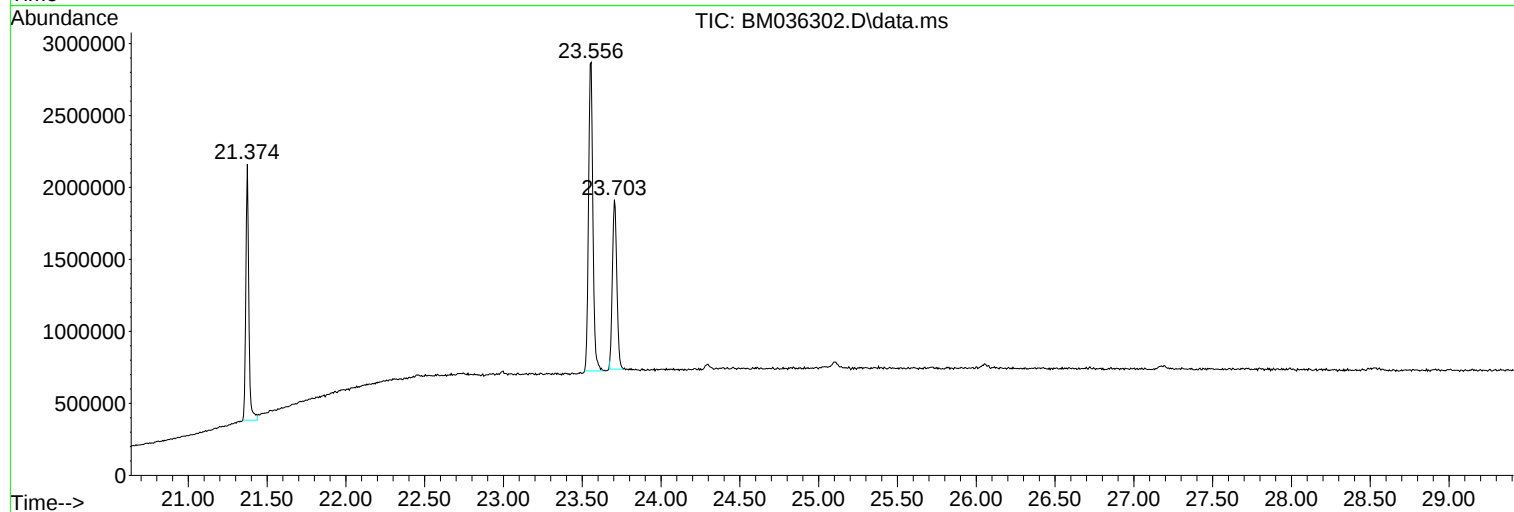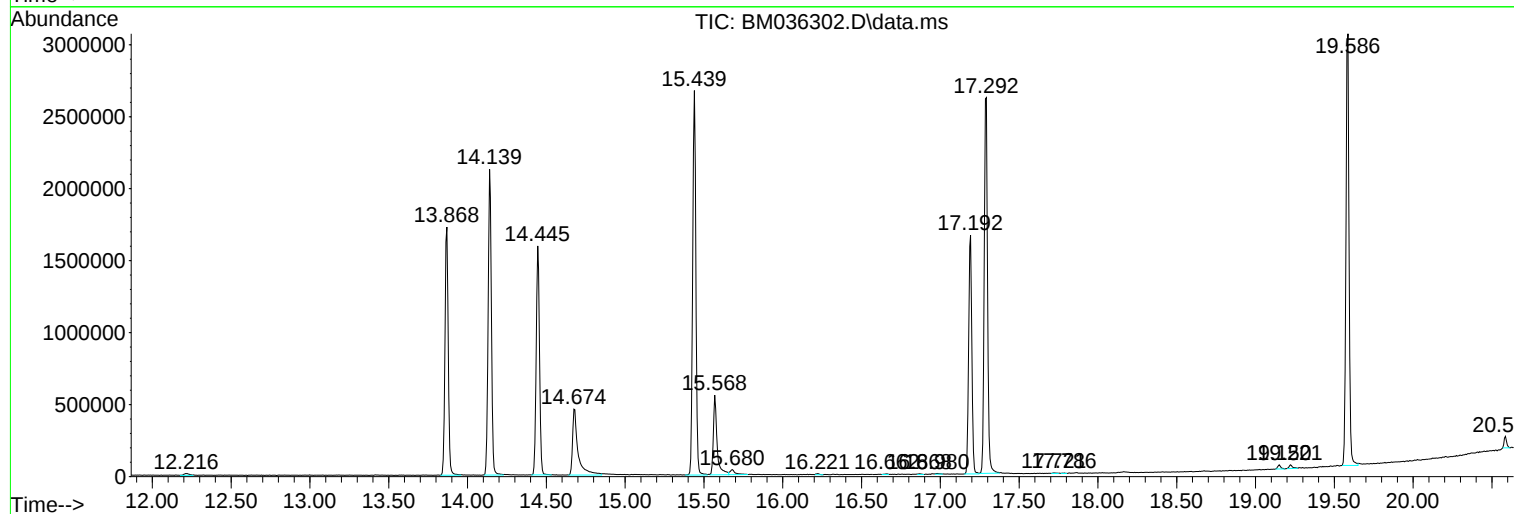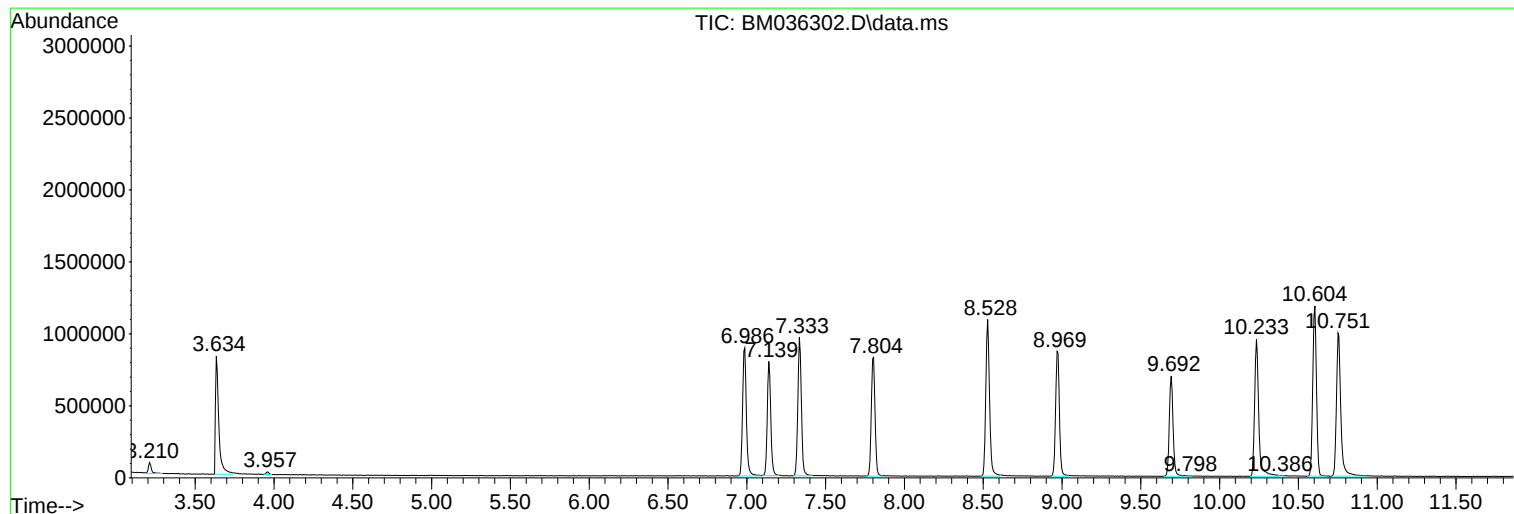

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036302.D
Acq On : 16 Aug 2022 16:12
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036302.D
Acq On : 16 Aug 2022 16:12
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc