

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
 Data File : BM036303.D
 Acq On : 16 Aug 2022 16:49
 Operator : CG/JU
 Sample : N4194-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.957	145	148	156	rVB	14609	19491	0.96%	0.192%
2	4.540	245	247	252	rVB6	1751	2120	0.10%	0.021%
3	4.893	304	307	309	rBV3	2205	2873	0.14%	0.028%
4	5.551	417	419	425	rVB5	2486	2931	0.14%	0.029%
5	5.910	478	480	485	rVB5	1804	2041	0.10%	0.020%
6	6.098	508	512	515	rBV5	1639	2917	0.14%	0.029%
7	6.128	515	517	519	rVB2	3011	2331	0.11%	0.023%
8	6.828	635	636	641	rVB5	2518	2798	0.14%	0.028%
9	6.916	648	651	657	rVB7	2222	3537	0.17%	0.035%
10	7.804	794	802	820	rBV	590592	1010968	49.87%	9.953%
11	8.375	896	899	904	rBV5	1865	3445	0.17%	0.034%
12	8.516	921	923	926	rBV3	1800	2307	0.11%	0.023%
13	8.563	926	931	932	rVB5	2349	3431	0.17%	0.034%
14	8.992	1002	1004	1007	rBV4	1851	2052	0.10%	0.020%
15	9.675	1119	1120	1124	rBV4	2316	2856	0.14%	0.028%
16	9.845	1146	1149	1153	rVB5	1837	3078	0.15%	0.030%
17	10.516	1260	1263	1265	rBV4	1898	2492	0.12%	0.025%
18	10.604	1271	1278	1303	rBV	754068	1386345	68.39%	13.649%
19	10.804	1309	1312	1314	rBV3	1757	2102	0.10%	0.021%
20	11.351	1400	1405	1407	rBV5	2080	2949	0.15%	0.029%
21	13.098	1699	1702	1705	rBV4	2125	3086	0.15%	0.030%
22	13.557	1777	1780	1783	rVB4	1734	2536	0.13%	0.025%
23	13.739	1806	1811	1814	rVB7	1329	2557	0.13%	0.025%
24	14.145	1879	1880	1886	rVB5	1960	2945	0.15%	0.029%
25	14.227	1890	1894	1895	rVB3	2215	2219	0.11%	0.022%
26	14.251	1895	1898	1900	rBV4	1731	2194	0.11%	0.022%
27	14.445	1924	1931	1946	rBV	1065656	1677024	82.73%	16.510%
28	14.657	1964	1967	1969	rVB4	2387	2332	0.12%	0.023%
29	15.157	2048	2052	2055	rVB5	2377	3927	0.19%	0.039%
30	15.192	2055	2058	2062	rBV5	2709	3476	0.17%	0.034%
31	15.409	2090	2095	2098	rVB5	2063	2744	0.14%	0.027%
32	15.621	2128	2131	2135	rVB5	1631	2123	0.10%	0.021%
33	15.662	2135	2138	2143	rVB4	1986	2410	0.12%	0.024%
34	15.792	2156	2160	2162	rVB5	2146	2802	0.14%	0.028%
35	15.833	2162	2167	2170	rBV6	2341	3565	0.18%	0.035%
36	16.451	2268	2272	2274	rBV4	2464	4088	0.20%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
 Data File : BM036303.D
 Acq On : 16 Aug 2022 16:49
 Operator : CG/JU
 Sample : N4194-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M

Title : SVOA CALIBRATION

37	16.615	2296	2300	2303	rBV5	1641	2279	0.11%	0.022%
38	16.656	2303	2307	2311	rVB5	2865	4003	0.20%	0.039%
39	16.733	2318	2320	2322	rBV3	2424	2441	0.12%	0.024%
40	17.121	2383	2386	2389	rBV4	2393	4144	0.20%	0.041%
41	17.192	2391	2398	2420	rBV	1182019	1855907	91.56%	18.272%
42	18.145	2556	2560	2561	rBV4	4465	6387	0.32%	0.063%
43	20.586	2972	2975	2980	rBV2	53704	63607	3.14%	0.626%
44	21.374	3104	3109	3120	rBV	1443254	2027012	100.00%	19.956%
45	23.703	3499	3505	3516	rBV2	1028483	2008495	99.09%	19.774%




Sum of corrected areas: 10157367

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036303.D
Acq On : 16 Aug 2022 16:49
Operator : CG/JU
Sample : N4194-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

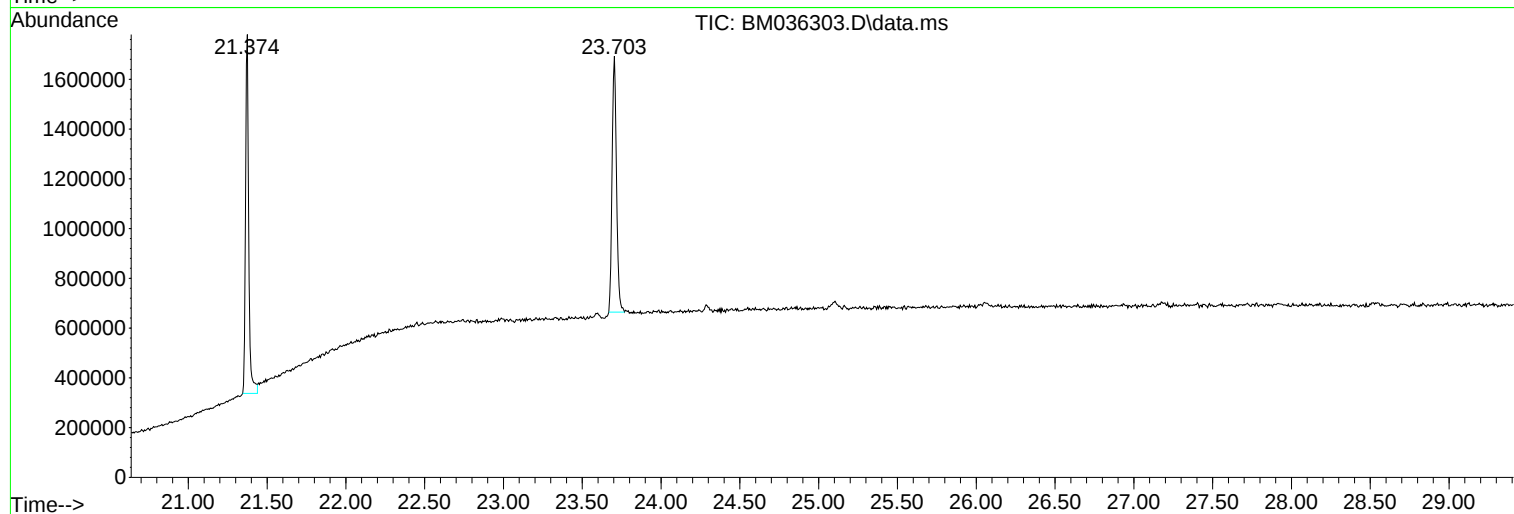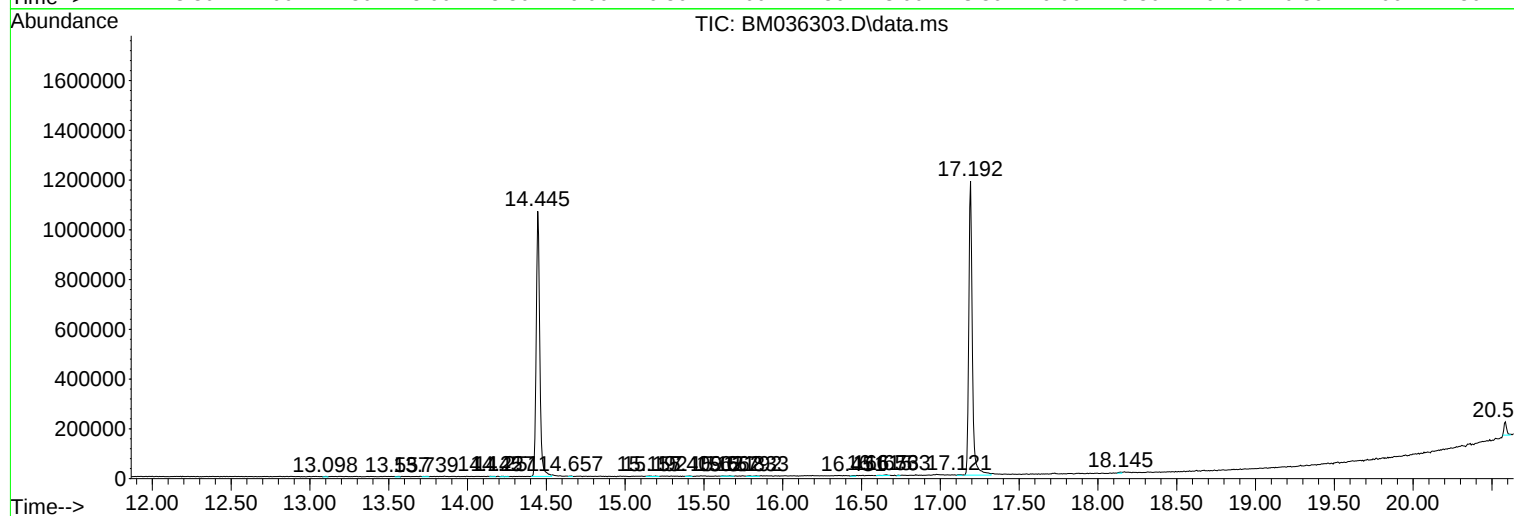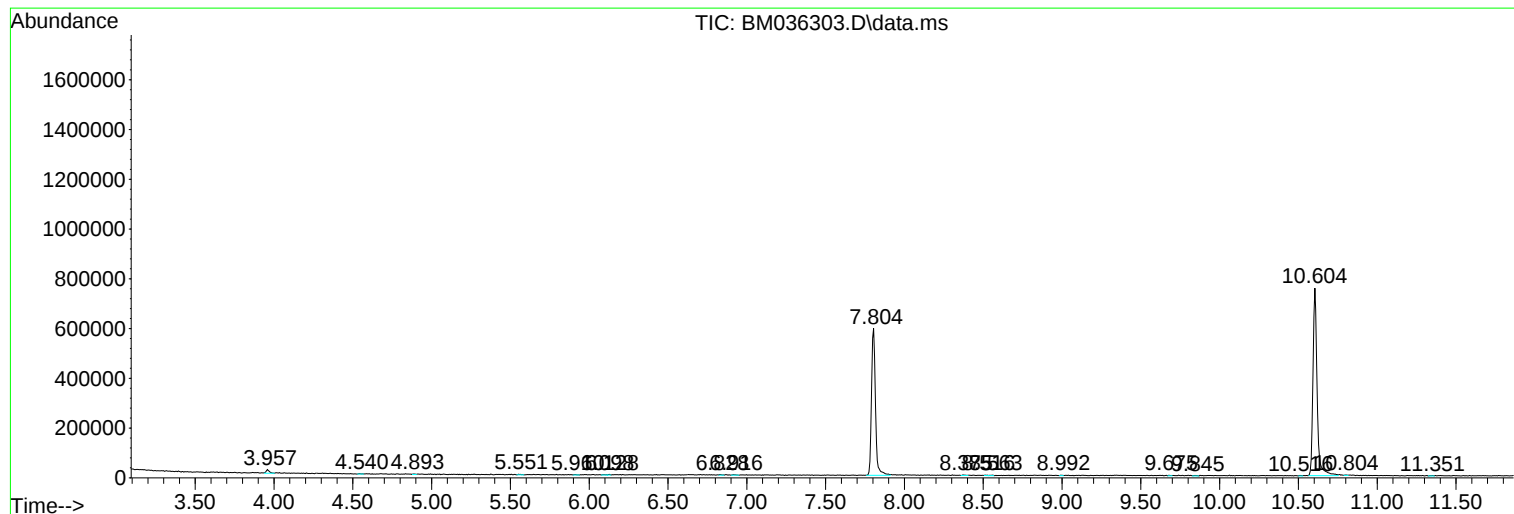

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036303.D
Acq On : 16 Aug 2022 16:49
Operator : CG/JU
Sample : N4194-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081622\
Data File : BM036303.D
Acq On : 16 Aug 2022 16:49
Operator : CG/JU
Sample : N4194-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc