

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081624\
 Data File : BM047228.D
 Acq On : 16 Aug 2024 10:27
 Operator : RC/JU
 Sample : PB162754BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB162754BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM047228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.575	282	287	295	rVB	297038	412453	2.68%	0.558%
2	5.022	356	363	381	rBV	4777326	6947966	45.11%	9.405%
3	6.581	620	628	643	rBV	4635778	7273096	47.23%	9.845%
4	7.363	753	761	769	rBV	1142527	1739620	11.30%	2.355%
5	8.510	947	956	973	rBV	3031704	4893285	31.77%	6.623%
6	10.116	1222	1229	1243	rBV	1404619	2339792	15.19%	3.167%
7	12.628	1649	1656	1672	rBV	7688940	11581198	75.20%	15.676%
8	14.022	1885	1893	1910	rBV	2327615	3351724	21.76%	4.537%
9	15.528	2143	2149	2168	rBV	6058814	9245362	60.03%	12.514%
10	16.786	2356	2363	2369	rBV	2854900	3961098	25.72%	5.362%
11	17.722	2517	2522	2537	rBV	145981	310355	2.02%	0.420%
12	19.451	2810	2816	2822	rBV	12430228	15400749	100.00%	20.846%
13	21.021	3078	3083	3091	rBV	2470159	3271334	21.24%	4.428%
14	23.715	3534	3541	3558	rVB	1355997	3150119	20.45%	4.264%




Sum of corrected areas: 73878151

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081624\
Data File : BM047228.D
Acq On : 16 Aug 2024 10:27
Operator : RC/JU
Sample : PB162754BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162754BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

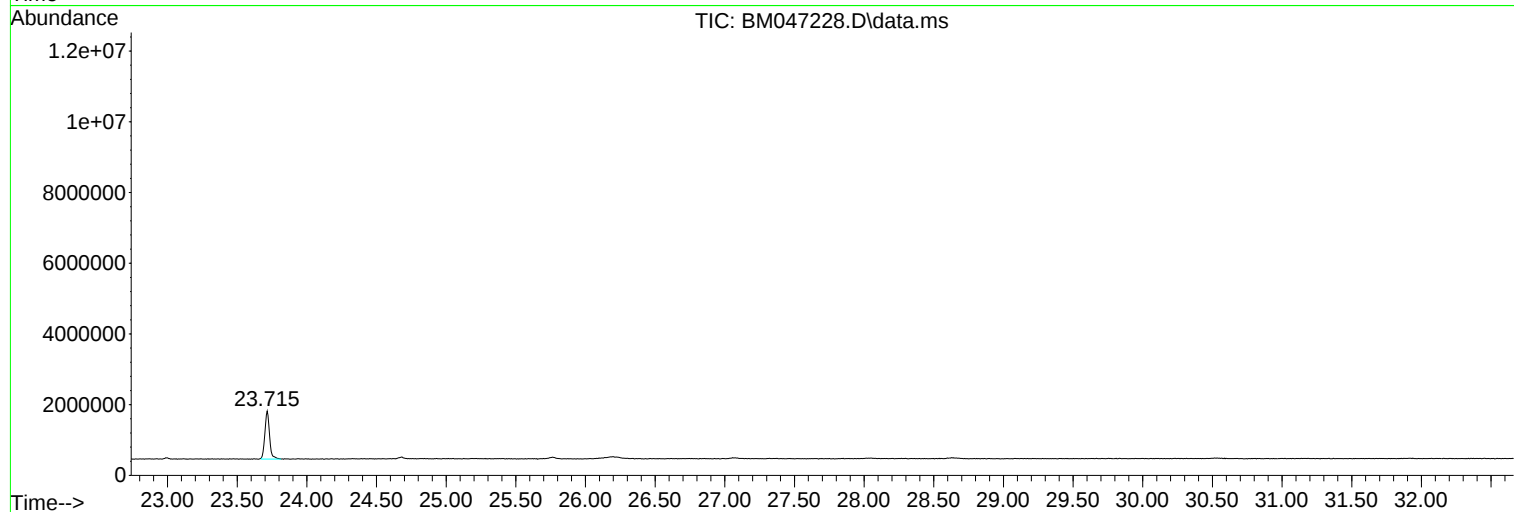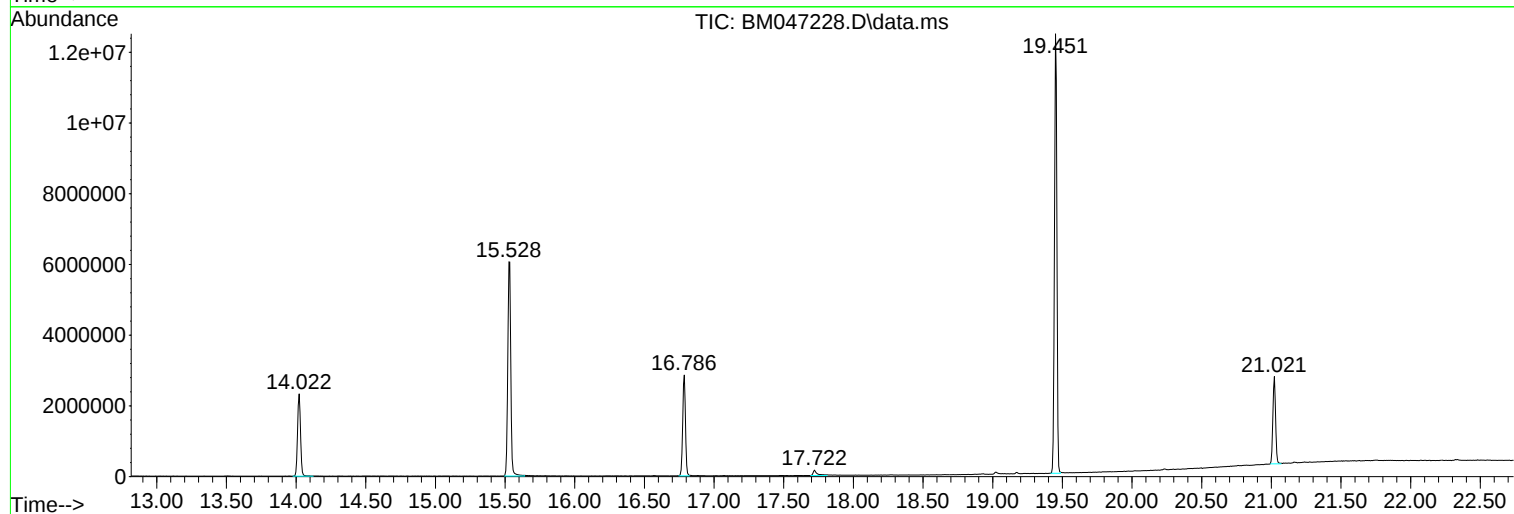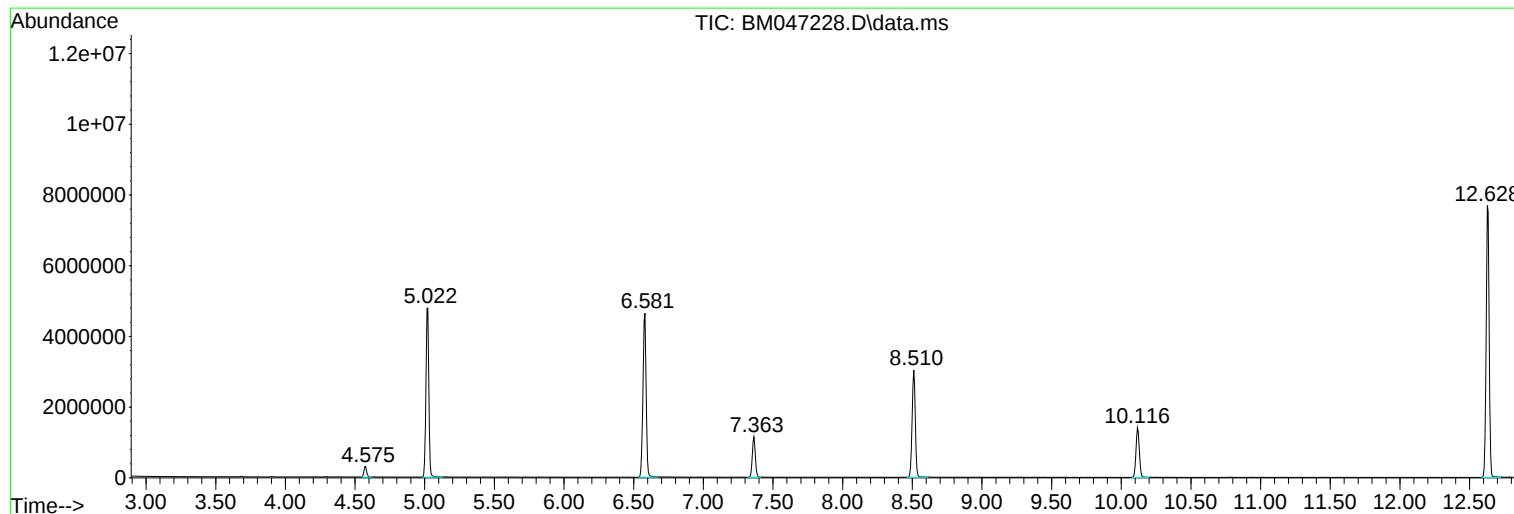

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081624\
Data File : BM047228.D
Acq On : 16 Aug 2024 10:27
Operator : RC/JU
Sample : PB162754BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162754BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.575	4.74 ng	412453	1,4-Dichlorobenzene-d4	7.363

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

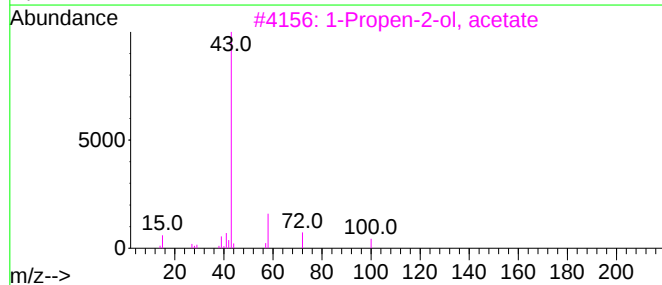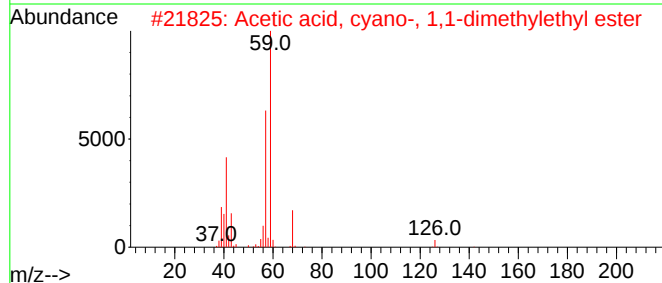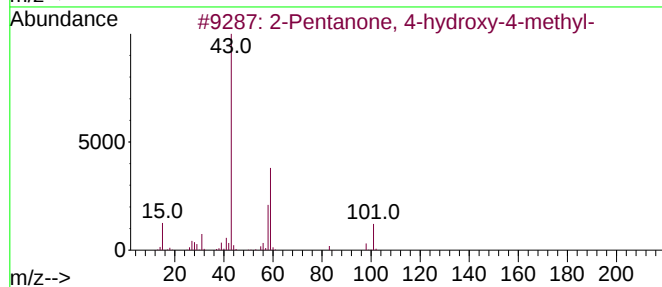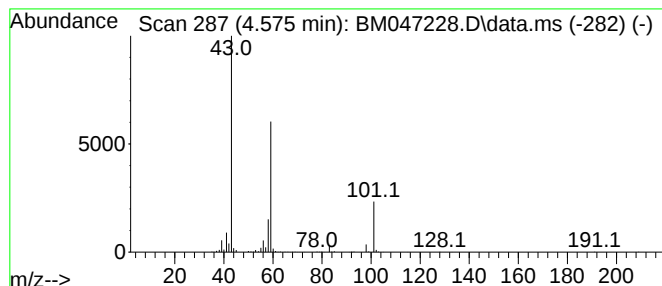

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081624\
Data File : BM047228.D
Acq On : 16 Aug 2024 10:27
Operator : RC/JU
Sample : PB162754BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB162754BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.575	4.7	ng	412453	1	7.363	1739620	20.0