
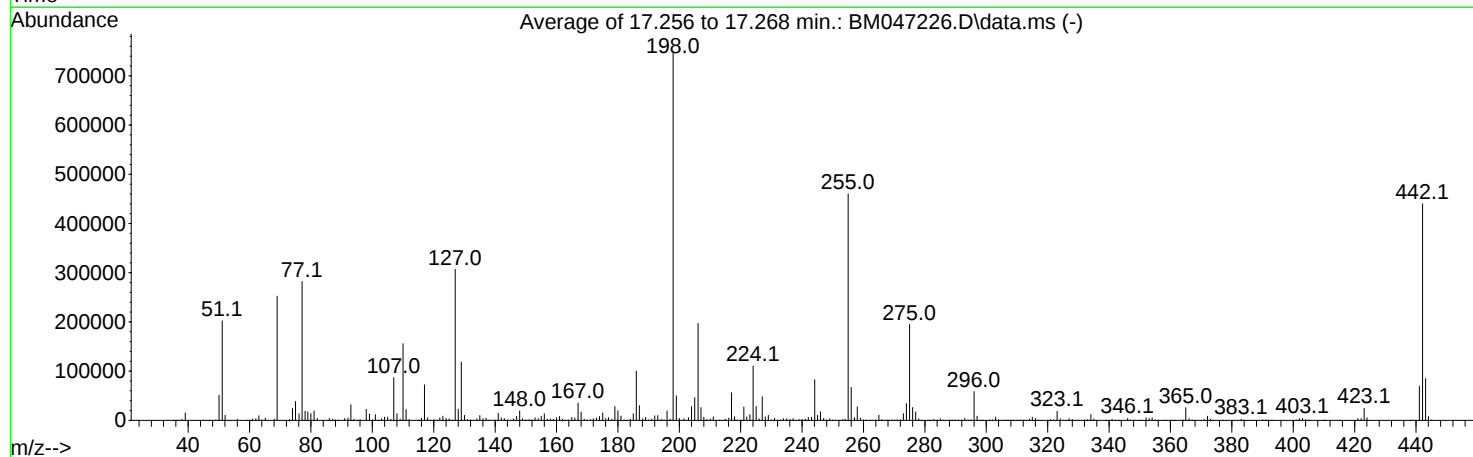


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081624\
Data File : BM047226.D
Acq On : 16 Aug 2024 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

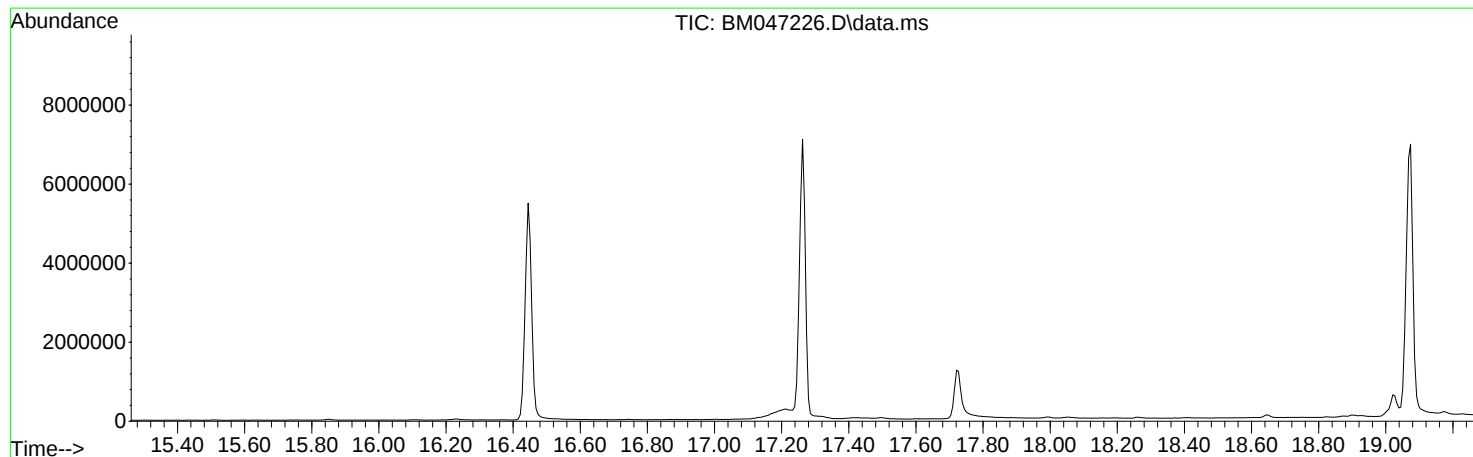

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	202212	PASS
68	69	0.00	2	1.0	2550	PASS
69	198	0.00	100	33.8	252268	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	306704	PASS
197	198	0.00	2	0.3	2488	PASS
198	198	100	100	100.0	747456	PASS
199	198	5	9	6.7	50011	PASS
275	198	10	60	26.1	194773	PASS
365	198	1	100	3.4	25557	PASS
441	198	0.01	100	9.3	69304	PASS
442	442	50	100	100.0	440021	PASS
443	442	15	24	19.3	84829	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/16/2024	BNA_M	<u>BM047226.D</u>
Compound Name	Response	Retention Time
DDT	2267239	20.315
DDD	136978	19.874
DDE	2317	19.362
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
139295	2406534	5.79

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081624\
Data File : BM047226.D
Acq On : 16 Aug 2024 09:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 16 11:27:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

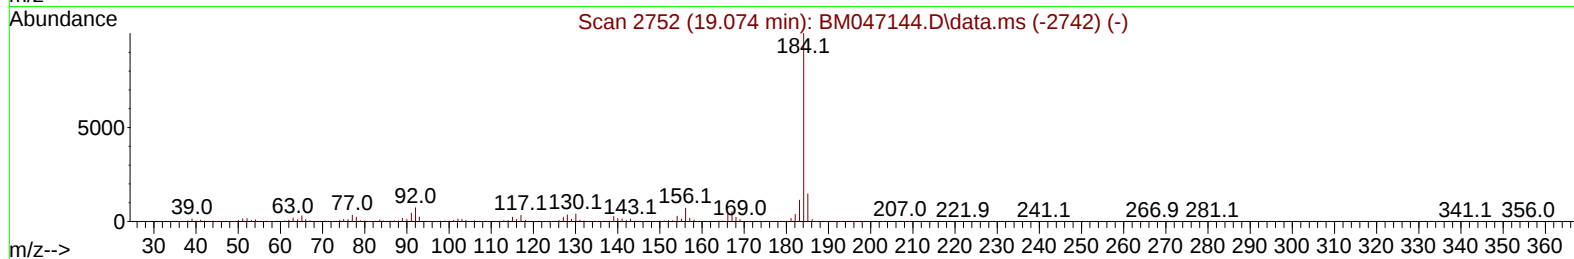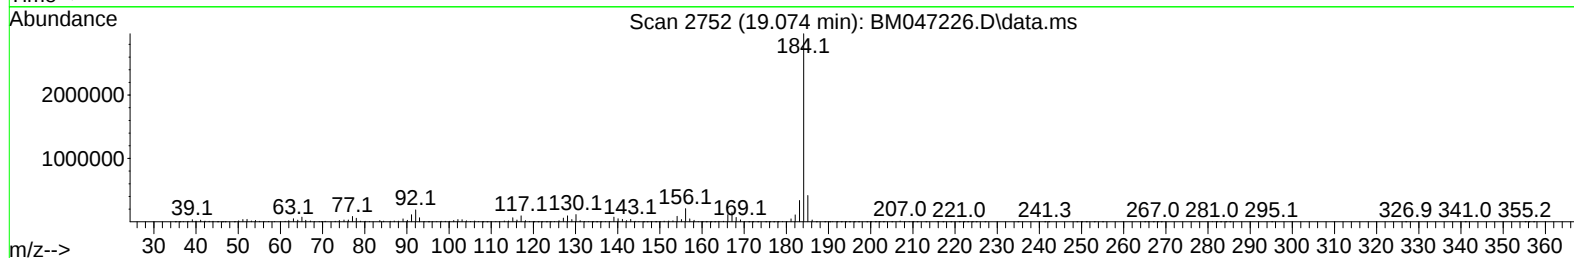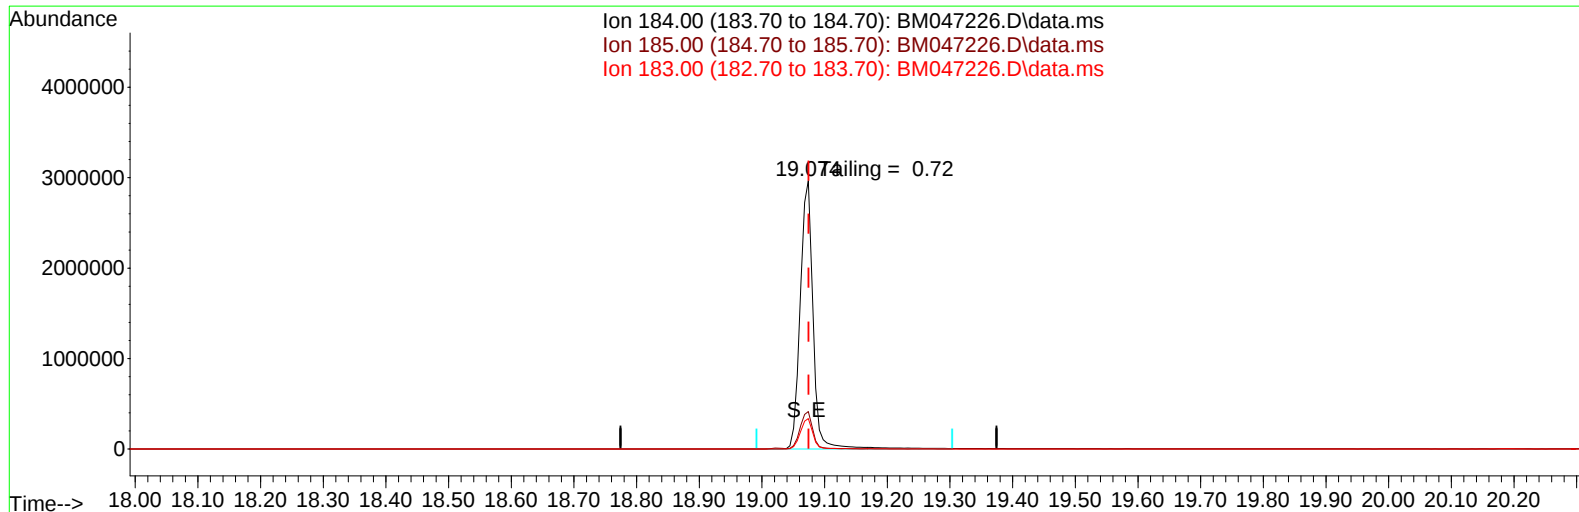

TIC: BM047226.D\data.ms

(77) Benzidine

19.074min (-0.000) 123625.67 ng

response 4262186

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.99
183.00	11.30	11.33
0.00	0.00	0.00