

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081715\
 Data File : BM002460.D
 Acq On : 17 Aug 2015 20:32
 Operator : UM/IZ
 Sample : G3227-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 18 02:03:16 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 18 01:54:16 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.88	152	144098	20.00	ng/ul	0.00
2) Naphthalene-d8	11.75	136	647995	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.46	164	329353	20.00	ng/ul	0.01
12) Phenanthrene-d10	18.17	188	598646	20.00	ng/ul	0.00
17) Chrysene-d12	22.25	240	414701	20.00	ng/ul	0.01
22) Perylene-d12	24.94	264	410085	20.00	ng/ul	0.03
System Monitoring Compounds						
7) Acenaphthylene-d8	15.17	160	565880	16.80	ng/ul	0.01
10) Fluorene-d10	16.43	176	376807	15.93	ng/ul	0.01
14) Anthracene-d10	18.27	188	487903	16.90	ng/ul	0.01
18) Pyrene-d10	20.49	212	384964	20.94	ng/ul	0.01
25) Benzo(a)pyrene-d12	24.76	264	328622	15.26	ng/ul	0.02
Target Compounds						
					Ovalue	
3) Naphthalene	11.80	128	92075	2.78	ng/ul	99
4) 2-Methylnaphthalene	13.34	142	57880	2.34	ng/ul	98
5) 1-Methylnaphthalene	13.56	142	41227	1.68	ng/ul	99
8) Acenaphthylene	15.19	152	87325	2.48	ng/ul	99
13) Phenanthrene	18.21	178	300235	8.69	ng/ul	100
15) Anthracene	18.30	178	114209	3.26	ng/ul	100
16) Fluoranthene	20.16	202	607744	15.53	ng/ul	99
19) Pyrene	20.52	202	527528	21.71	ng/ul	99
20) Benzo(a)anthracene	22.23	228	321784	12.98	ng/ul	96
21) Chrysene	22.29	228	401983	17.33	ng/ul	96
23) Benzo(b)fluoranthene	24.11	252	923911	37.27	ng/ul#	95
24) Benzo(k)fluoranthene	24.31	252	134210	5.71	ng/ul#	75
26) Benzo(a)pyrene	24.82	252	686758	29.00	ng/ul	96
27) Indeno(1,2,3-cd)pyrene	27.79	276	765754	28.12	ng/ul	94
28) Dibenzo(a,h)anthracene	27.79	278	205839	9.04	ng/ul#	84
29) Benzo(a,h,i)perylene	28.69	276	731826	32.28	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081715\
Data File : BM002460.D
Acq On : 17 Aug 2015 20:32
Operator : UM/IZ
Sample : G3227-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 18 02:03:16 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 18 01:54:16 2015
Response via : Initial Calibration

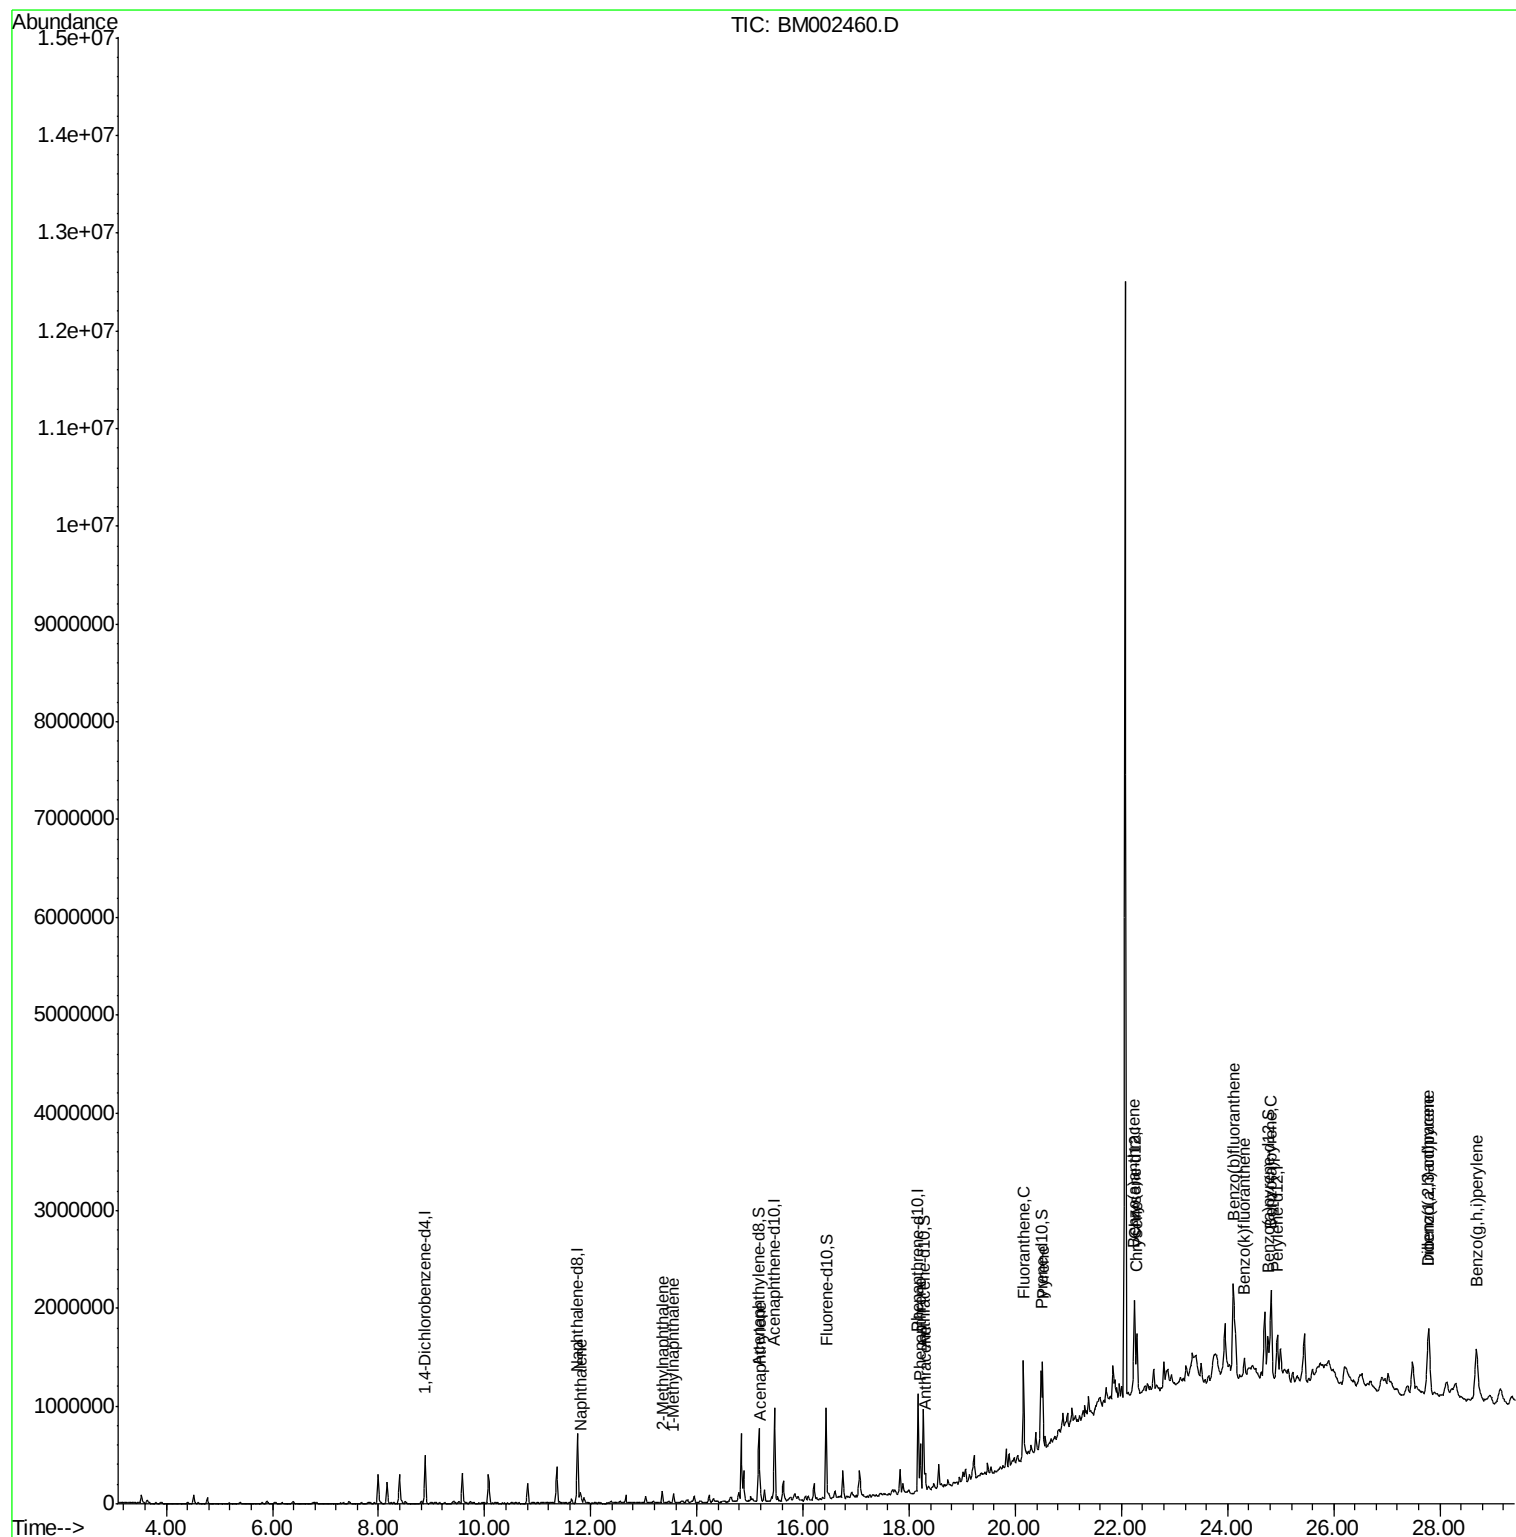

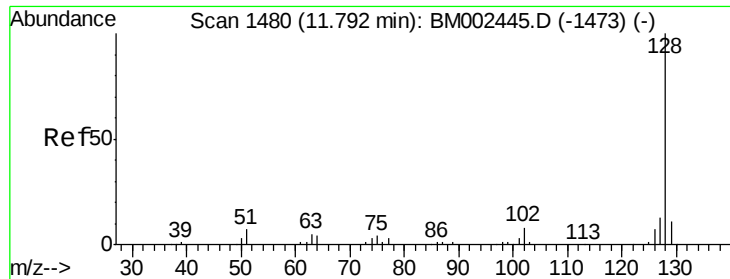

#3

Naphthalene

Concen: 2.78 ng/ul

RT: 11.80 min Scan# 1482

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 92075

Ion Ratio Lower Upper

128 100

129 11.1 8.6 12.8




127 12.9 10.4 15.6

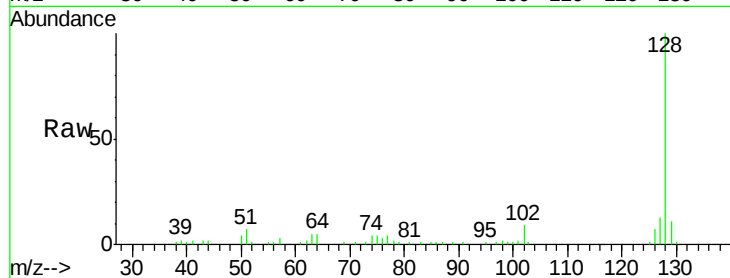

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

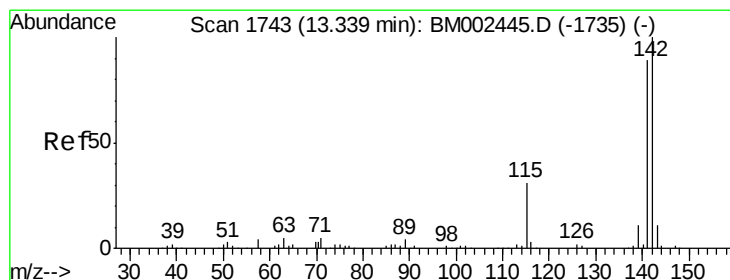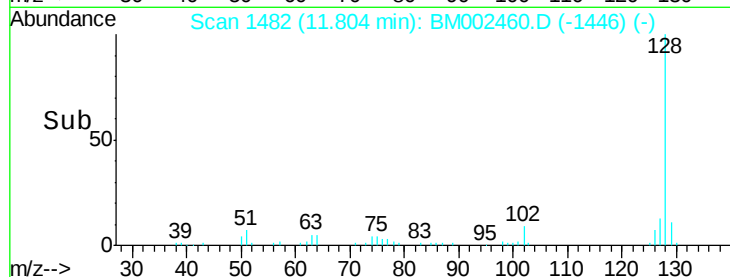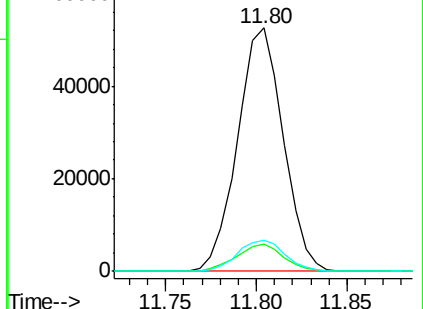

#4

2-Methylnaphthalene

Concen: 2.34 ng/ul

RT: 13.34 min Scan# 1744

Delta R.T. 0.01 min

Lab File: BM002460.D


Acq: 17 Aug 2015 20:32

Tgt Ion:142 Resp: 57880

Ion Ratio Lower Upper



142 100


141 88.7 72.2 108.2

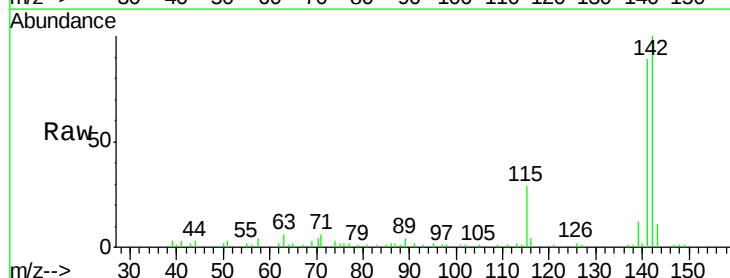

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

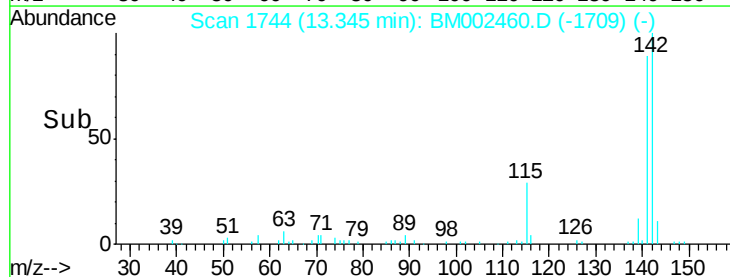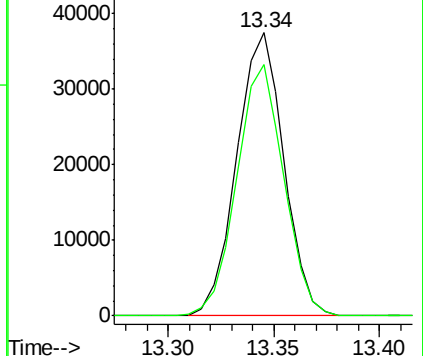

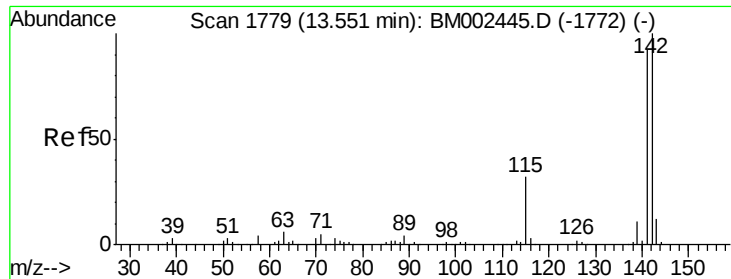

#5

1-Methylnaphthalene

Concen: 1.68 ng/ul

RT: 13.56 min Scan# 1780

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:142 Resp: 41227

Ion Ratio Lower Upper

142 100

141 93.0 73.9 110.9




116 3.8 3.0 4.4

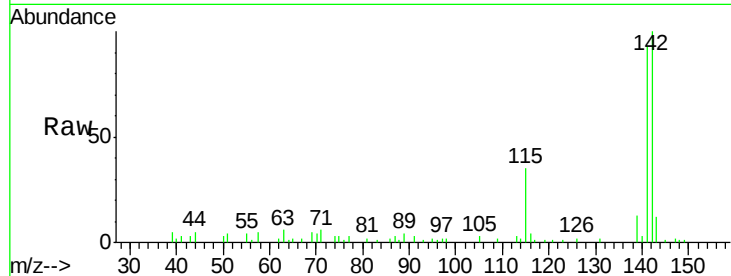

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

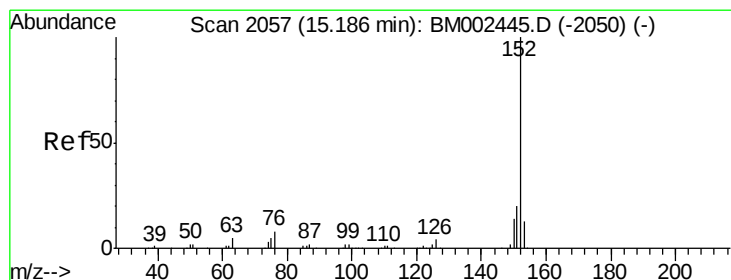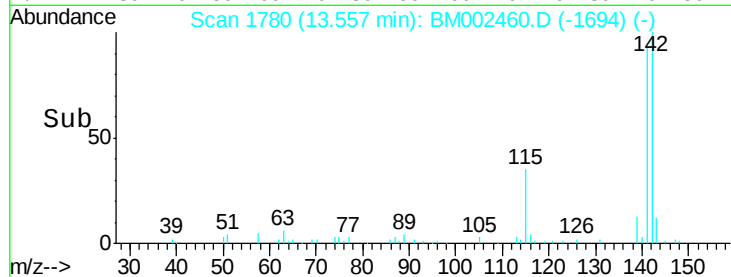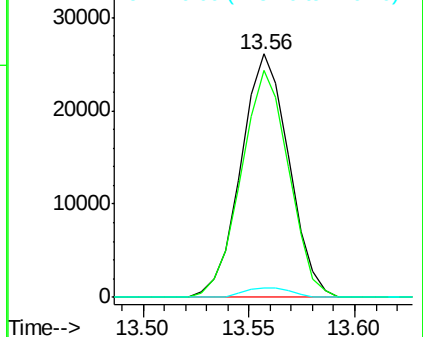

#8

Acenaphthylene

Concen: 2.48 ng/ul

RT: 15.19 min Scan# 2058

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32


Tgt Ion:152 Resp: 87325

Ion Ratio Lower Upper

152 100

151 20.1 15.7 23.5



153 13.1 10.2 15.4

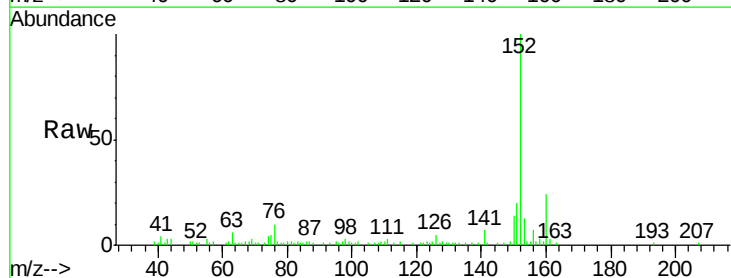


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

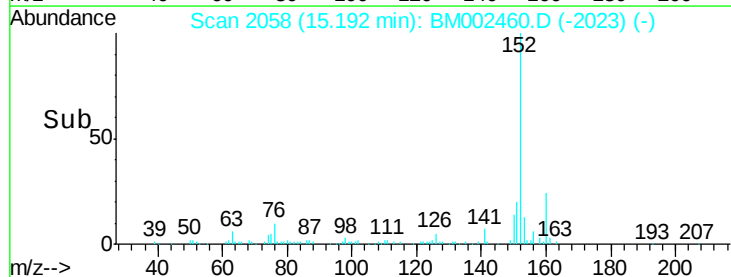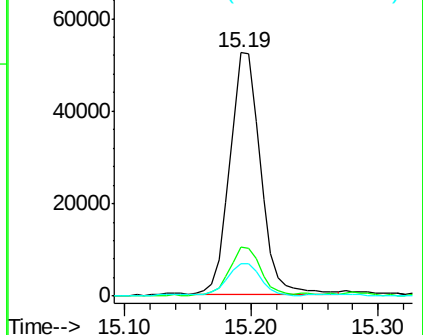

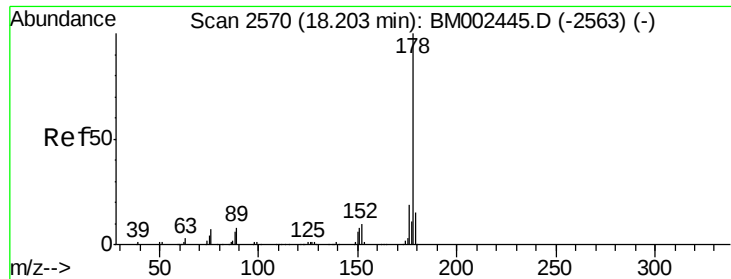

#13

Phenanthrene

Concen: 8.69 ng/ul

RT: 18.21 min Scan# 2571

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampled :


Tot Ion:178 Resp: 300235

Ion Ratio Lower Upper

178 100

179 15.4 12.4 18.6




176 18.7 15.1 22.7

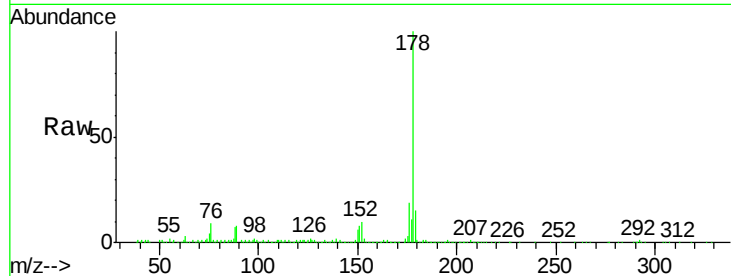

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

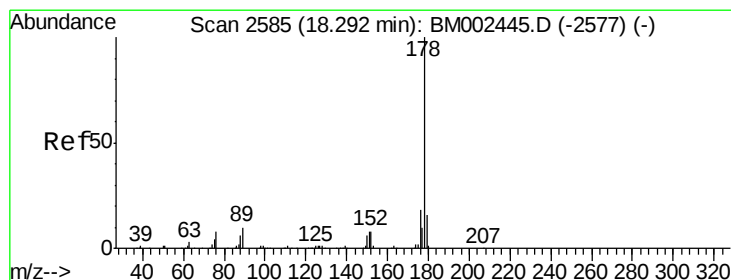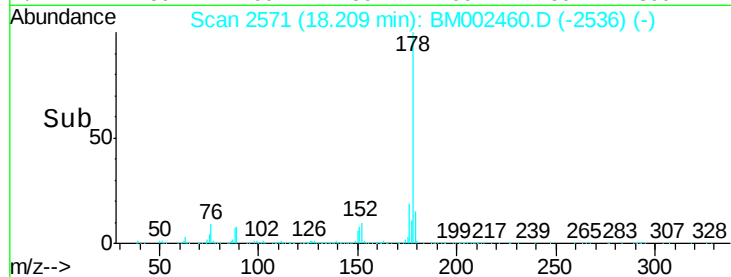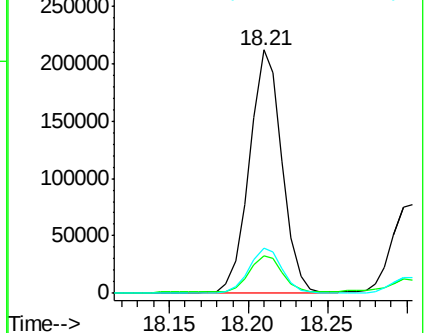

#15

Anthracene

Concen: 3.26 ng/ul

RT: 18.30 min Scan# 2587

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32


Tgt Ion:178 Resp: 114209

Ion Ratio Lower Upper

178 100

179 15.5 12.6 18.8



176 18.4 14.5 21.7

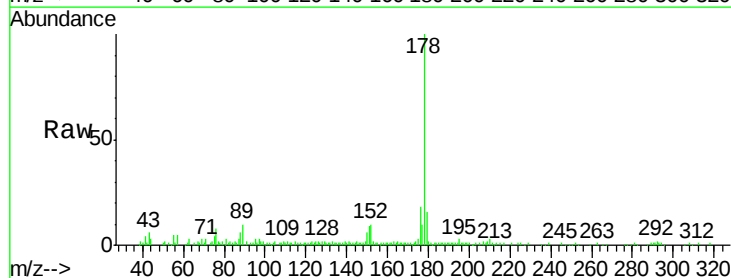


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



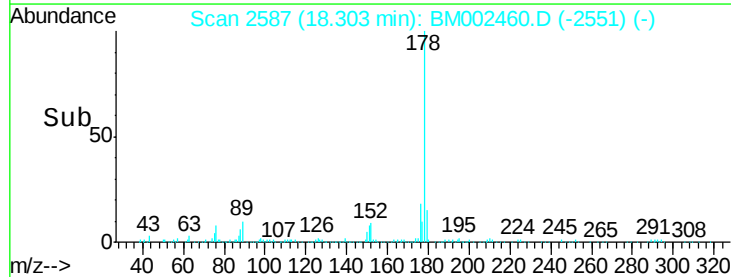
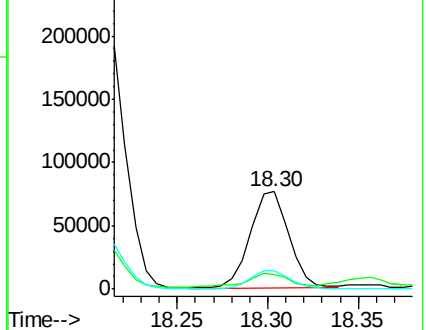


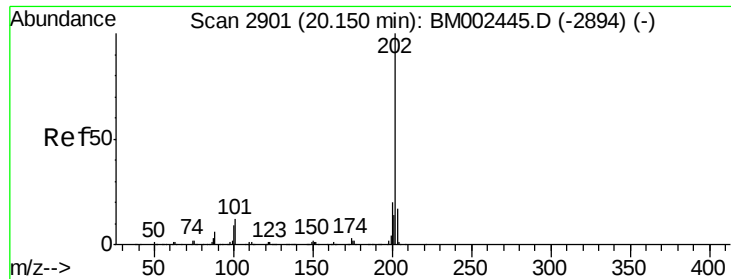

#16
 Fluoranthene
 Concen: 15.53 ng/ul
 RT: 20.16 min Scan# 2902
 Delta R.T. 0.01 min
 Lab File: BM002460.D
 Acq: 17 Aug 2015 20:32




Instrument :
 BNA_M
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
202	100		
101	12.7	9.7	14.5
100	9.8	7.4	11.2

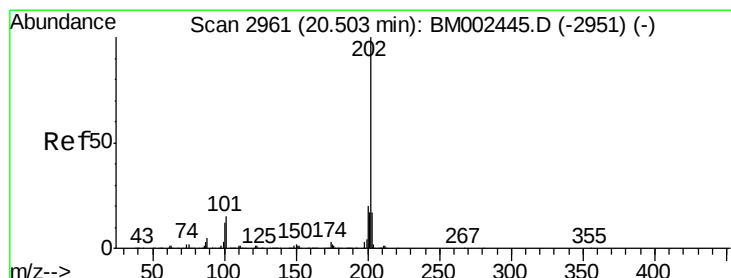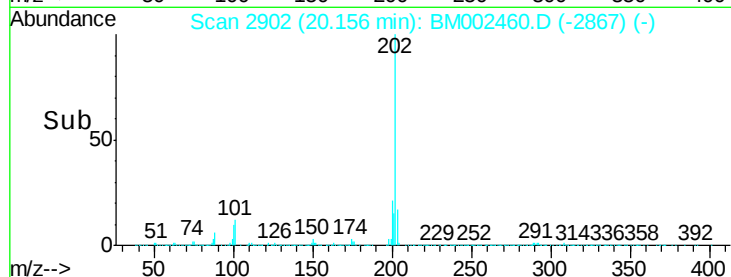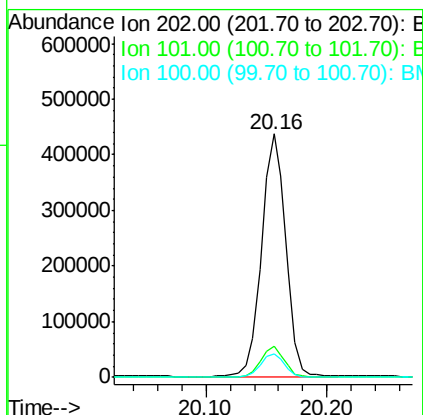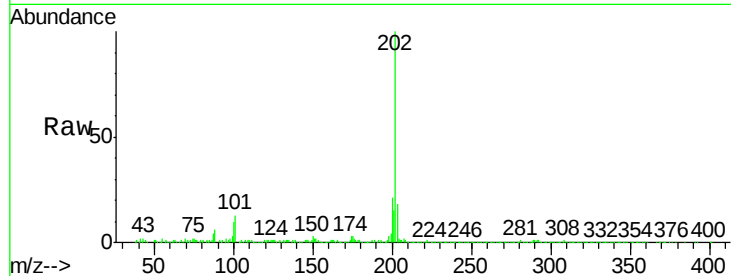

#19
 Pyrene
 Concen: 21.71 ng/ul
 RT: 20.52 min Scan# 2963
 Delta R.T. 0.01 min
 Lab File: BM002460.D
 Acq: 17 Aug 2015 20:32

Tgt Ion	Ratio	Lower	Upper
202	100		
101	14.3	12.0	18.0
100	11.6	9.7	14.5

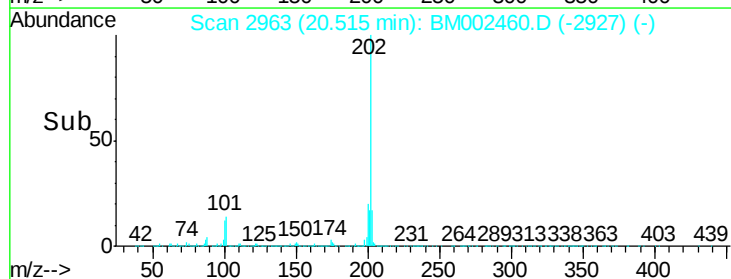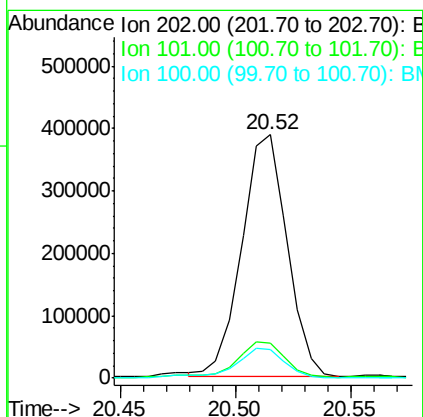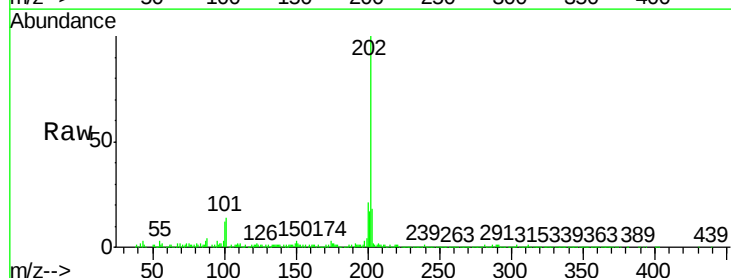

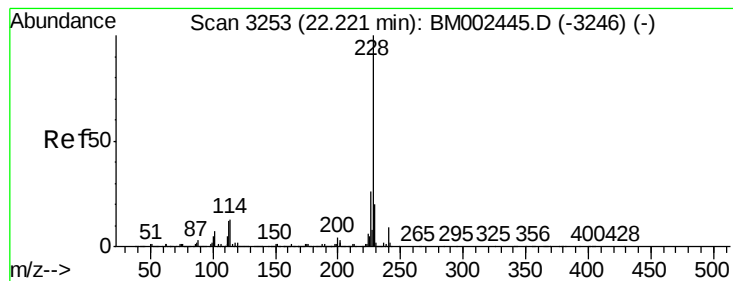

#20

Benzo(a)anthracene

Concen: 12.98 ng/ul

RT: 22.23 min Scan# 3255

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampled :


Tot Ion:228 Resp: 321784

Ion Ratio Lower Upper




228 100

229 22.1 15.8 23.6

226 28.2 21.1 31.7

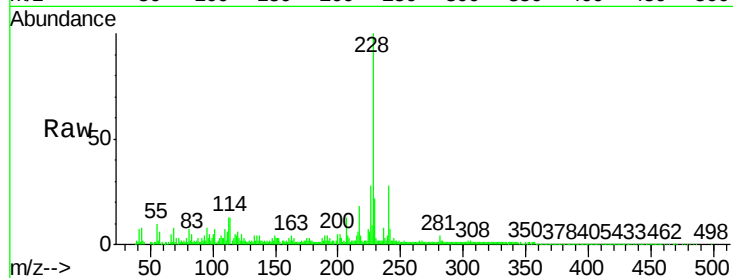

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

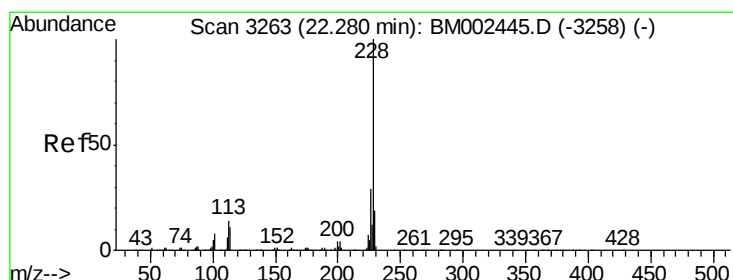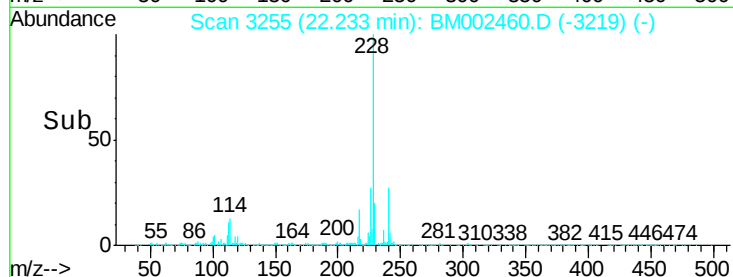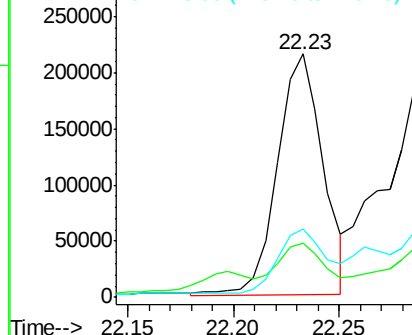

#21

Chrysene

Concen: 17.33 ng/ul

RT: 22.29 min Scan# 3265

Delta R.T. 0.01 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32


Tgt Ion:228 Resp: 401983

Ion Ratio Lower Upper



228 100


226 30.3 23.4 35.2

229 23.5 15.7 23.5

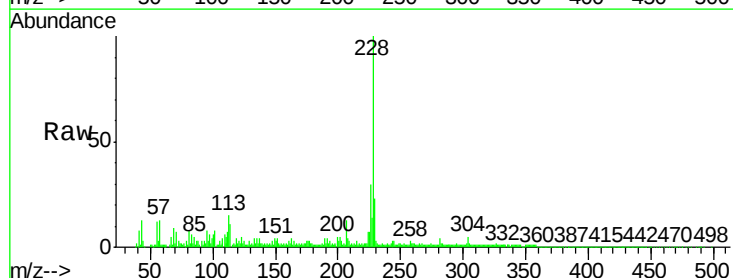

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

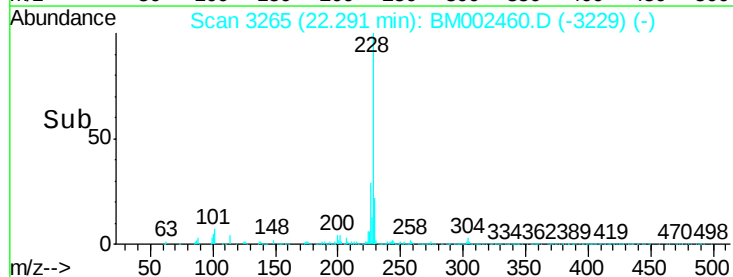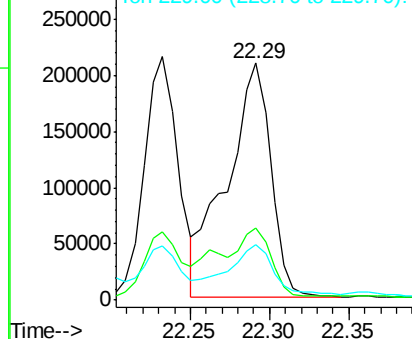

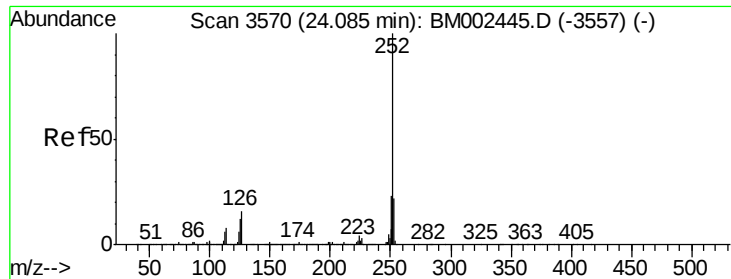

#23

Benzo(b)fluoranthene

Concen: 37.27 ng/ul

RT: 24.11 min Scan# 3574

Delta R.T. 0.02 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampled :


Tot Ion:252 Resp: 923911

Ion Ratio Lower Upper

252 100

253 23.4 17.4 26.0




125 15.2 10.0 15.0#

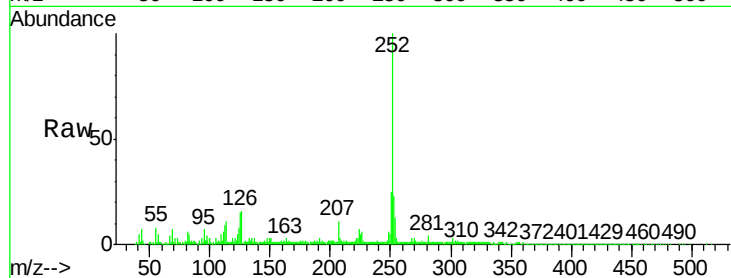

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

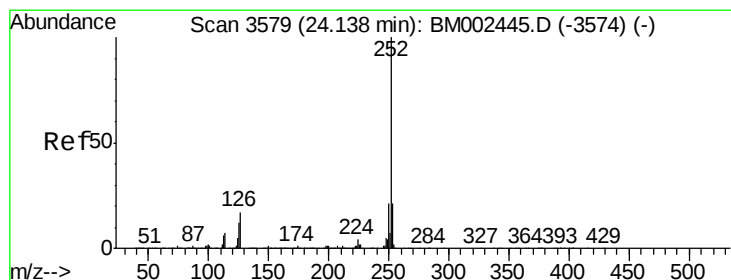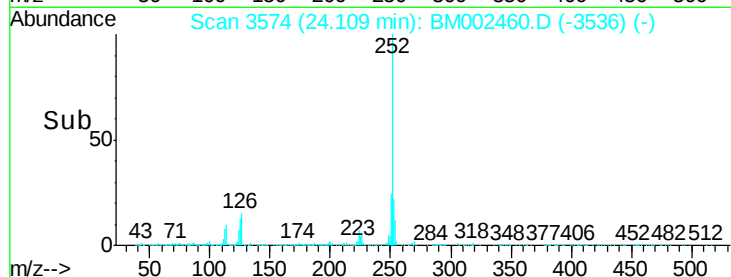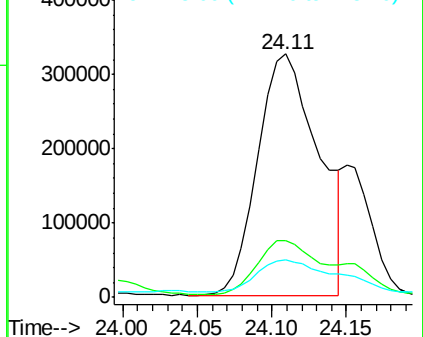

#24

Benzo(k)fluoranthene

Concen: 5.71 ng/ul

RT: 24.31 min Scan# 3609

Delta R.T. 0.18 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32


Tgt Ion:252 Resp: 134210

Ion Ratio Lower Upper

252 100

253 32.2 17.8 26.6#



125 24.5 9.8 14.8#

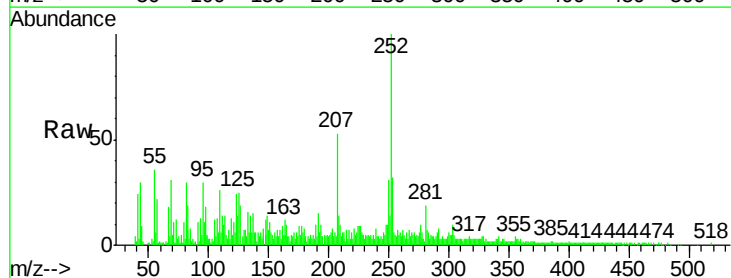


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

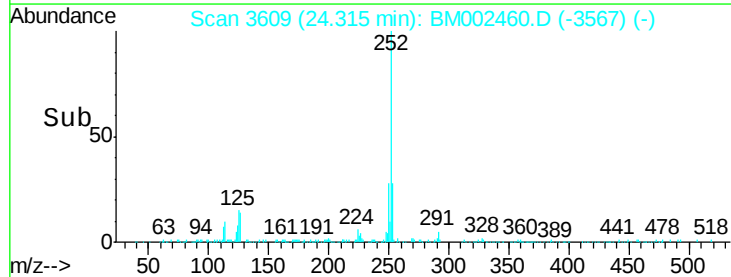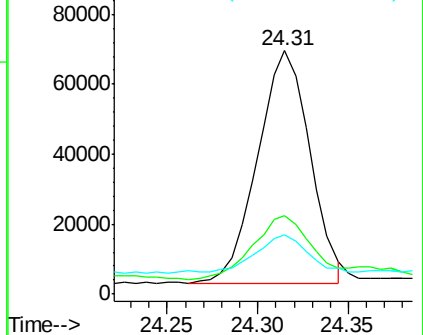

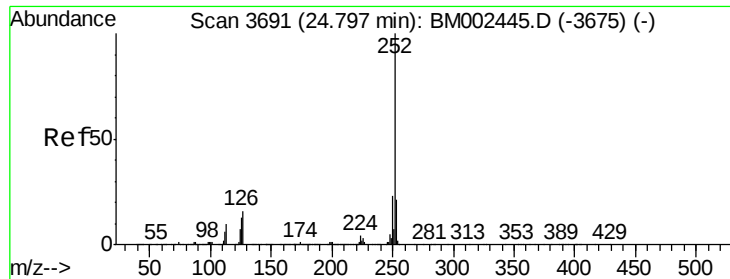

#26

Benzo(a)pyrene

Concen: 29.00 ng/ul

RT: 24.82 min Scan# 3695

Delta R.T. 0.02 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 686758

Ion Ratio Lower Upper




252 100

253 23.7 17.6 26.4

125 15.4 10.7 16.1

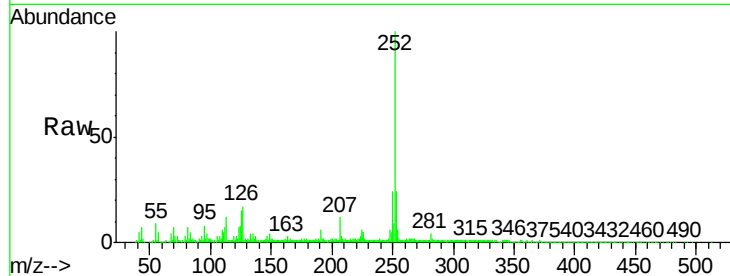

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

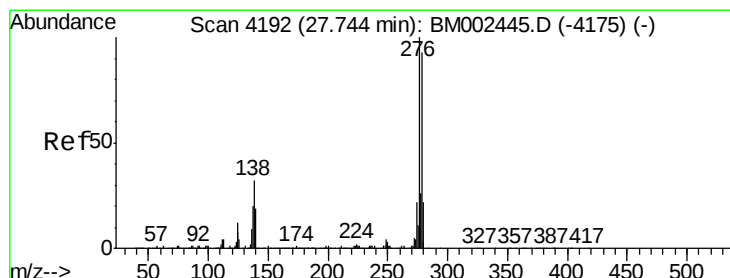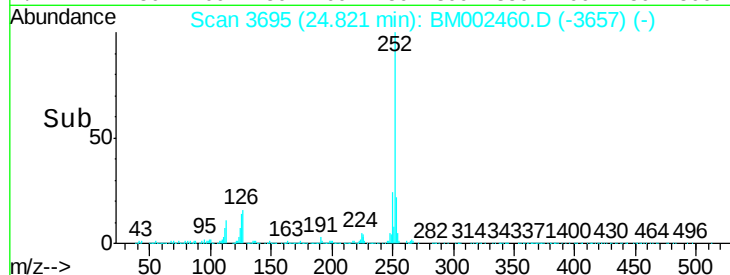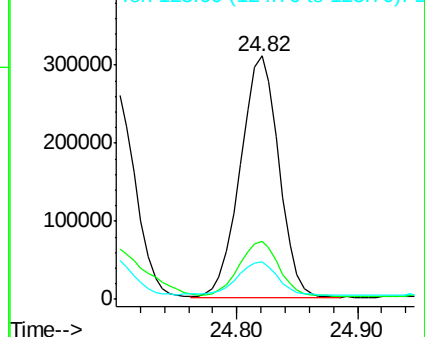

#27

Indeno(1,2,3-cd)pyrene

Concen: 28.12 ng/ul

RT: 27.79 min Scan# 4200

Delta R.T. 0.05 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32


Tgt Ion:276 Resp: 765754

Ion Ratio Lower Upper



276 100


138 26.1 25.3 37.9

277 25.7 20.2 30.2

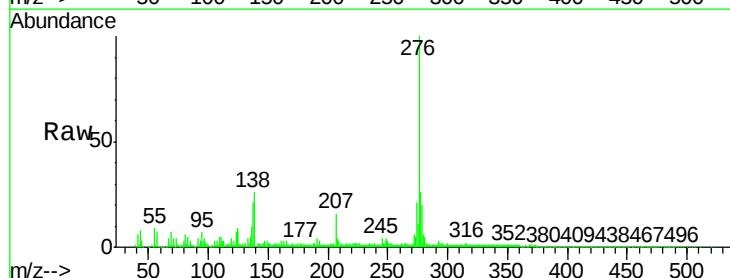

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

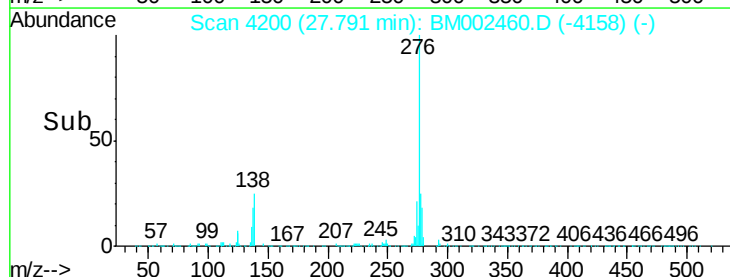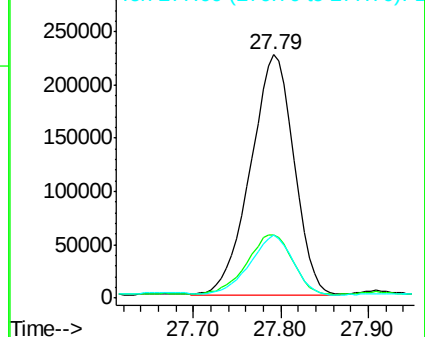

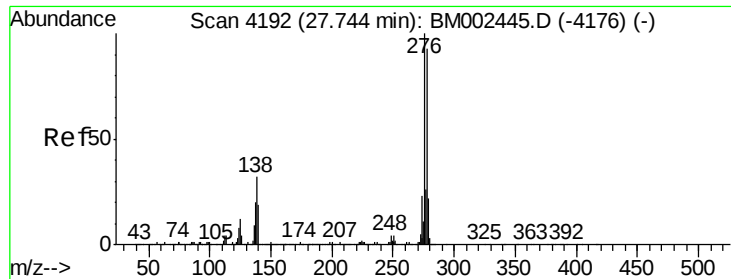

#28

Dibenzo(a,h)anthracene

Concen: 9.04 ng/ul

RT: 27.79 min Scan# 4199

Delta R.T. 0.04 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:278 Resp: 205839

Ion Ratio Lower Upper

278 100

139 30.9 16.5 24.7#




279 28.8 18.8 28.2#

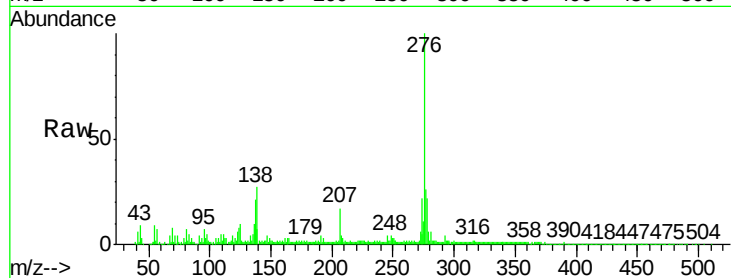

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

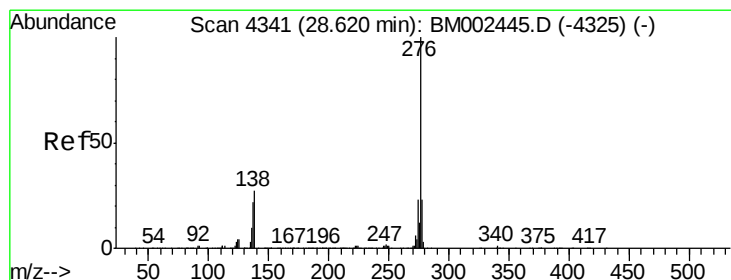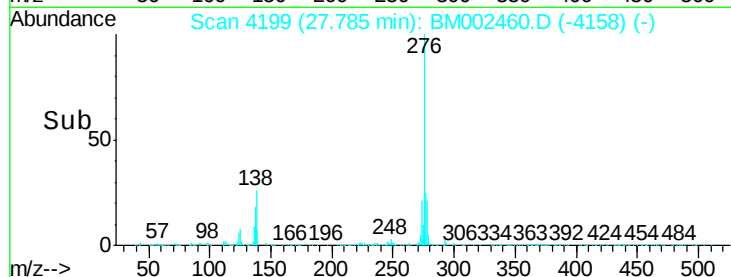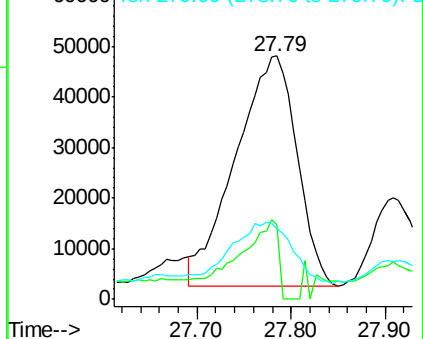

#29

Benzo(g,h,i)perylene

Concen: 32.28 ng/ul

RT: 28.69 min Scan# 4352

Delta R.T. 0.06 min

Lab File: BM002460.D

Acq: 17 Aug 2015 20:32


Tgt Ion:276 Resp: 731826

Ion Ratio Lower Upper

276 100

138 27.8 21.0 31.6

277 24.5 19.2 28.8

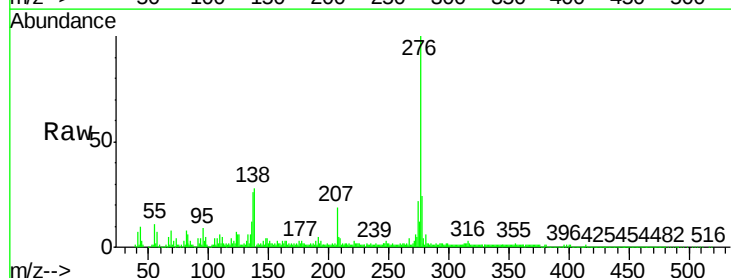

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

